

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034821.D
 Acq On : 02 Nov 2024 01:37
 Operator : RC/JU
 Sample : P4534-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L84

Quant Time: Nov 03 23:29:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	7946	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	24472	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	13716	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	27599	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.166	240	18550	0.400	ng/ul	0.00
23) Perylene-d12	23.211	264	629472	0.400	ng/ul	#-0.15
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	27138	3.299	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	8304	0.271	ng/ul	-0.01
18) Fluoranthene-d10	19.004	212	17903	0.297	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.199	88	248	0.027	ng/ul#	6
20) Pyrene	19.372	202	3254	0.035	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034821.D
Acq On : 02 Nov 2024 01:37
Operator : RC/JU
Sample : P4534-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L84

Quant Time: Nov 03 23:29:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration




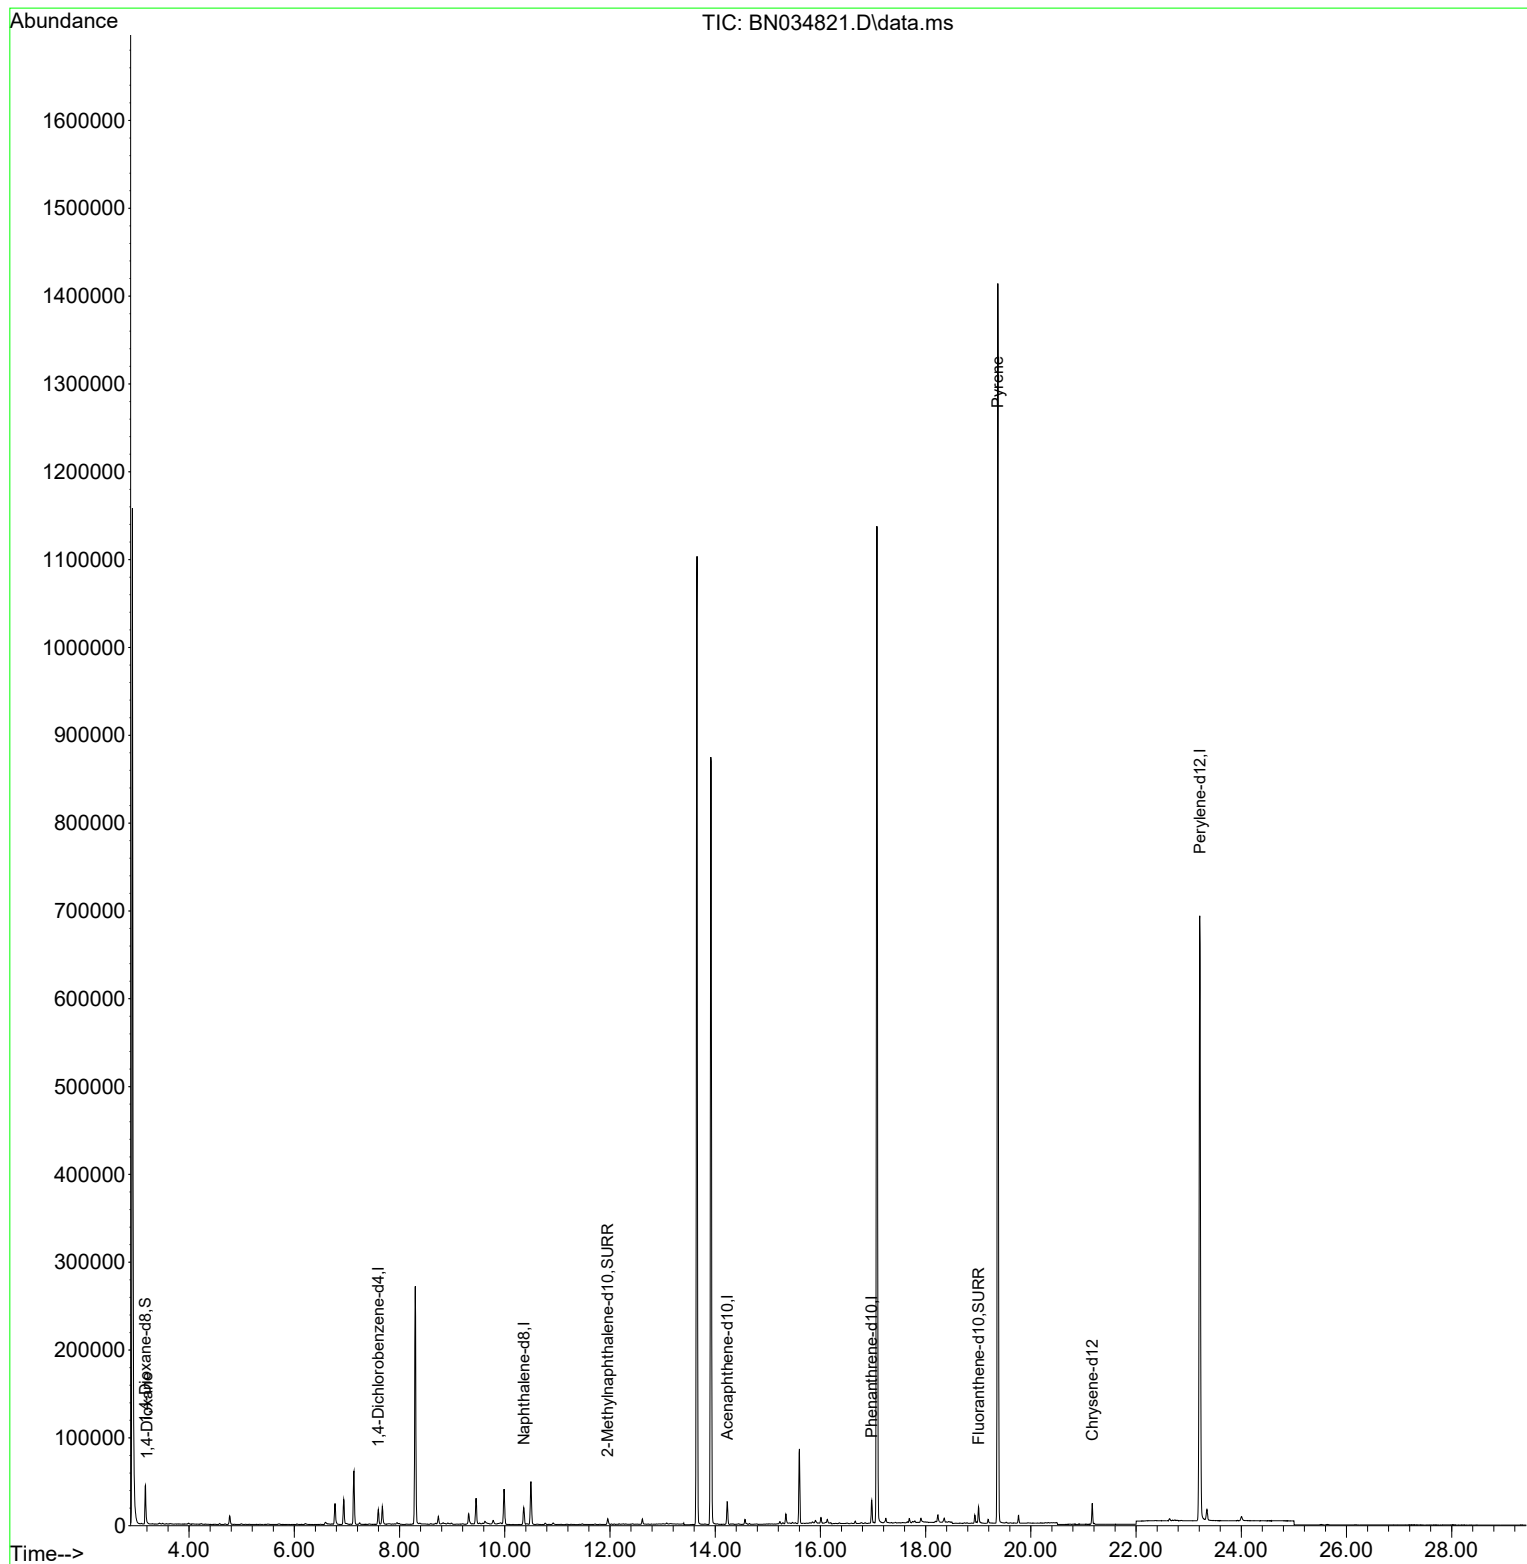


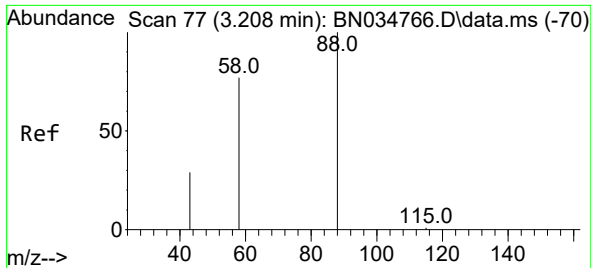

#2
1,4-Dioxane
Concen: 0.027 ng/ul
RT: 3.199 min Scan# 71
Delta R.T. -0.009 min
Lab File: BN034821.D
Acq: 02 Nov 2024 01:37

Instrument :
BNA_N
ClientSampleId :
E1L84

Tgt Ion: 88 Resp: 248
Ion Ratio Lower Upper
88 100
43 172.0 41.9 62.9#
58 39.6 57.5 86.3#

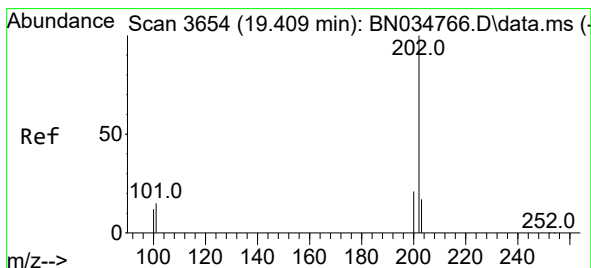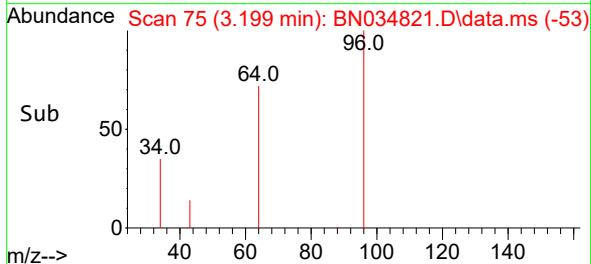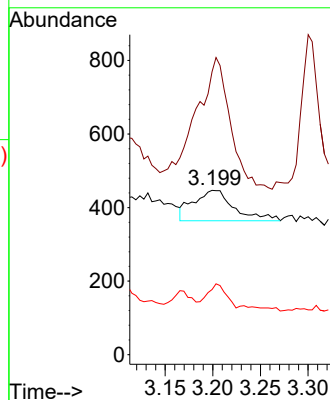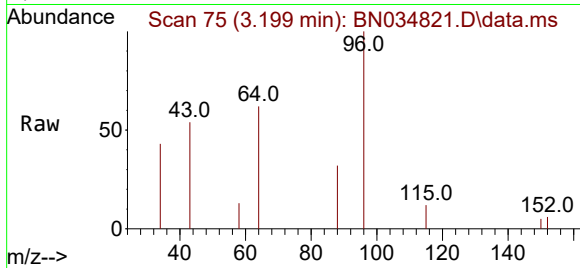

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.372 min Scan# 3646
Delta R.T. -0.037 min
Lab File: BN034821.D
Acq: 02 Nov 2024 01:37

Tgt Ion: 202 Resp: 3254
Ion Ratio Lower Upper
202 100
101 178.4 12.4 18.6#
100 1248.9 10.0 15.0#

