

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034823.D
 Acq On : 02 Nov 2024 02:49
 Operator : RC/JU
 Sample : P4534-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L88

Quant Time: Nov 03 23:29:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	7401	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	22316	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.226	164	12088	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.166	240	18832	0.400	ng/ul	0.00
23) Perylene-d12	23.212	264	778349	0.400	ng/ul	#-0.15
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	28276	3.691	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	7594	0.271	ng/ul	-0.01
18) Fluoranthene-d10	19.005	212	18199	0.297	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.372	202	2784	0.029	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034823.D
Acq On : 02 Nov 2024 02:49
Operator : RC/JU
Sample : P4534-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L88

Quant Time: Nov 03 23:29:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

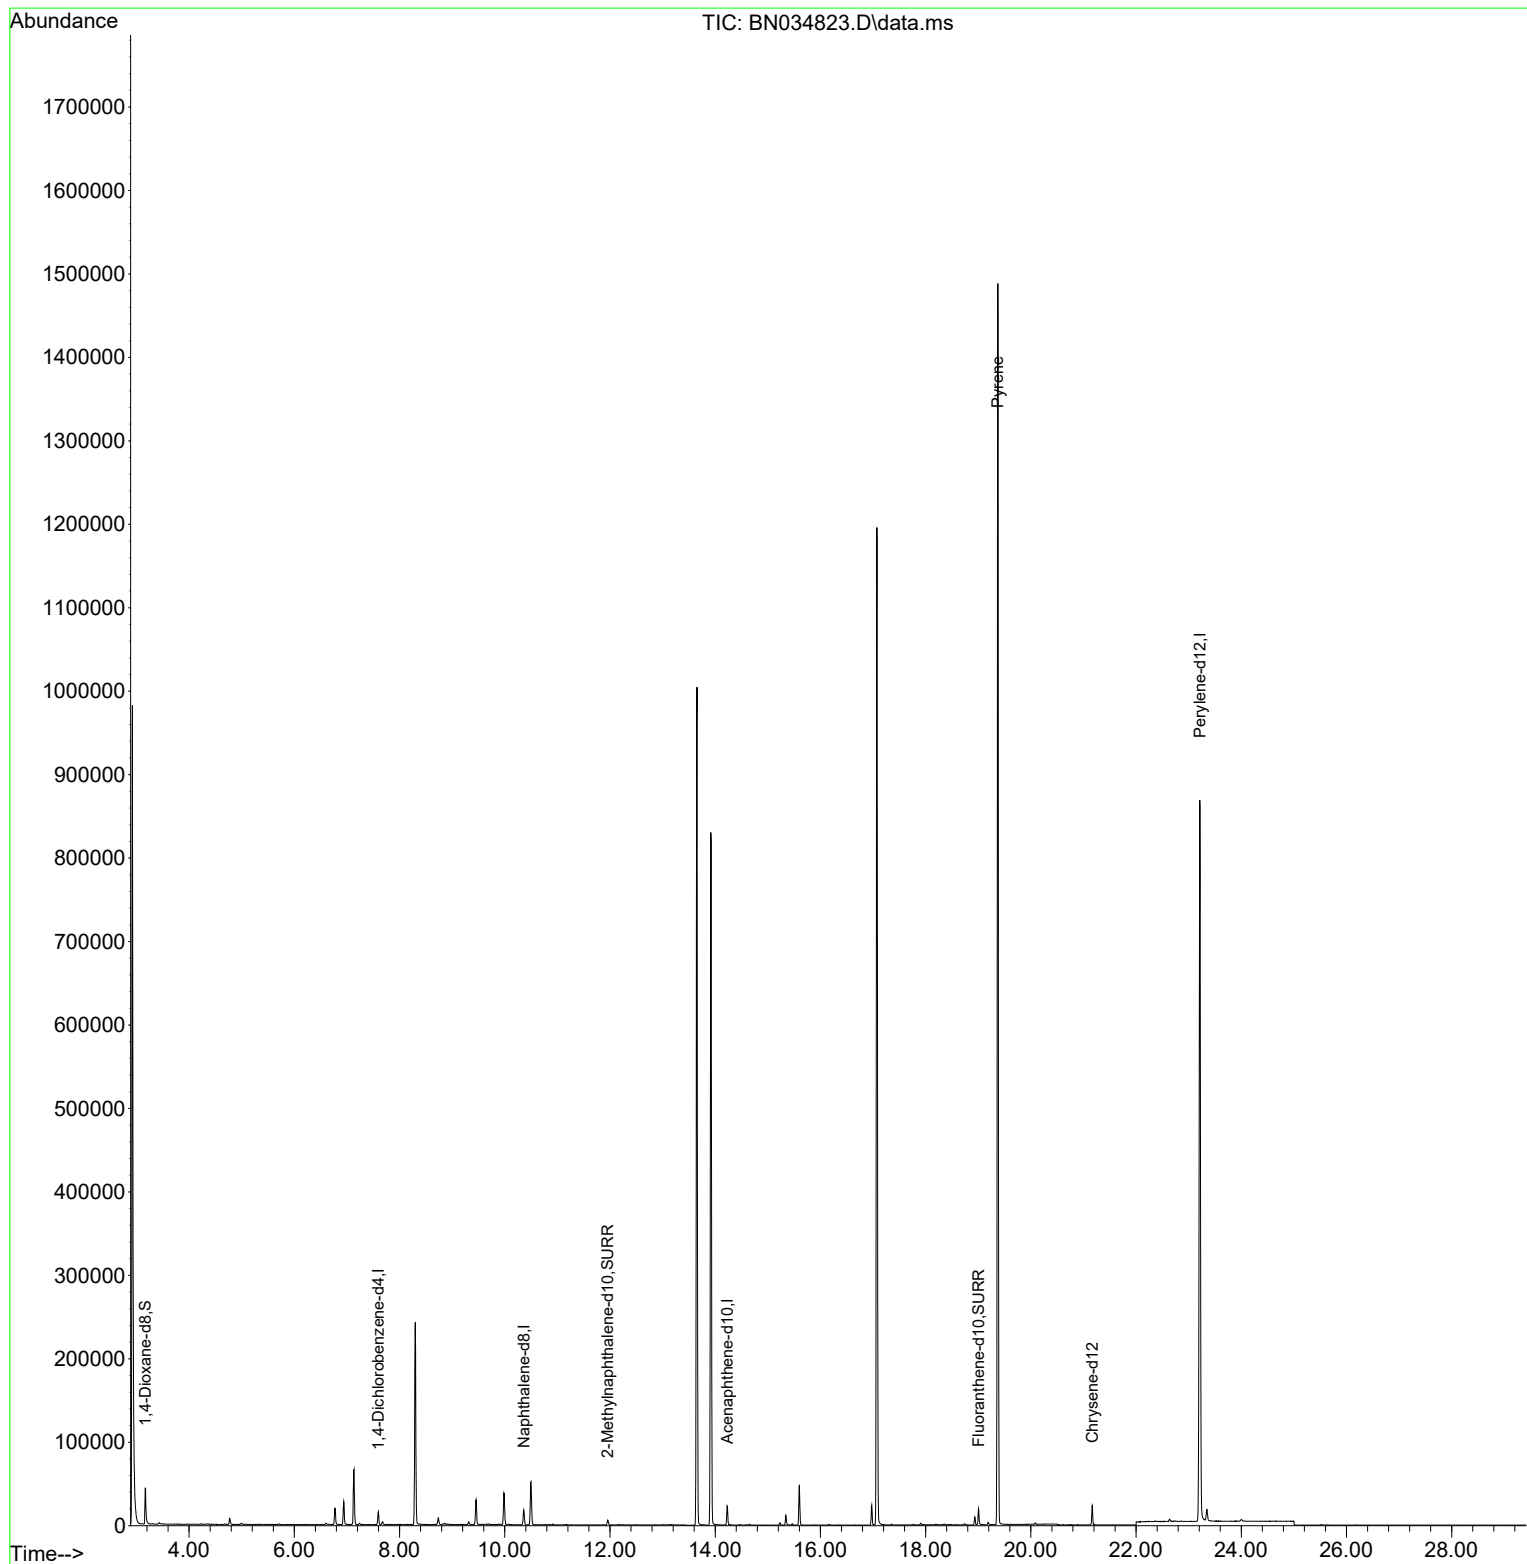

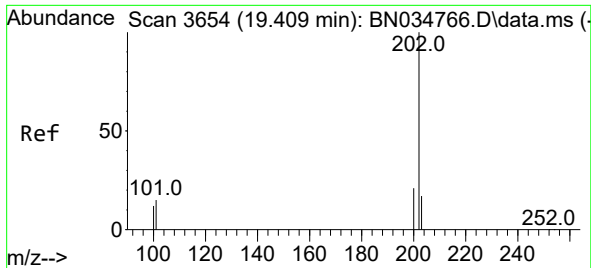

#20
 Pyrene
 Concen: 0.029 ng/ul
 RT: 19.372 min Scan# 30
 Delta R.T. -0.037 min
 Lab File: BN034823.D
 Acq: 02 Nov 2024 02:49

Instrument :
 BNA_N
 ClientSampleId :
 E1L88

Tgt Ion:202 Resp: 2784
 Ion Ratio Lower Upper
 202 100
 101 198.0 12.4 18.6#
 100 1422.4 10.0 15.0#

