

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034831.D
 Acq On : 02 Nov 2024 07:38
 Operator : RC/JU
 Sample : PB164515BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK515

Quant Time: Nov 03 23:30:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	6914	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	21600	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.226	164	12051	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.98
17) Chrysene-d12	21.166	240	15225	0.400	ng/ul	0.00
23) Perylene-d12	23.211	264	882882	0.400	ng/ul	#-0.15
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.165	96	47357	6.617	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	10769	0.398	ng/ul	-0.01
18) Fluoranthene-d10	19.004	212	20639	0.417	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.230	166	3108	0.066	ng/ul#	13
20) Pyrene	19.372	202	2671	0.035	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034831.D
Acq On : 02 Nov 2024 07:38
Operator : RC/JU
Sample : PB164515BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK515

Quant Time: Nov 03 23:30:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration




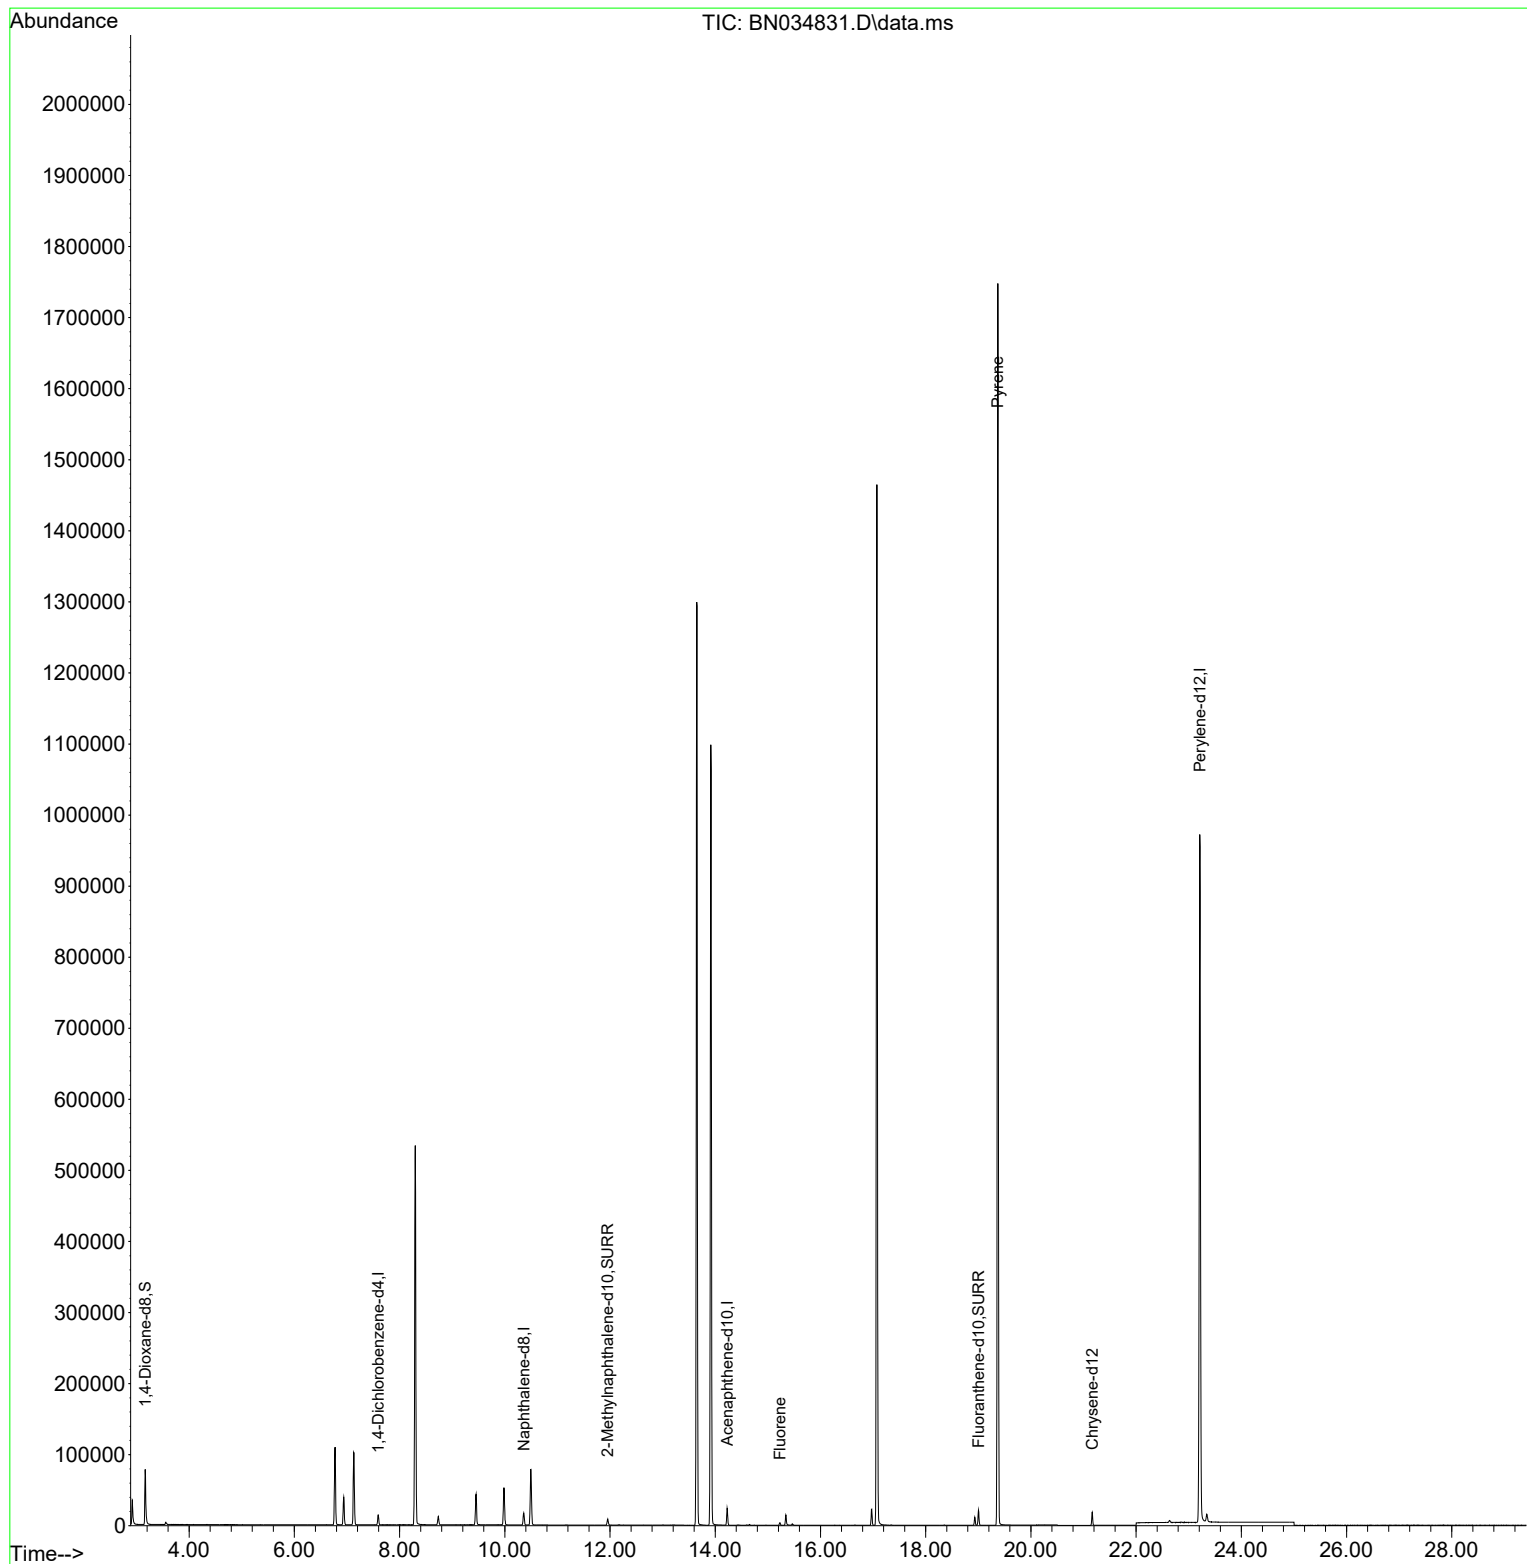


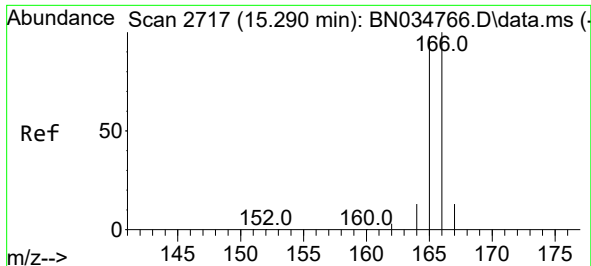

#12
Fluorene
Concen: 0.066 ng/ul
RT: 15.230 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN034831.D
Acq: 02 Nov 2024 07:38

Instrument :
BNA_N
ClientSampleId :
SBLK515

Tgt Ion:166 Resp: 3108
Ion Ratio Lower Upper
166 100
165 7.9 79.1 118.7#
167 35.8 11.0 16.4#

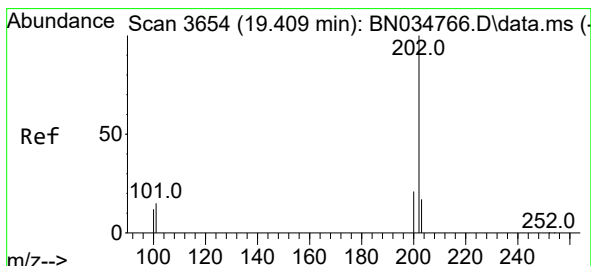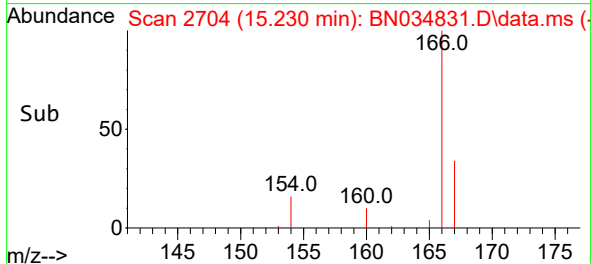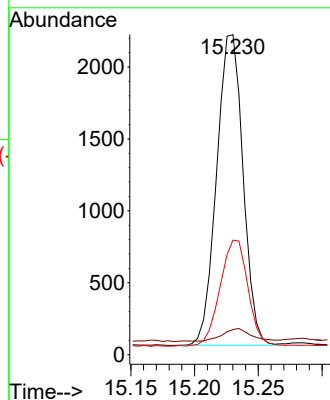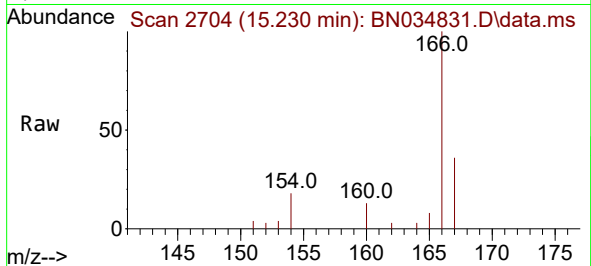

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.372 min Scan# 3646
Delta R.T. -0.037 min
Lab File: BN034831.D
Acq: 02 Nov 2024 07:38

Tgt Ion:202 Resp: 2671
Ion Ratio Lower Upper
202 100
101 200.7 12.4 18.6#
100 1492.5 10.0 15.0#

