




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034767.D
Acq On : 31 Oct 2024 15:52
Operator : RC/JU
Sample : PB164418BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:09:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

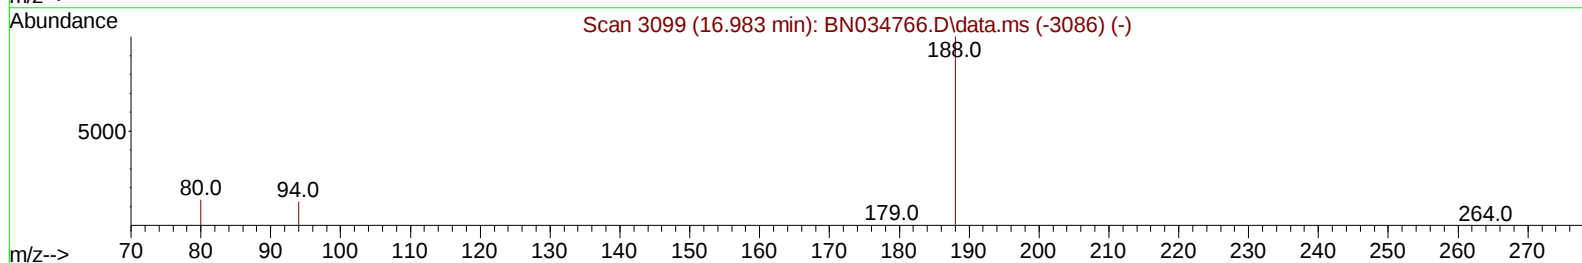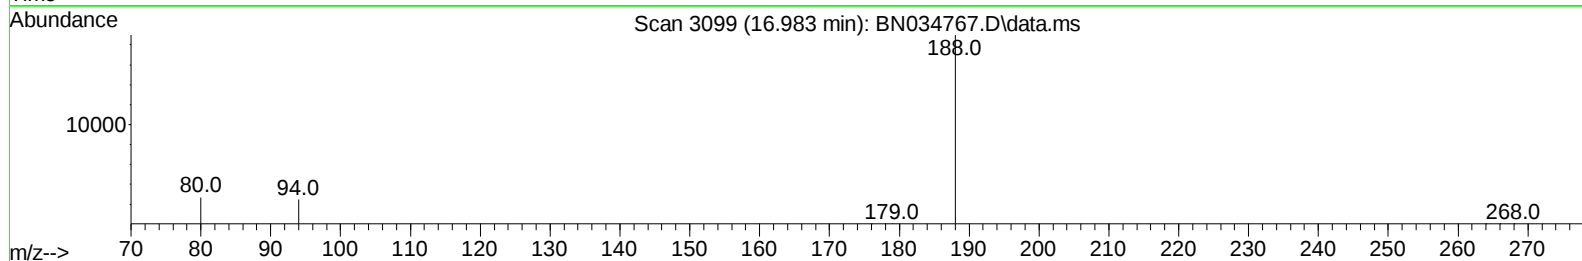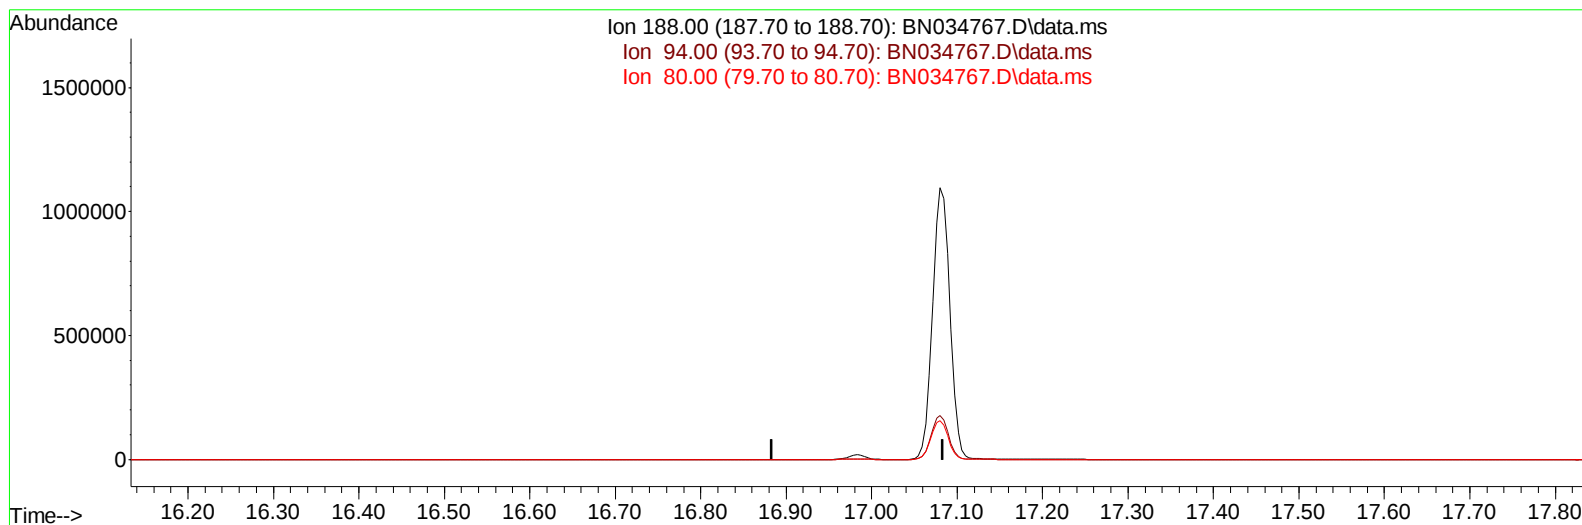

TIC: BN034767.D\data.ms

(13) Phenanthrene-d10 (I)

16.983min (-16.983) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.60	0.00#
80.00	14.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034767.D
Acq On : 31 Oct 2024 15:52
Operator : RC/JU
Sample : PB164418BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:09:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

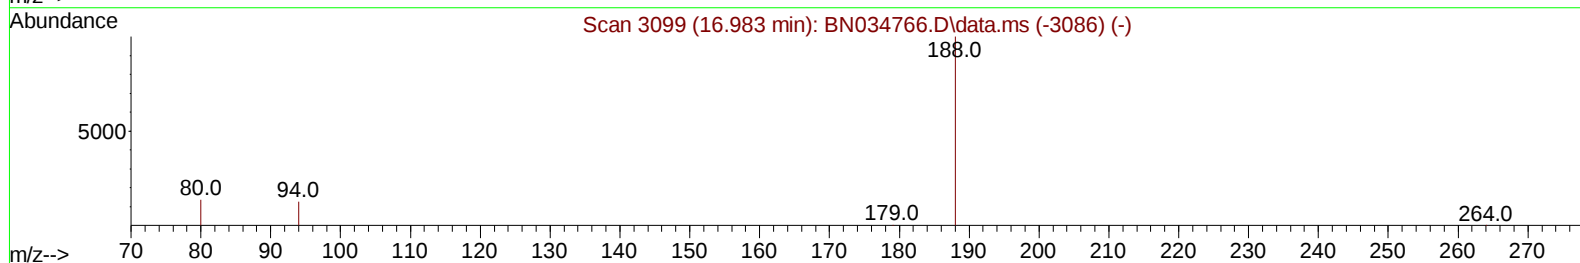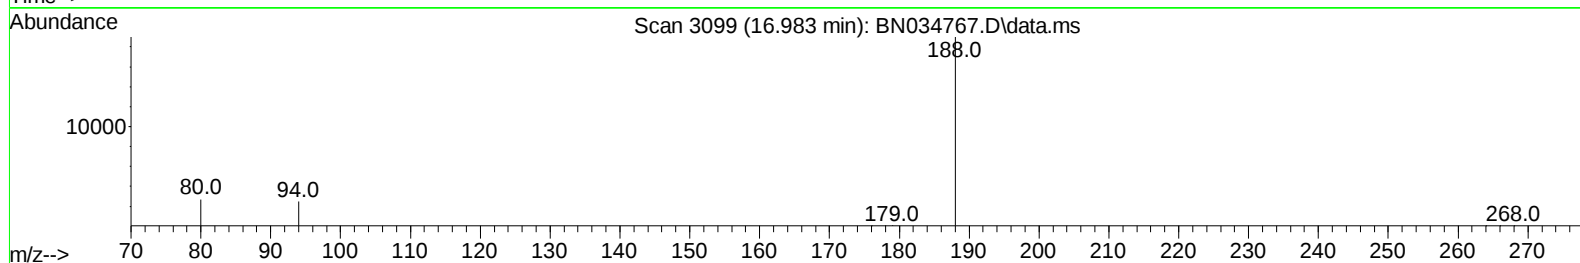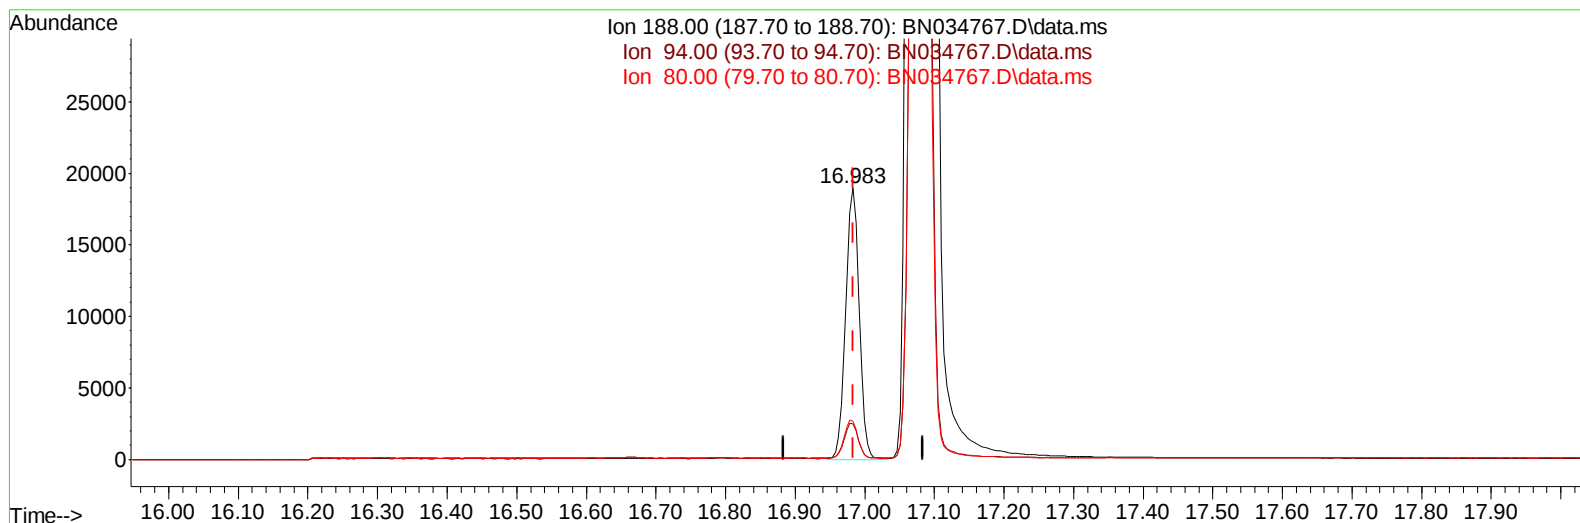

TIC: BN034767.D\data.ms

(13) Phenanthrene-d10 (I)

16.983min (-0.000) 0.40 ng/ul m

response 25752

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.60	13.09
80.00	14.50	14.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034767.D
Acq On : 31 Oct 2024 15:52
Operator : RC/JU
Sample : PB164418BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

Quant Time: Oct 31 18:09:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

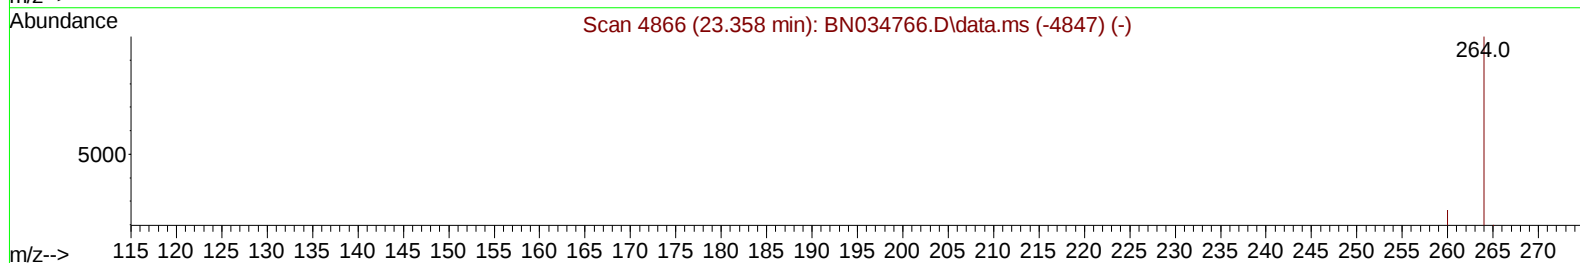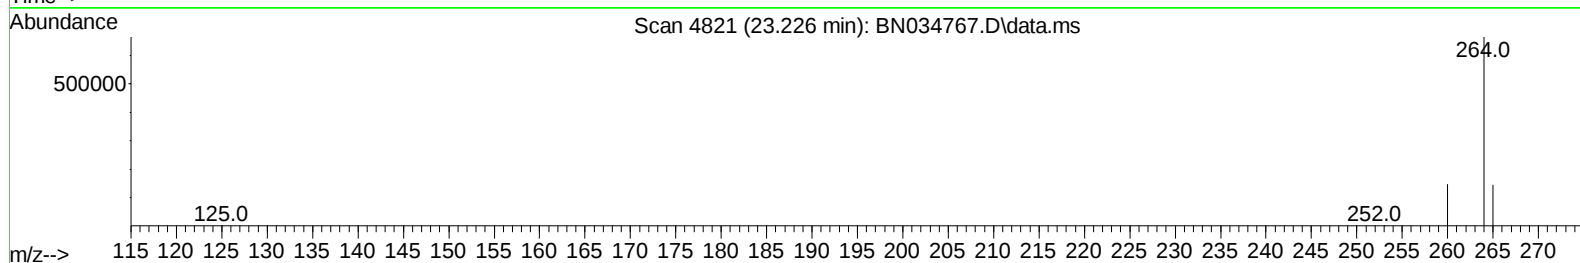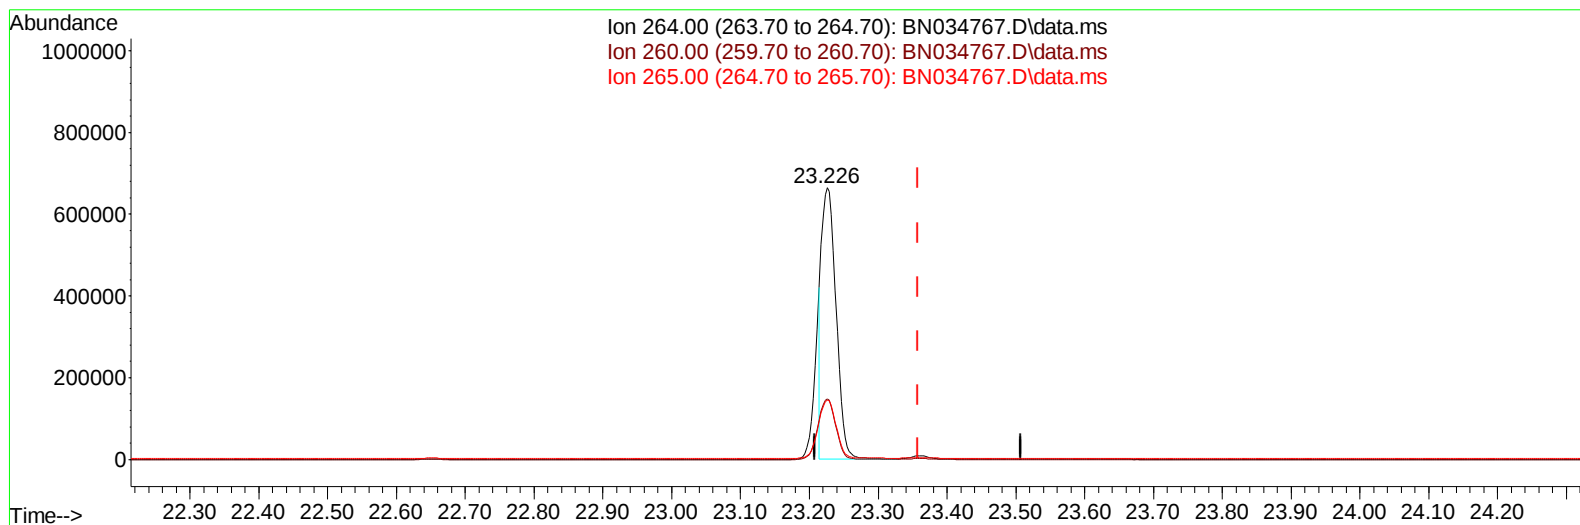

TIC: BN034767.D\data.ms

(23) Perylene-d12 (I)

23.226min (-0.132) 0.40 ng/u1

response 967400

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	22.25
265.00	57.90	21.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034767.D
Acq On : 31 Oct 2024 15:52
Operator : RC/JU
Sample : PB164418BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:09:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

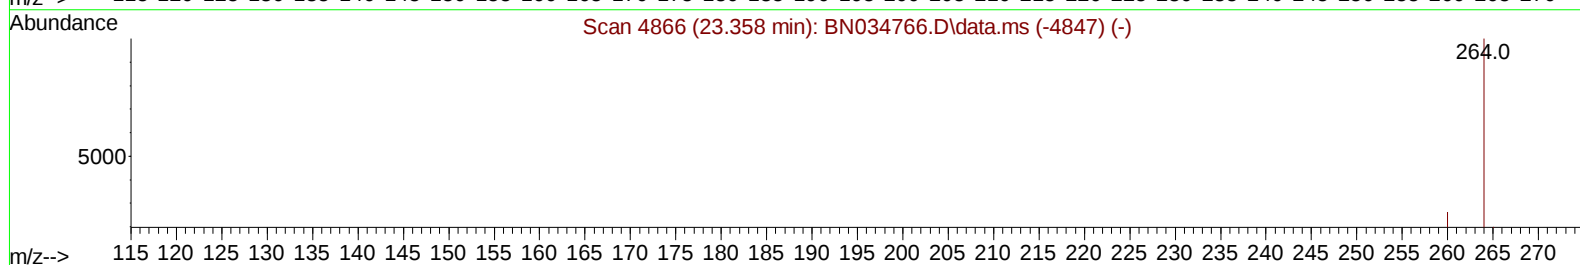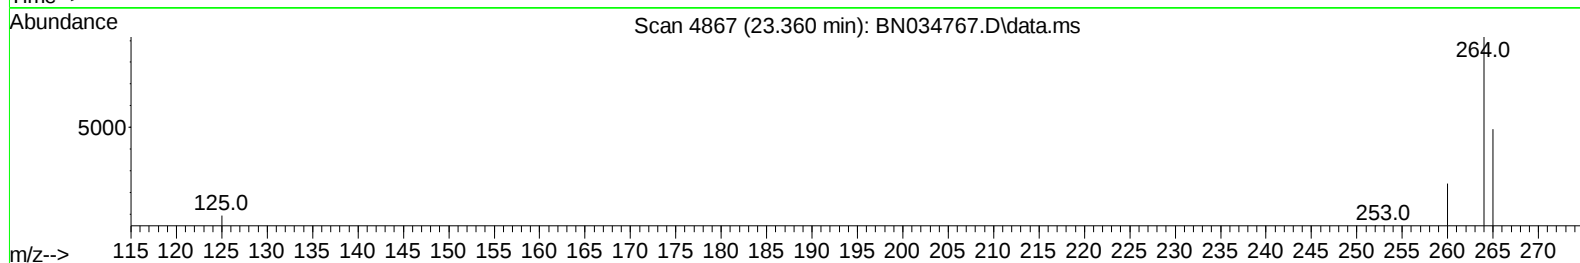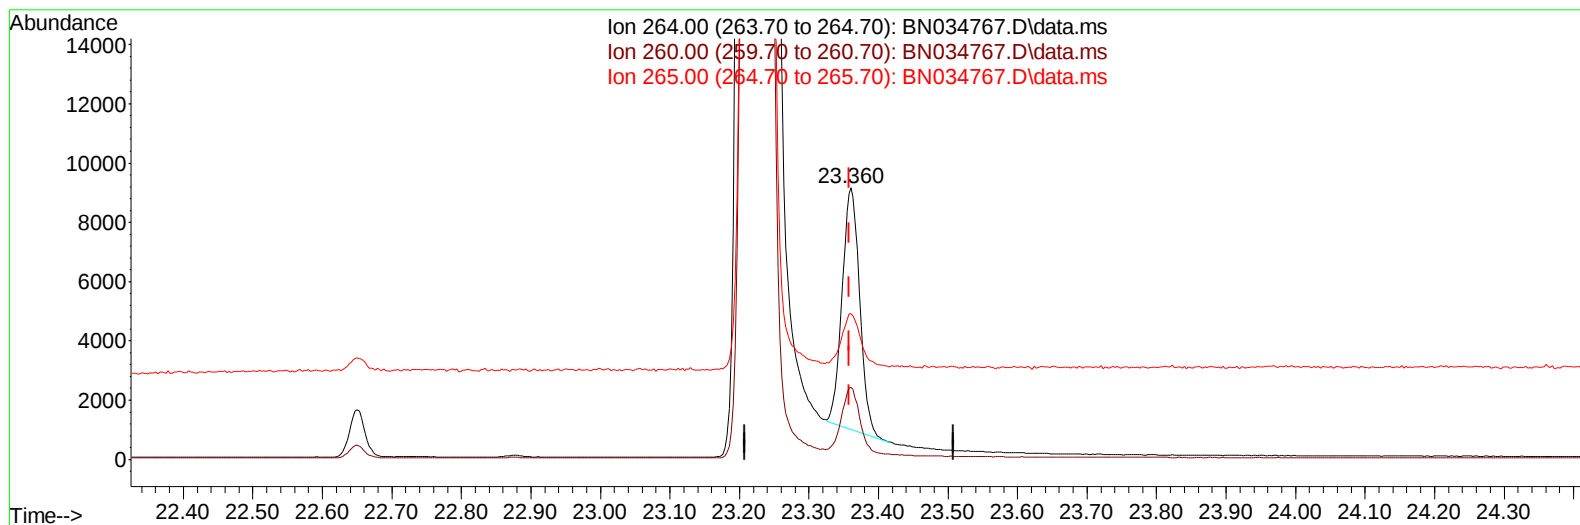

TIC: BN034767.D\data.ms

(23) Perylene-d12 (I)

23.360min (+ 0.003) 0.40 ng/ul m

response 14333

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	26.50
265.00	57.90	53.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034767.D
 Acq On : 31 Oct 2024 15:52
 Operator : RC/JU
 Sample : PB164418BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK418

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Oct 31 18:09:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.604	152	7566	0.400	ng/ul	0.00
4) Naphthalene-d8	10.372	136	23269	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.235	164	12797	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.983	188	25752m	0.400	ng/ul	0.00
17) Chrysene-d12	21.174	240	16659	0.400	ng/ul	0.00
23) Perylene-d12	23.360	264	14333m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	47291	6.038	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.967	152	10215	0.350	ng/ul	0.00
18) Fluoranthene-d10	19.014	212	19272	0.355	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034767.D
Acq On : 31 Oct 2024 15:52
Operator : RC/JU
Sample : PB164418BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK418

Manual IntegrationsAPPROVED

Quant Time: Oct 31 18:09:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

