




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034790.D
Acq On : 01 Nov 2024 06:19
Operator : RC/JU
Sample : P4529-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H22

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

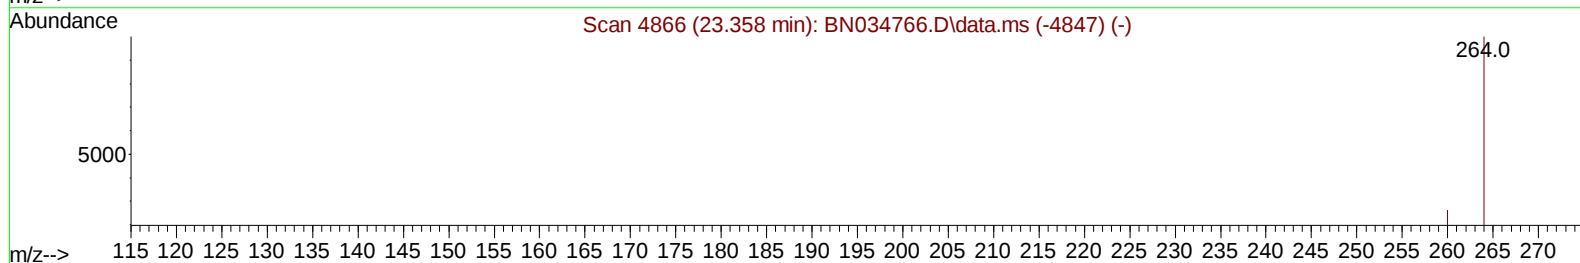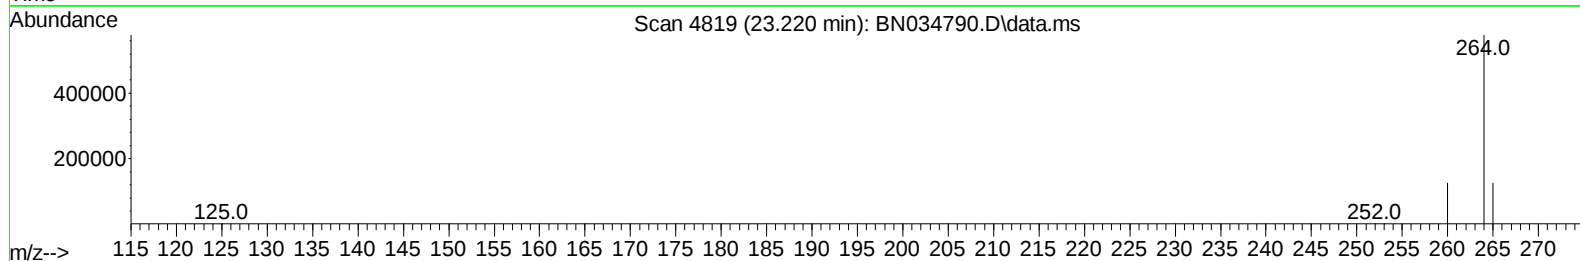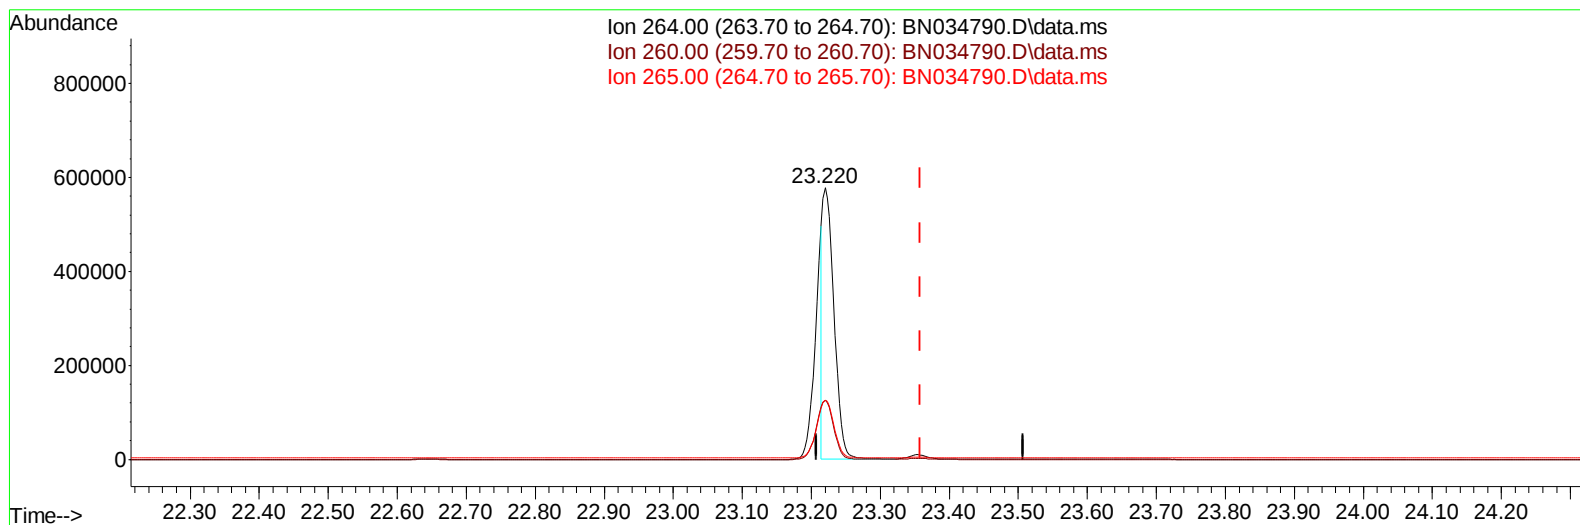

TIC: BN034790.D\data.ms

(23) Perylene-d12 (I)

23.220min (-0.138) 0.40 ng/u1

response 658698

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	21.79#
265.00	57.90	21.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034790.D
Acq On : 01 Nov 2024 06:19
Operator : RC/JU
Sample : P4529-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H22

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

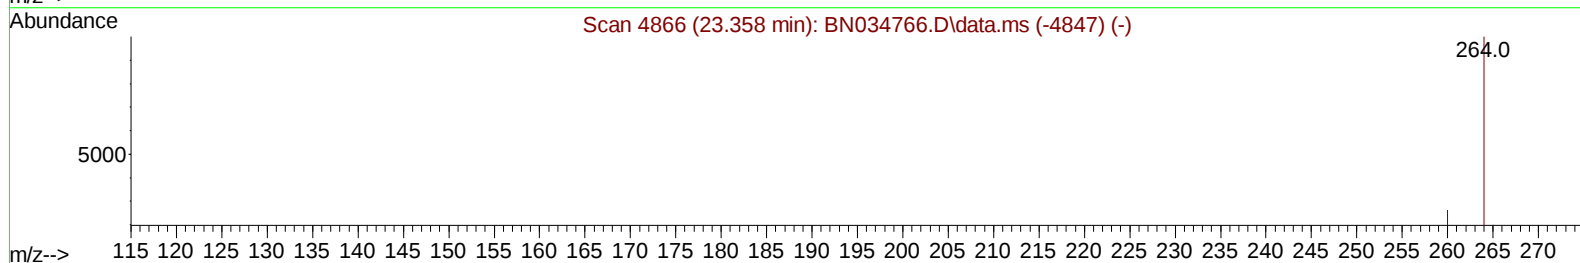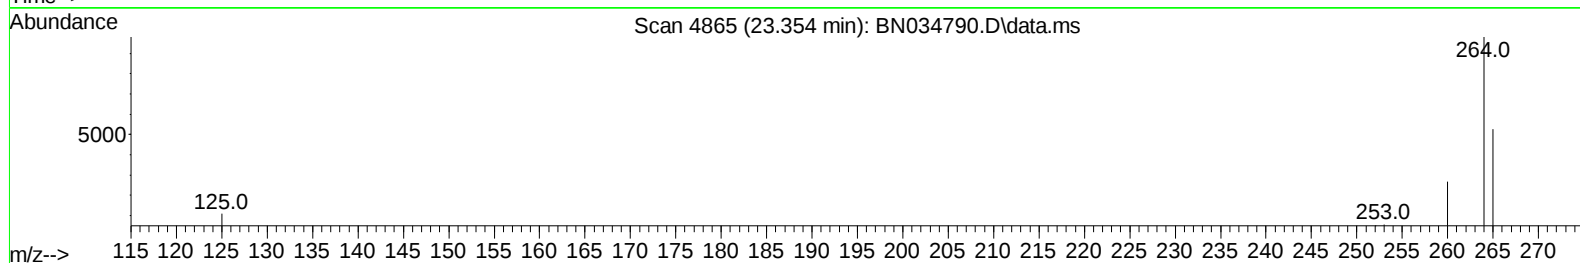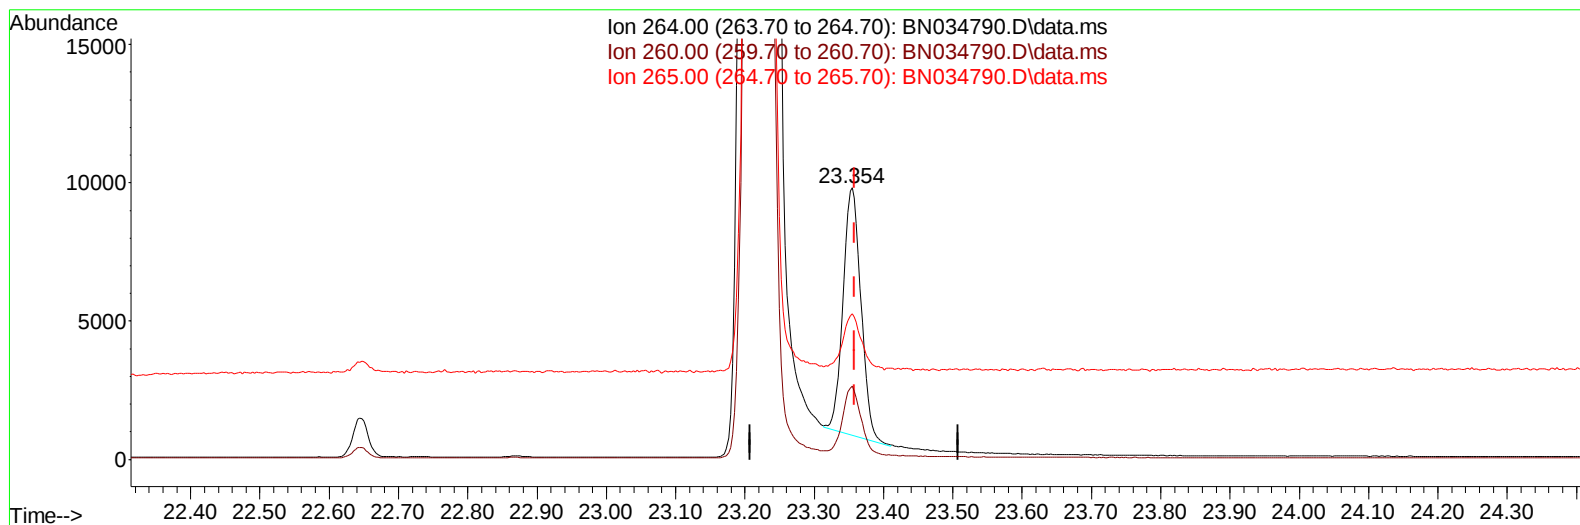

TIC: BN034790.D\data.ms

(23) Perylene-d12 (I)

23.354min (-0.003) 0.40 ng/ul m

response 16034

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	27.09
265.00	57.90	53.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034790.D
 Acq On : 01 Nov 2024 06:19
 Operator : RC/JU
 Sample : P4529-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H22

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:25:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	7847	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136	25146	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.235	164	14390	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.979	188	29038	0.400	ng/ul	0.00
17) Chrysene-d12	21.174	240	20095	0.400	ng/ul	0.00
23) Perylene-d12	23.354	264	16034m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	33029	4.066	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	8635	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	17848	0.273	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034790.D
Acq On : 01 Nov 2024 06:19
Operator : RC/JU
Sample : P4529-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H22

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

