




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

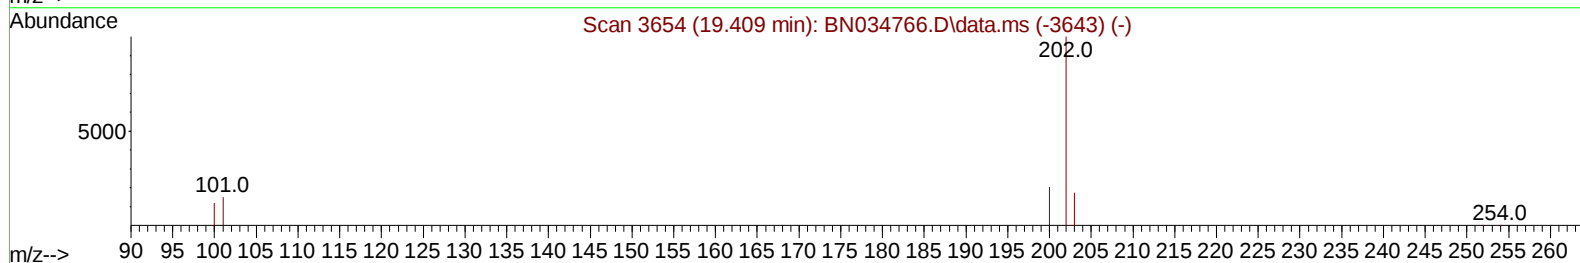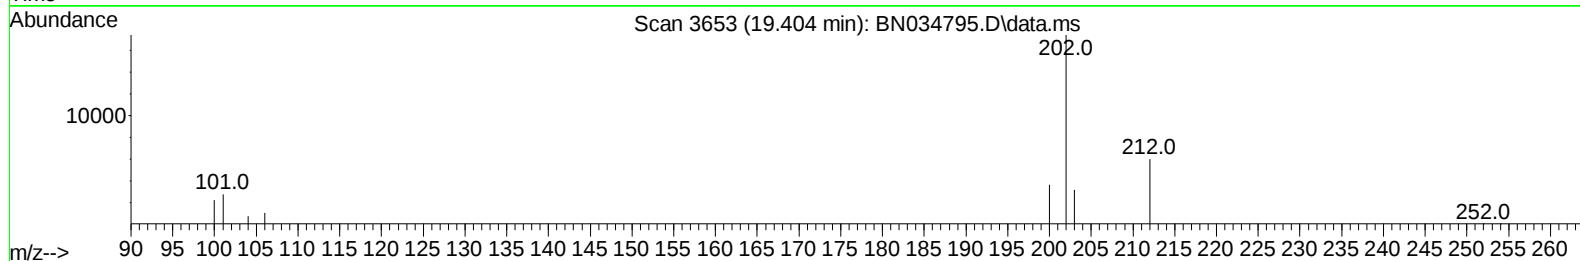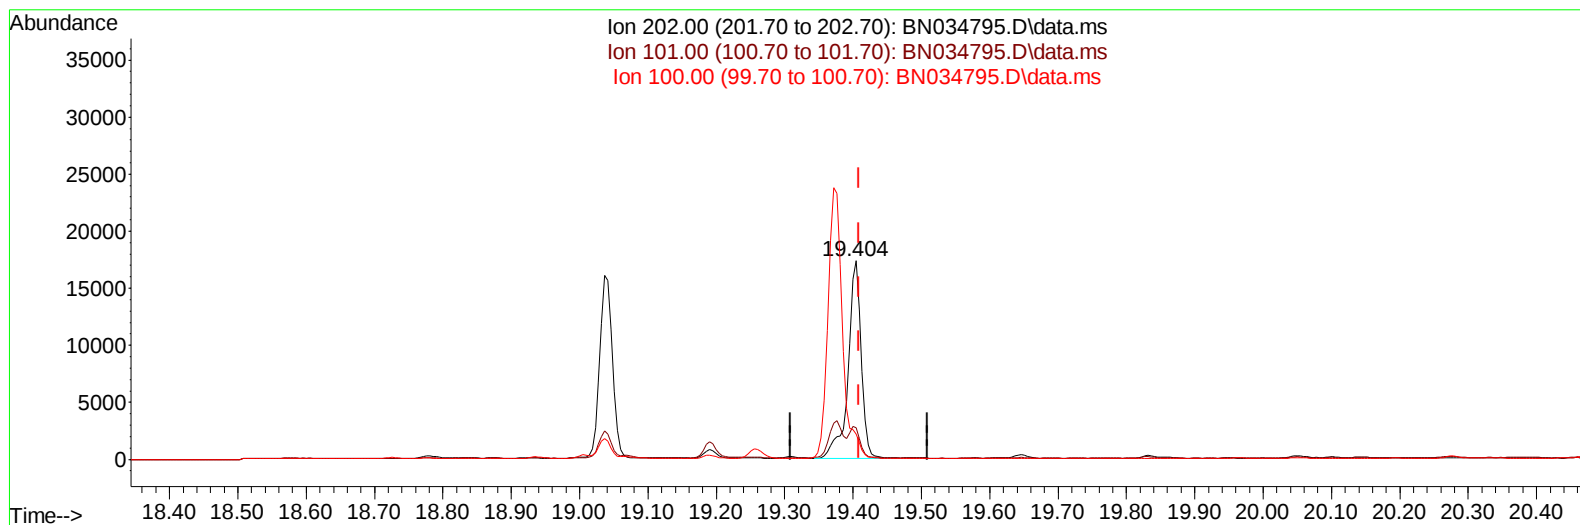

TIC: BN034795.D\data.ms

(20) Pyrene

19.404min (-0.005) 0.21 ng/u1

response 23470

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.50	16.04
100.00	12.50	12.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

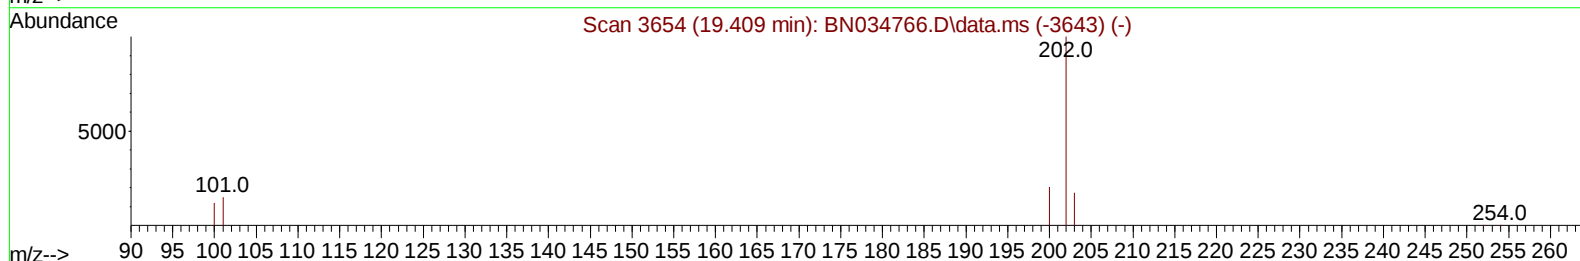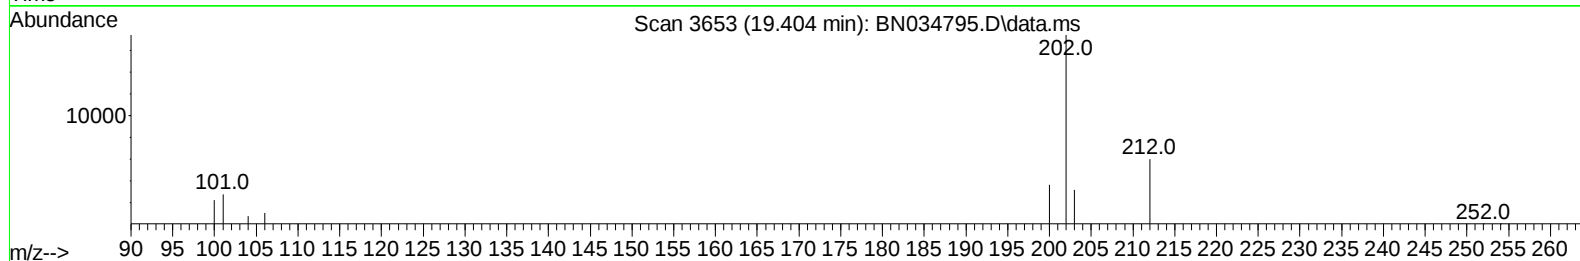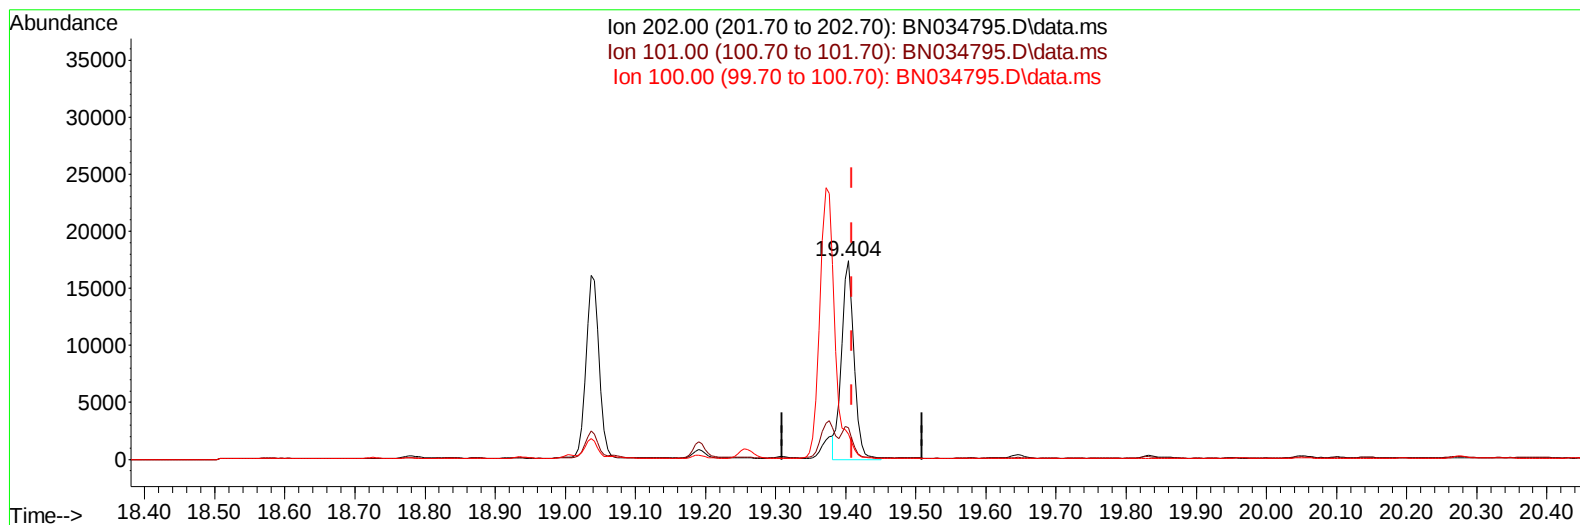

TIC: BN034795.D\data.ms

(20) Pyrene

19.404min (-0.005) 0.20 ng/ul m

response 21787

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.50	16.04
100.00	12.50	12.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

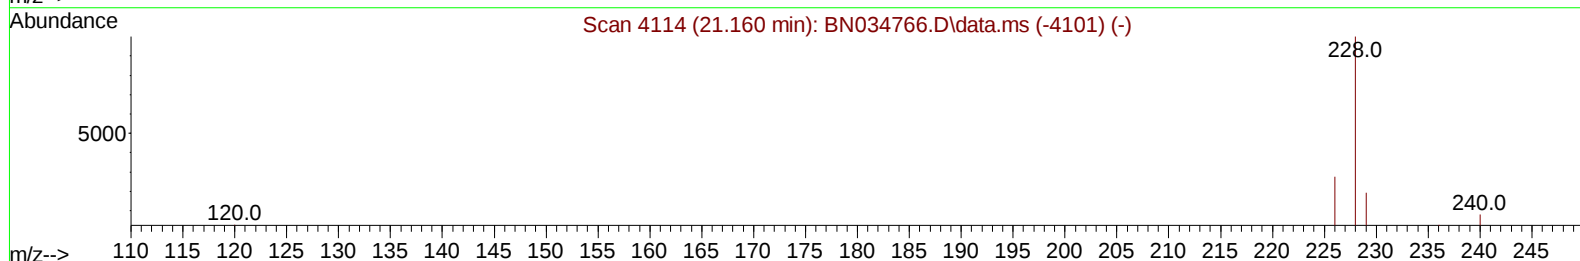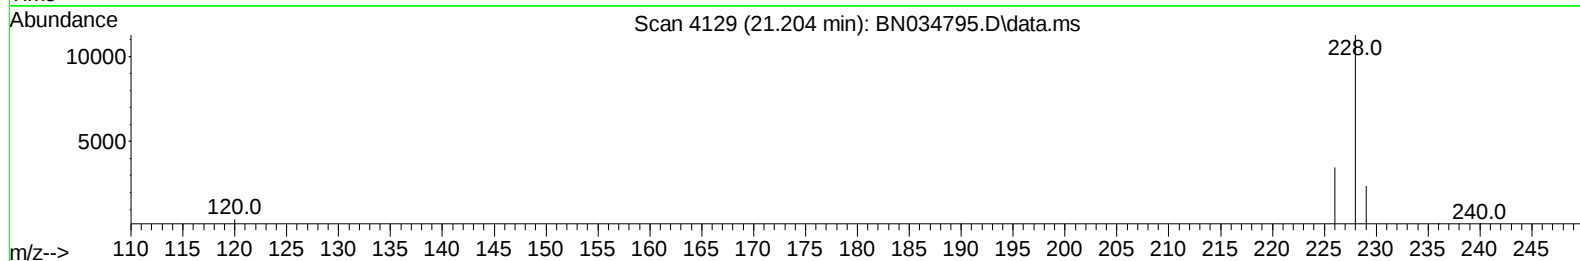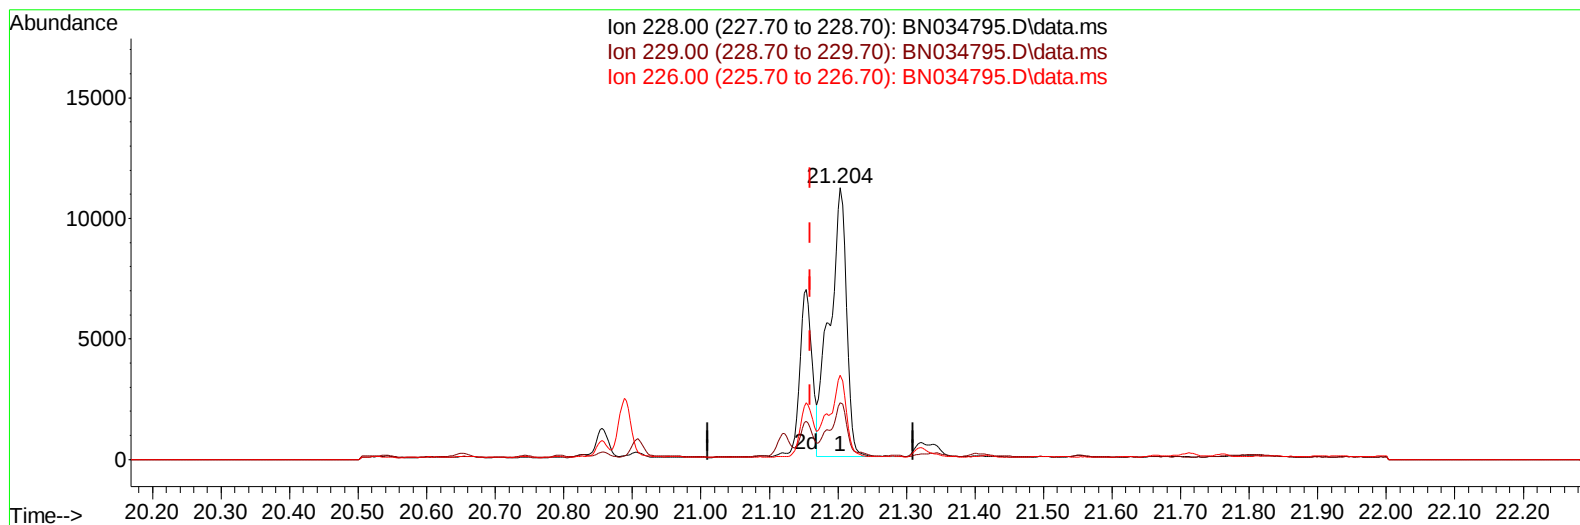

TIC: BN034795.D\data.ms

(21) Benzo(a)anthracene

21.204min (+ 0.044) 0.22 ng/u1

response 19051

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.40	20.99
226.00	27.60	30.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

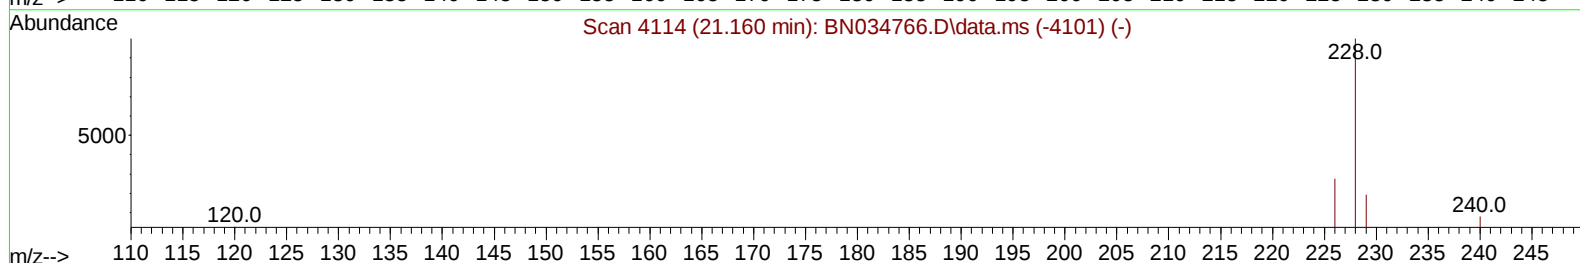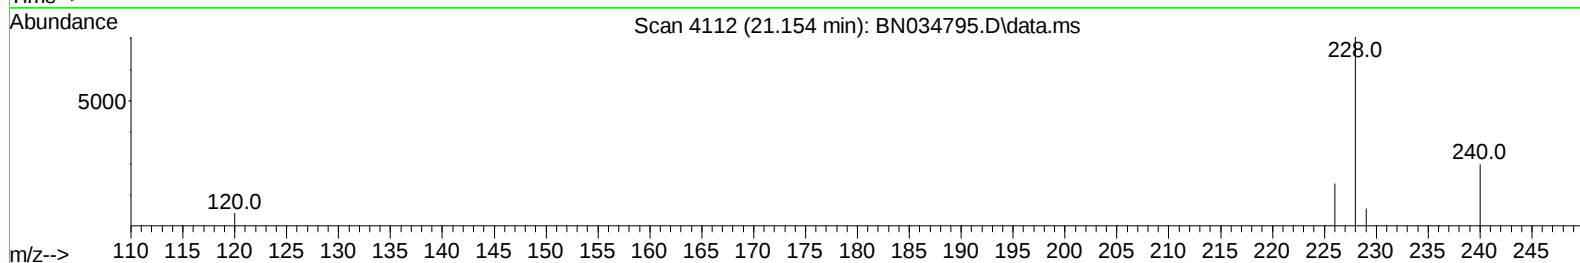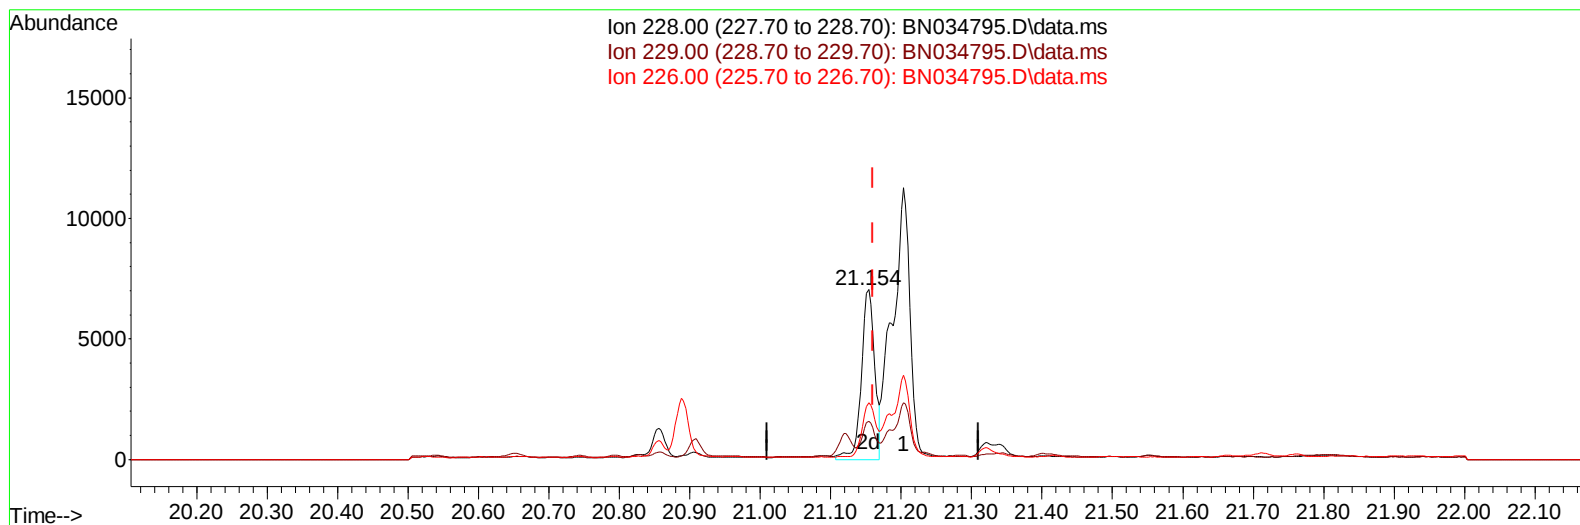

TIC: BN034795.D\data.ms

(21) Benzo(a)anthracene

21.154min (-0.006) 0.11 ng/u1 m

response 9189

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.40	22.28
226.00	27.60	33.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

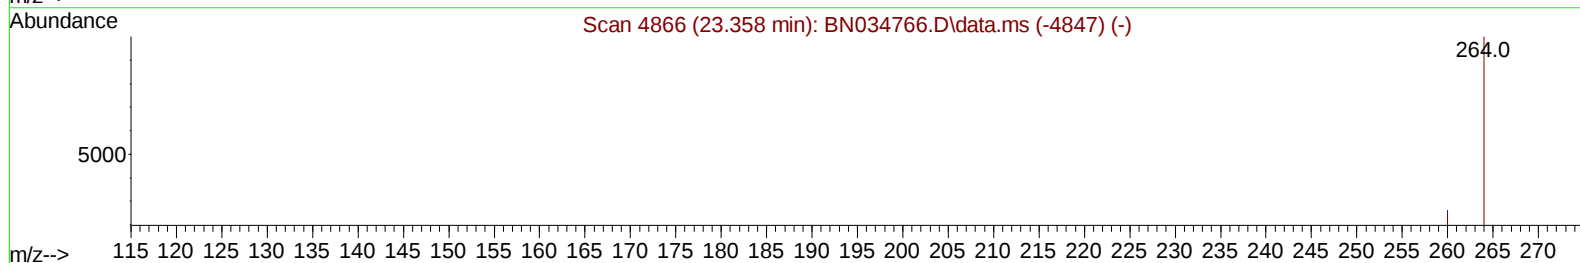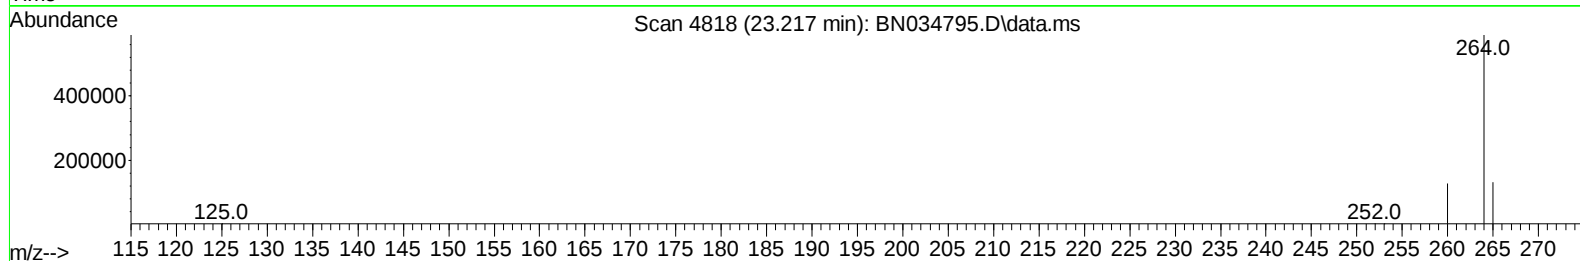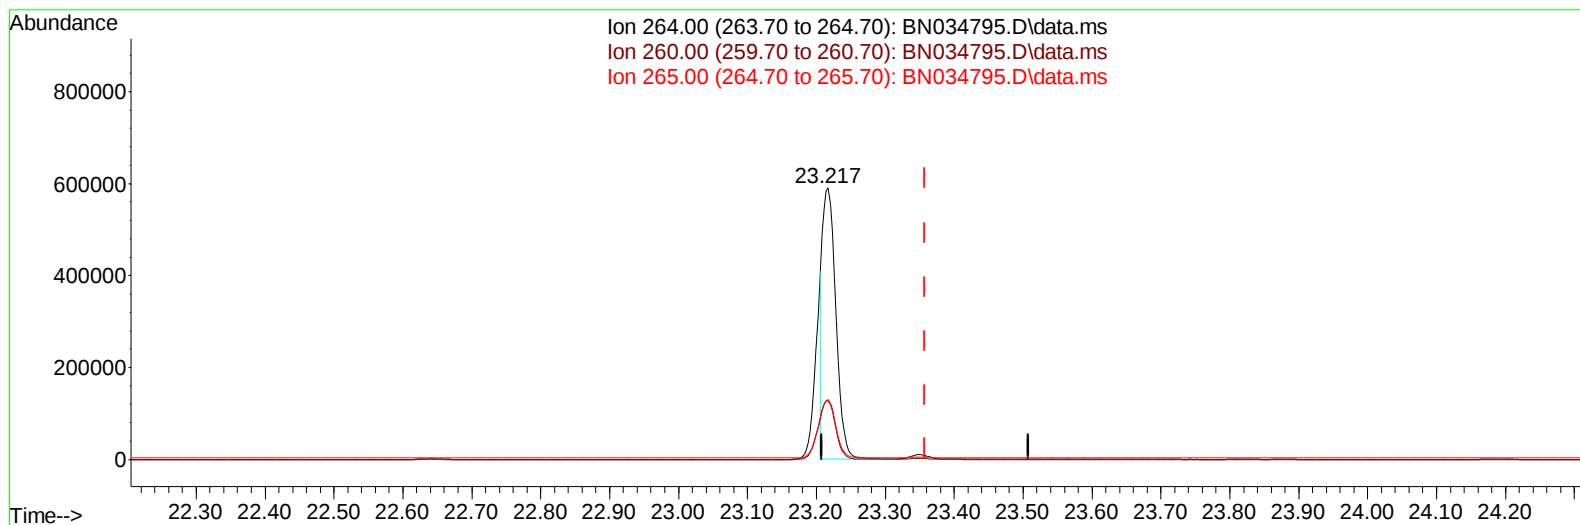

TIC: BN034795.D\data.ms

(23) Perylene-d12 (I)

23.217min (-0.141) 0.40 ng/u1

response 799668

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	21.66#
265.00	57.90	22.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

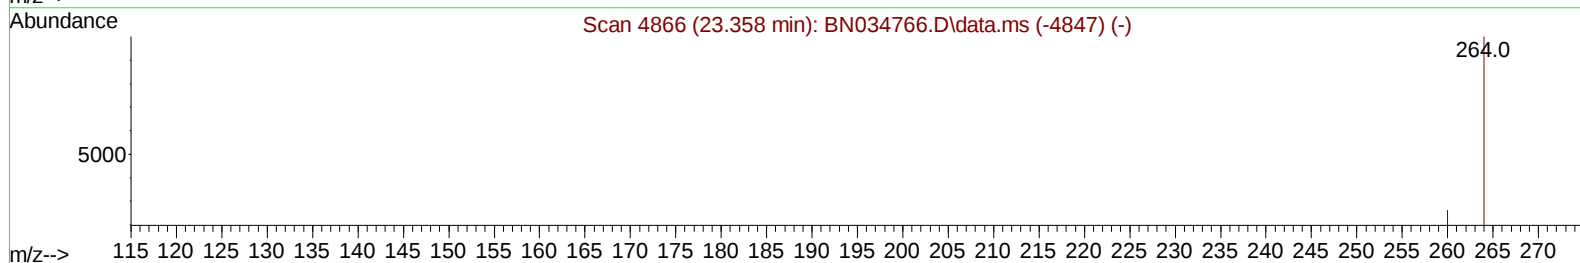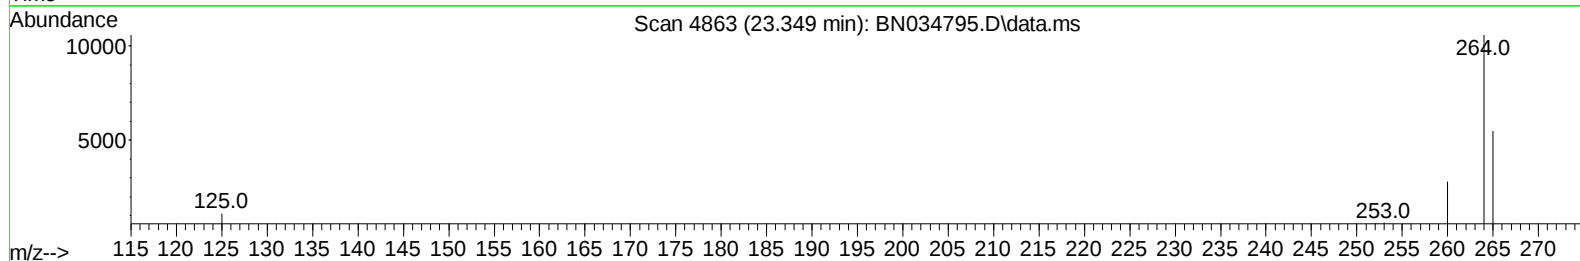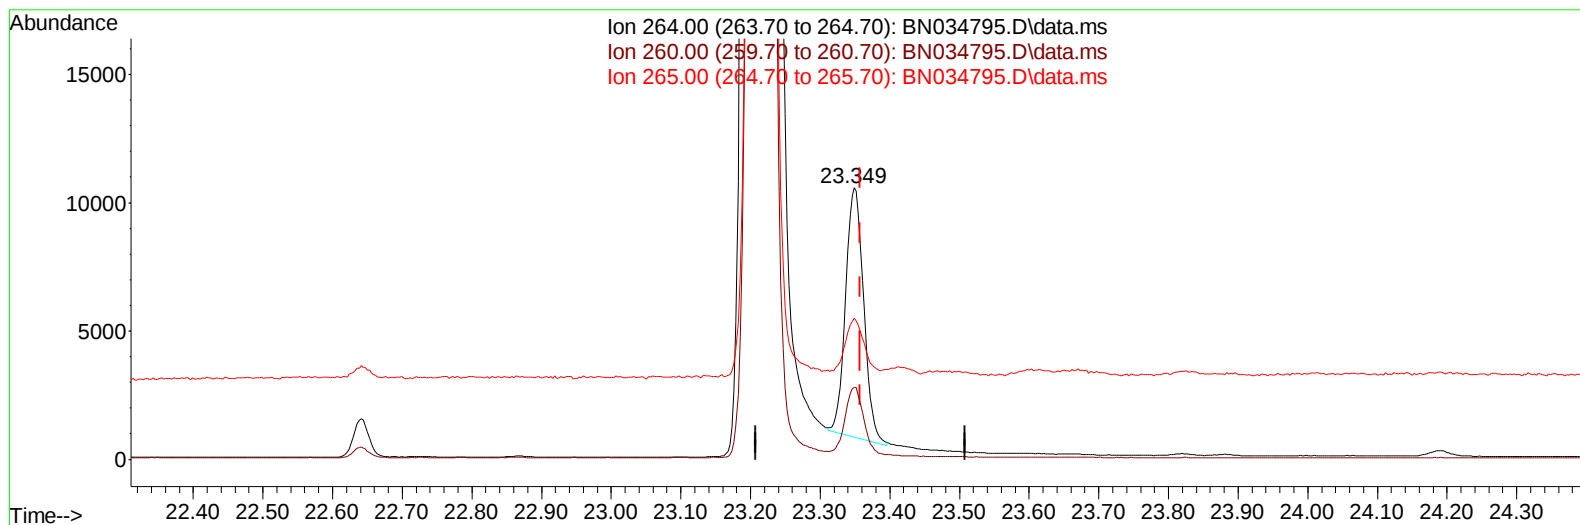

TIC: BN034795.D\data.ms

(23) Perylene-d12 (I)

23.349min (-0.009) 0.40 ng/ul m

response 17478

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	26.64
265.00	57.90	51.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

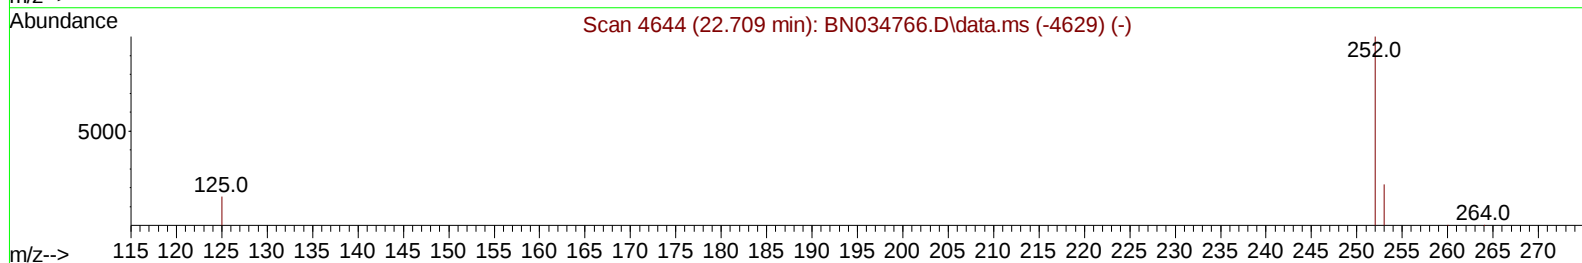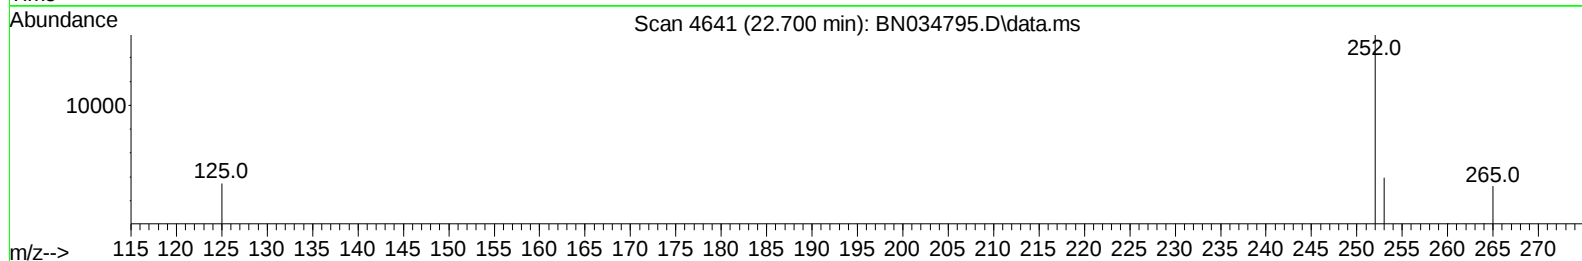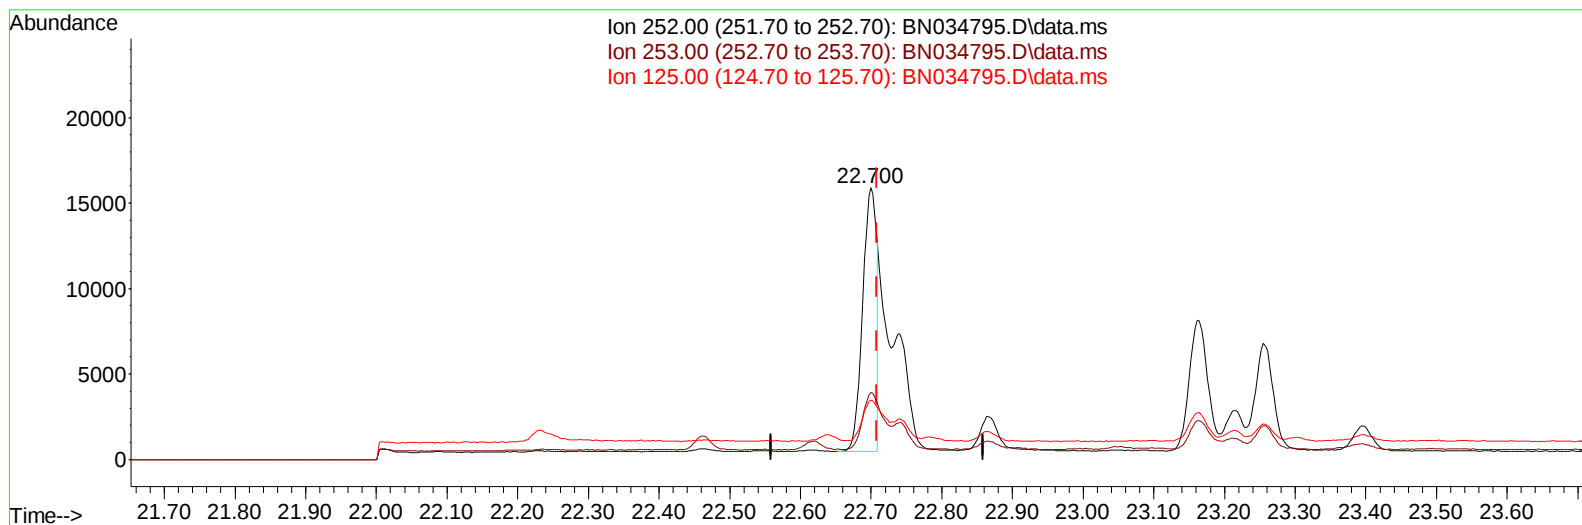

TIC: BN034795.D\data.ms

(24) Benzo(b)fluoranthene

22.700min (-0.009) 0.29 ng/u1

response 20970

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.80	24.76
125.00	20.70	21.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

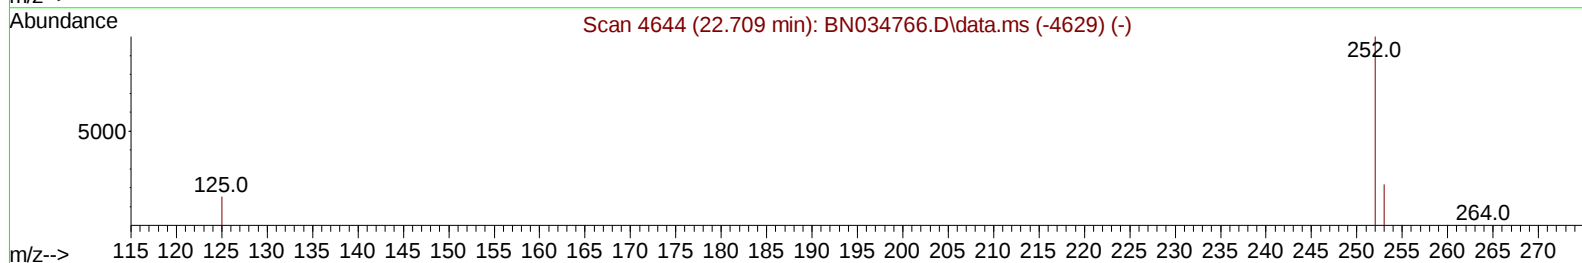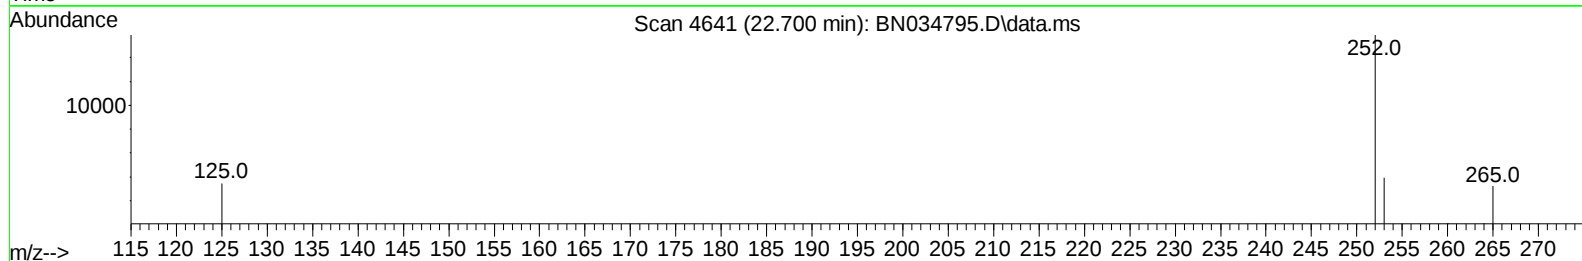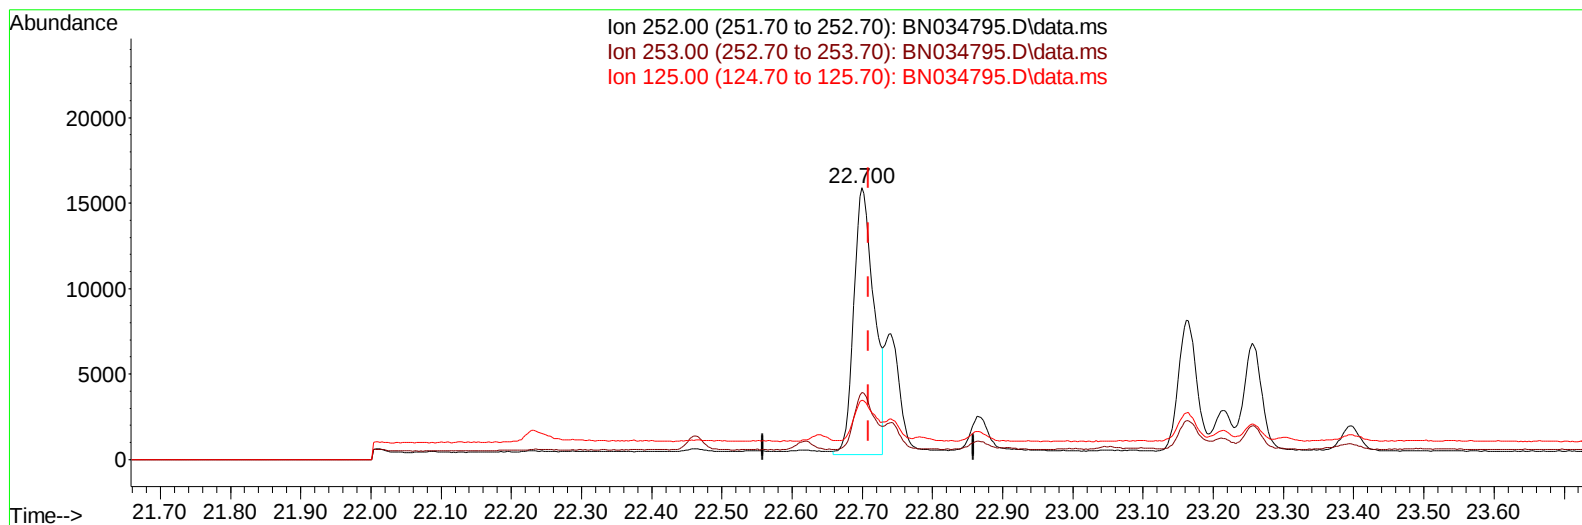

TIC: BN034795.D\data.ms

(24) Benzo(b)fluoranthene

22.700min (-0.009) 0.44 ng/u1 m

response 31287

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.80	24.76
125.00	20.70	21.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

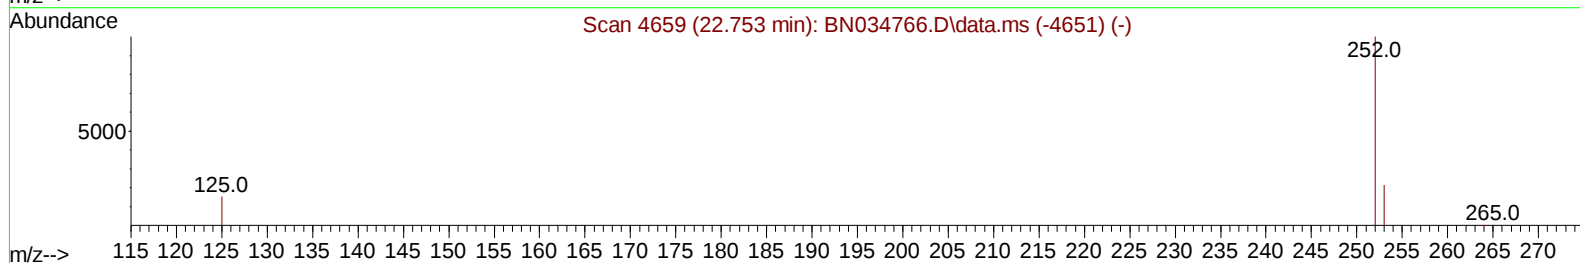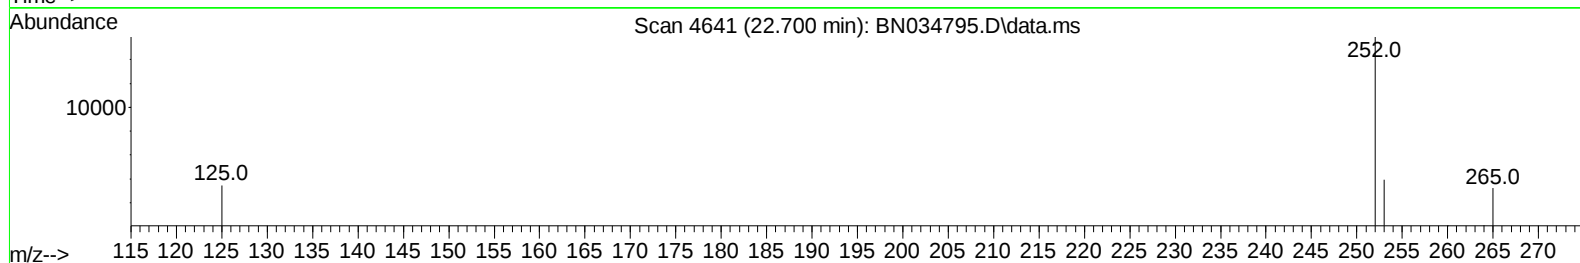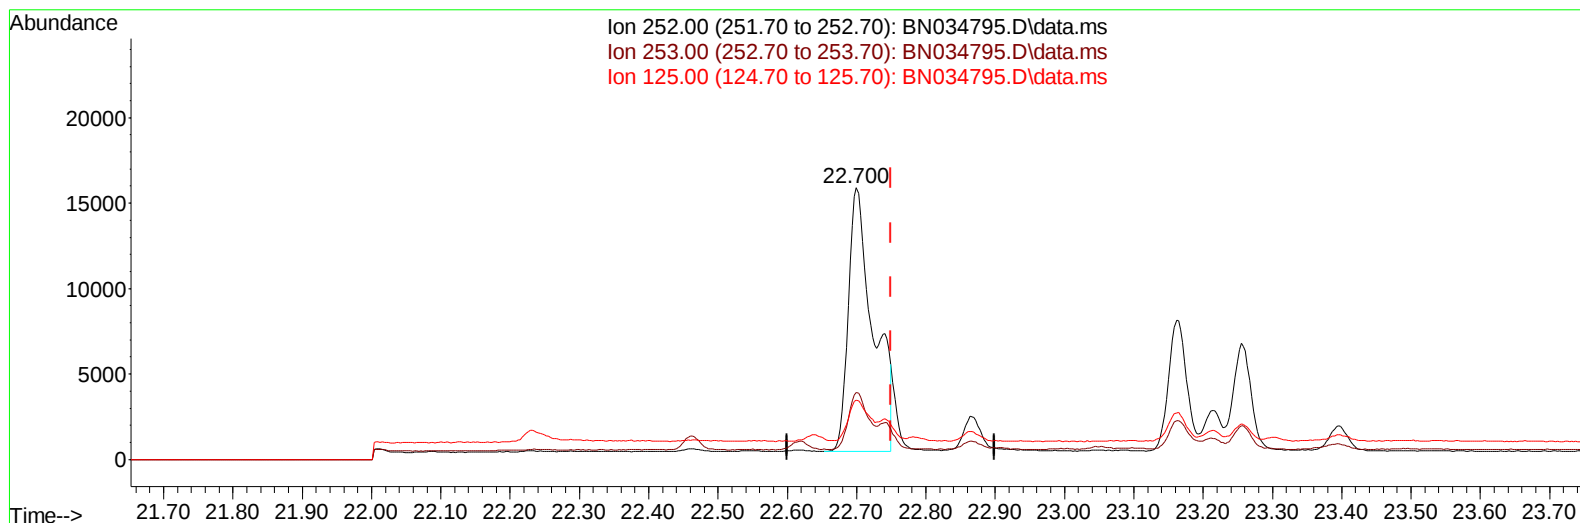

TIC: BN034795.D\data.ms

(25) Benzo(k)fluoranthene

22.700min (-0.050) 0.53 ng/u1

response 38365

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.90	24.76
125.00	21.20	21.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

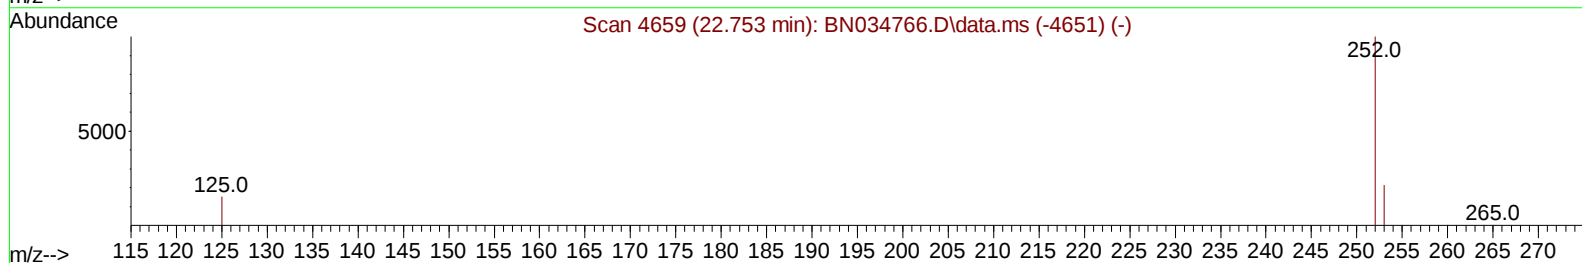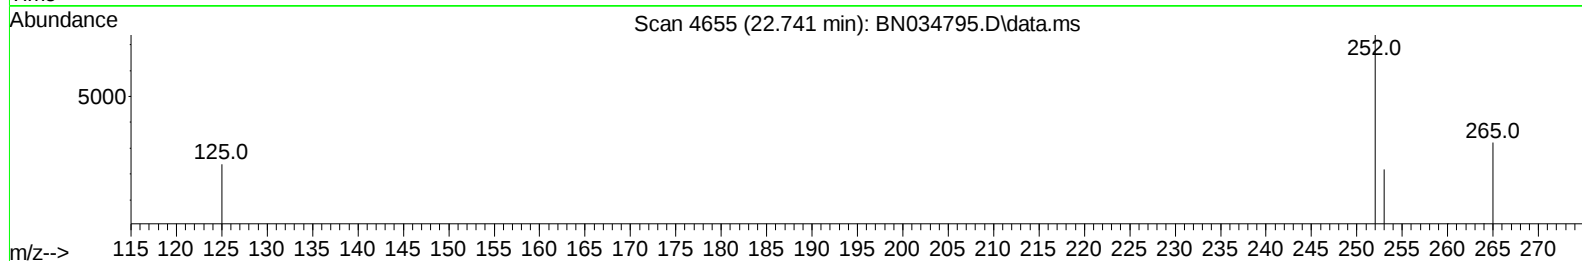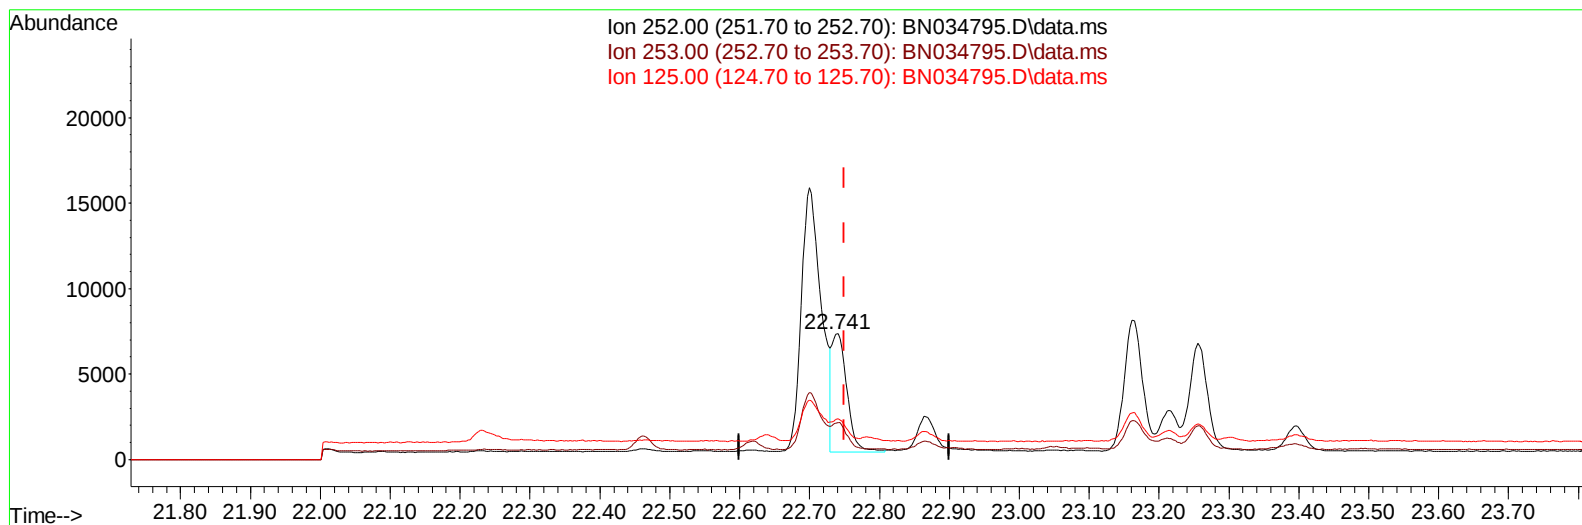

TIC: BN034795.D\data.ms

(25) Benzo(k)fluoranthene

22.741min (-0.009) 0.15 ng/u1 m

response 10431

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.90	29.39#
125.00	21.20	32.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

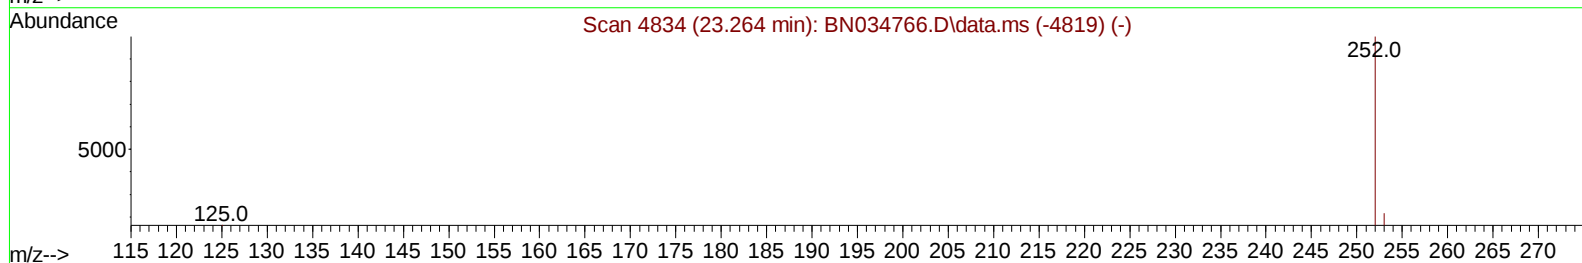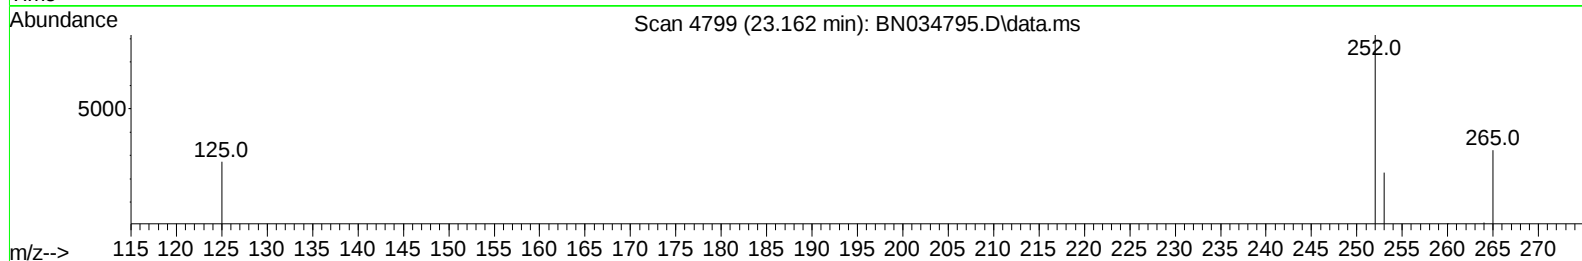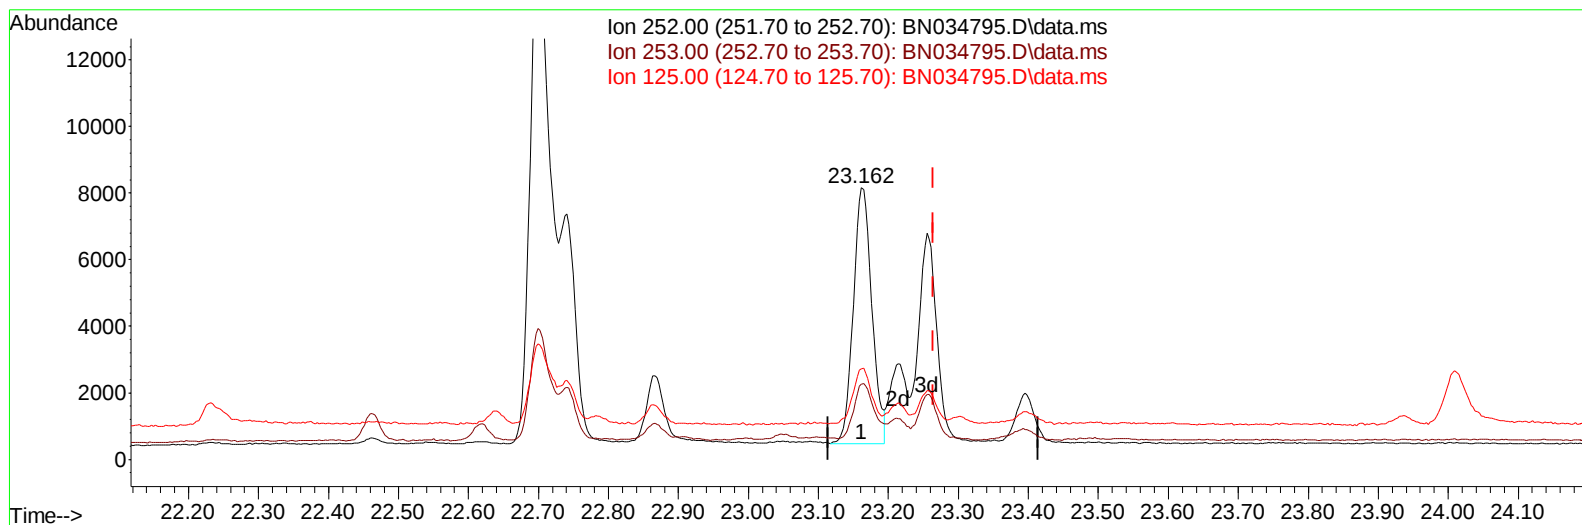

TIC: BN034795.D\data.ms

(26) Benzo(a)pyrene (C)

23.162min (-0.103) 0.23 ng/u1

response 14138

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	27.71
125.00	24.70	33.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

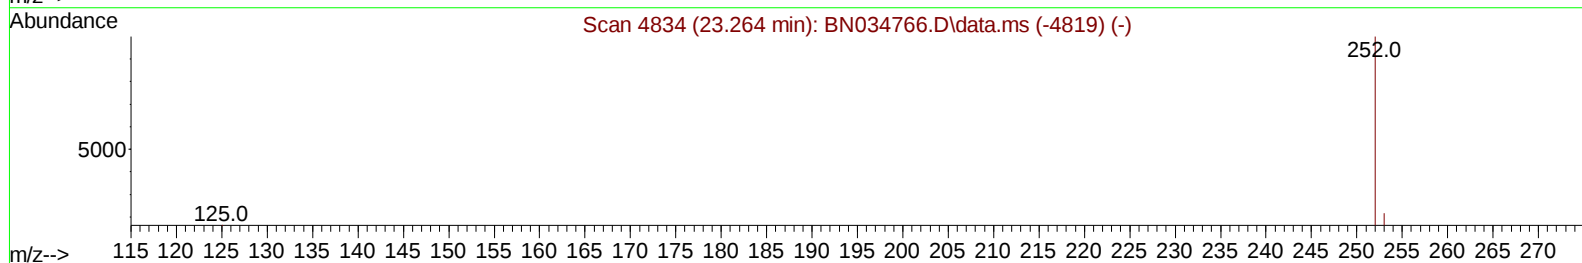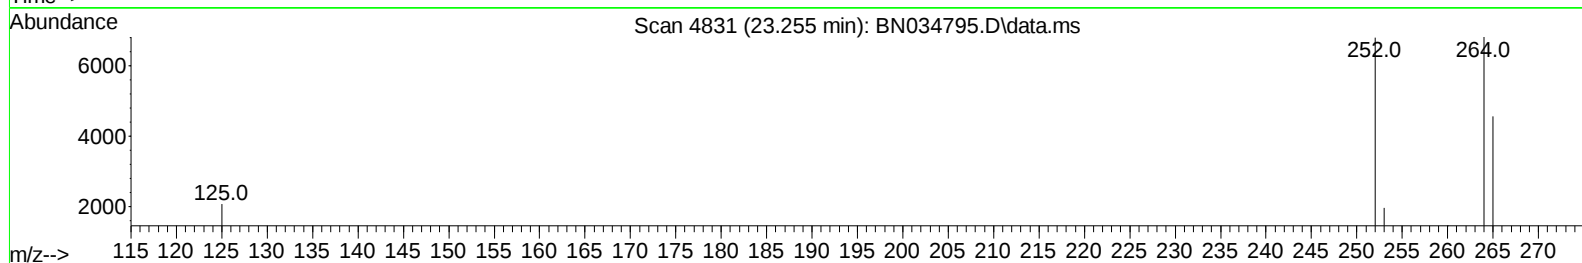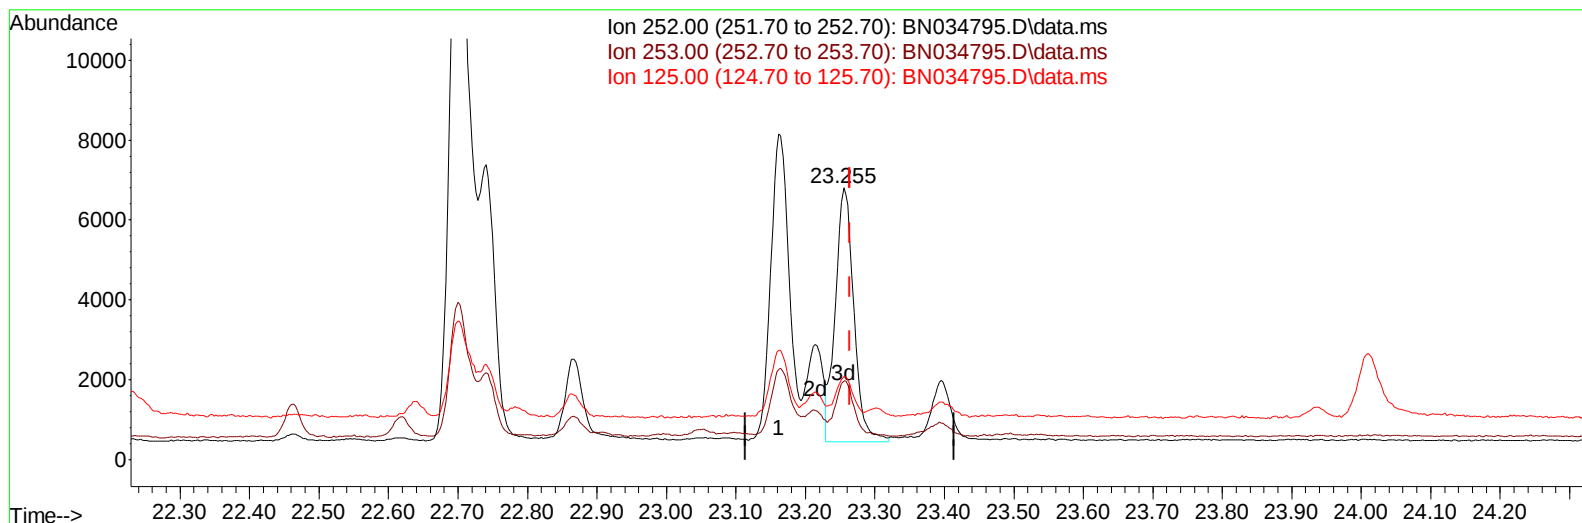

TIC: BN034795.D\data.ms

(26) Benzo(a)pyrene (C)

23.255min (-0.009) 0.19 ng/u1 m

response 11777

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	28.82
125.00	24.70	30.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034795.D
 Acq On : 01 Nov 2024 09:20
 Operator : RC/JU
 Sample : P4529-17
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

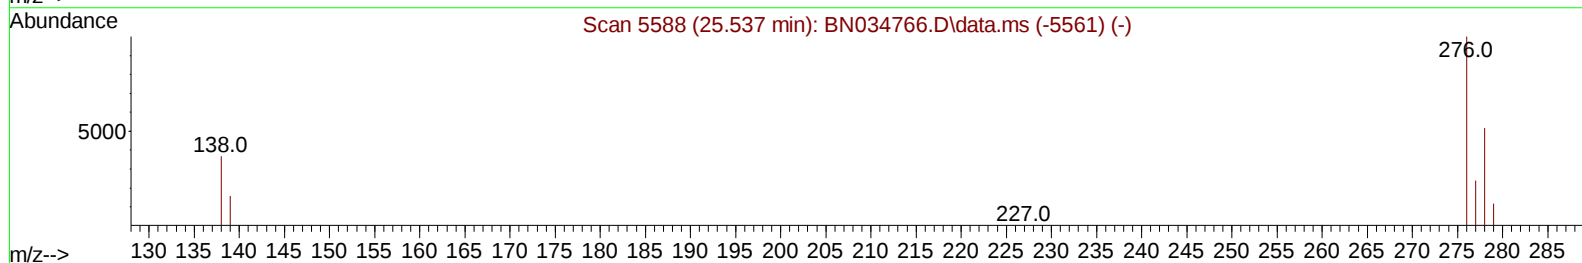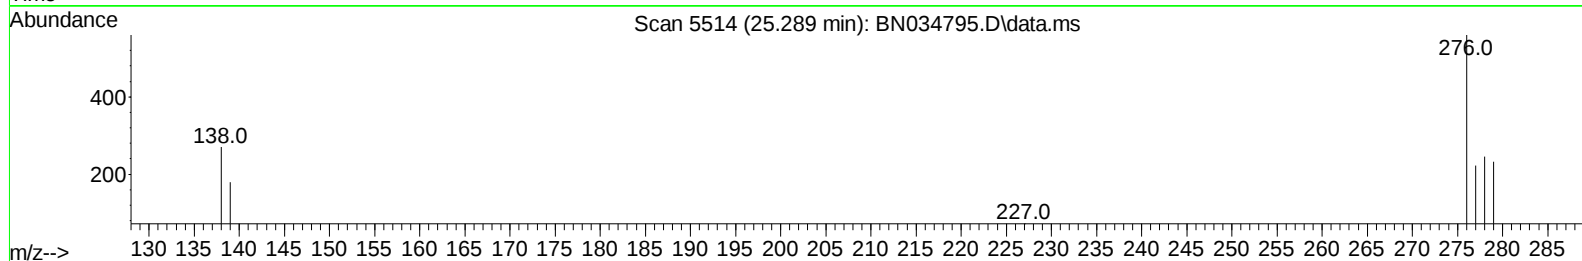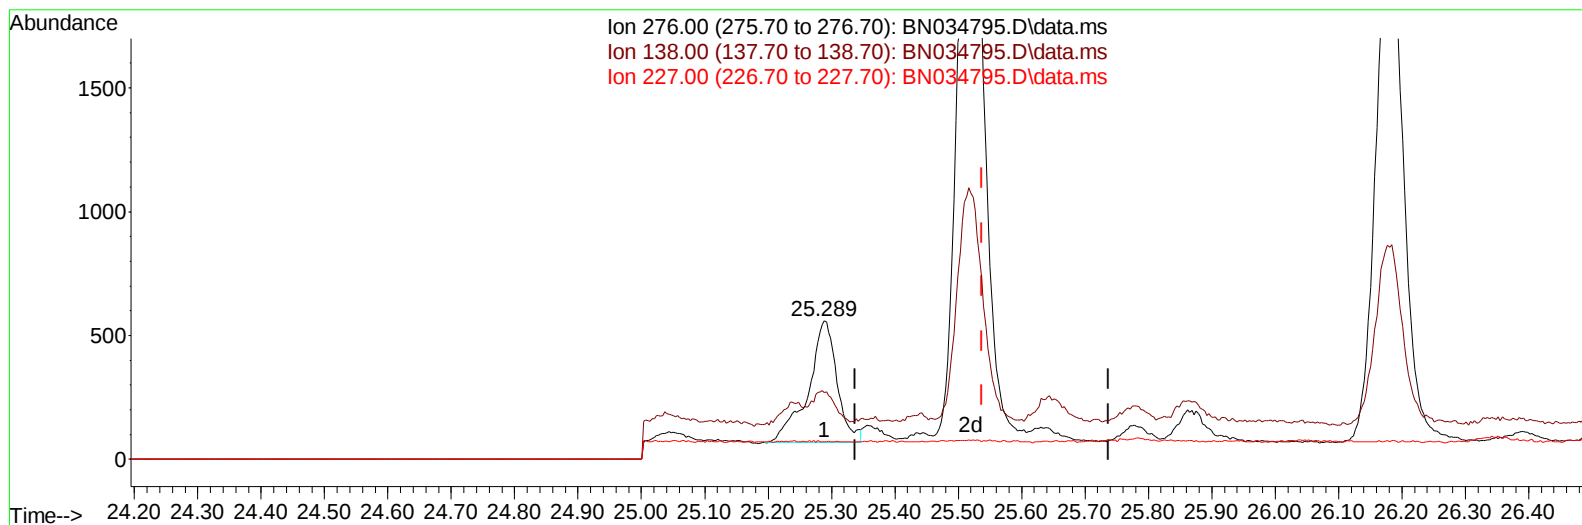

TIC: BN034795.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.289min (-0.248) 0.02 ng/u1

response 1546

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	39.70	19.92#
227.00	0.30	0.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

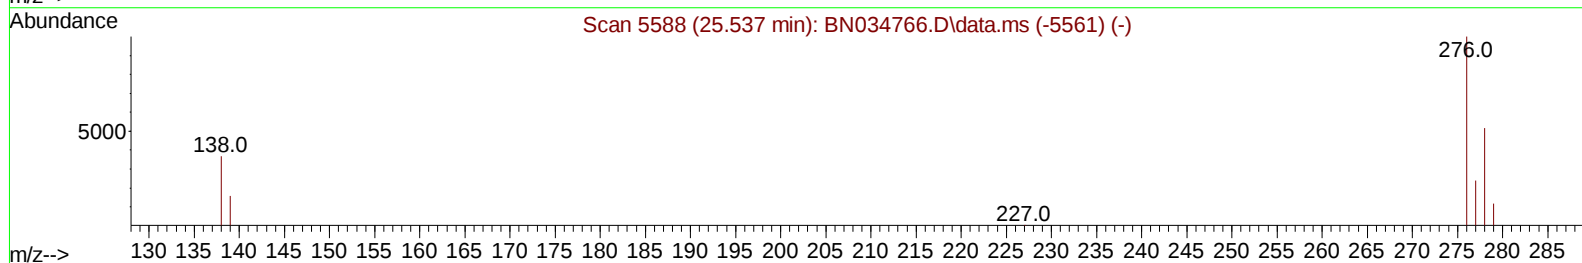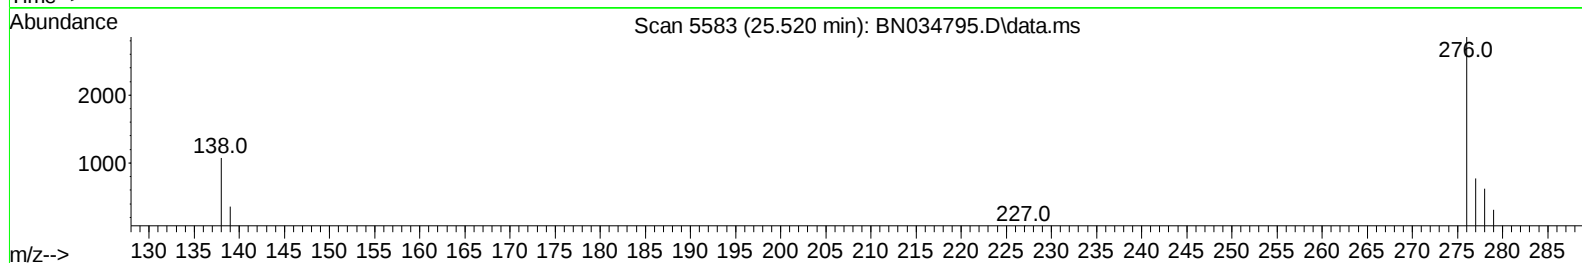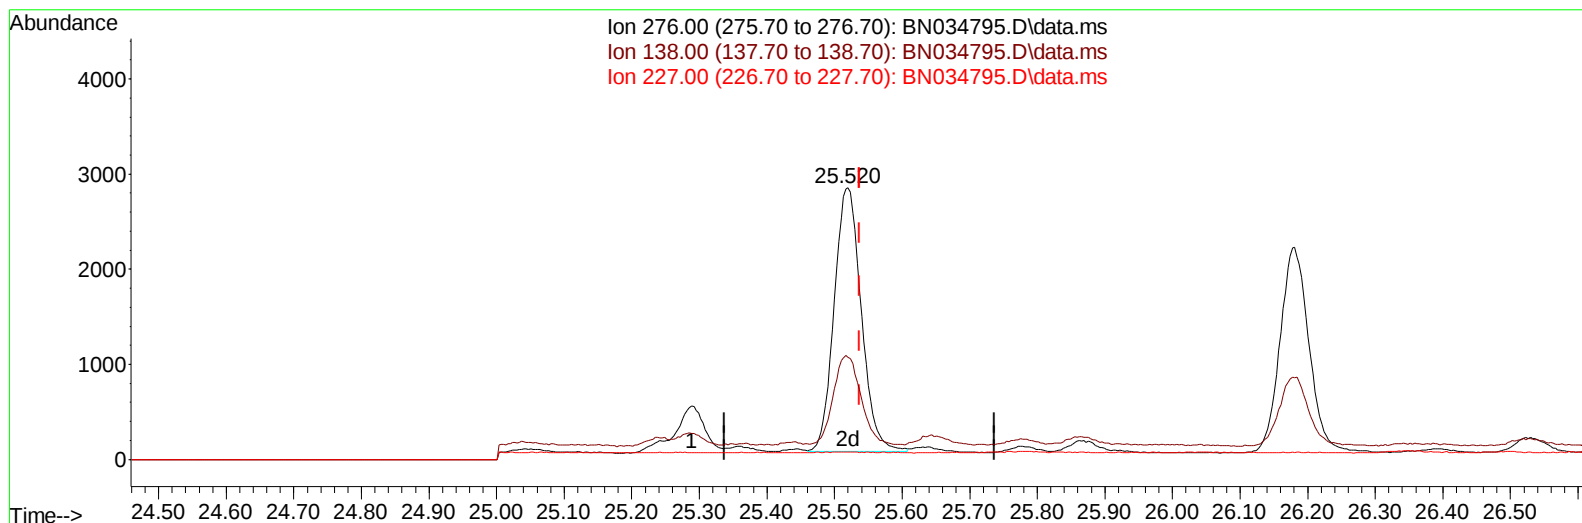

TIC: BN034795.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.520min (-0.017) 0.12 ng/u1 m

response 7691

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	39.70	4.00#
227.00	0.30	0.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

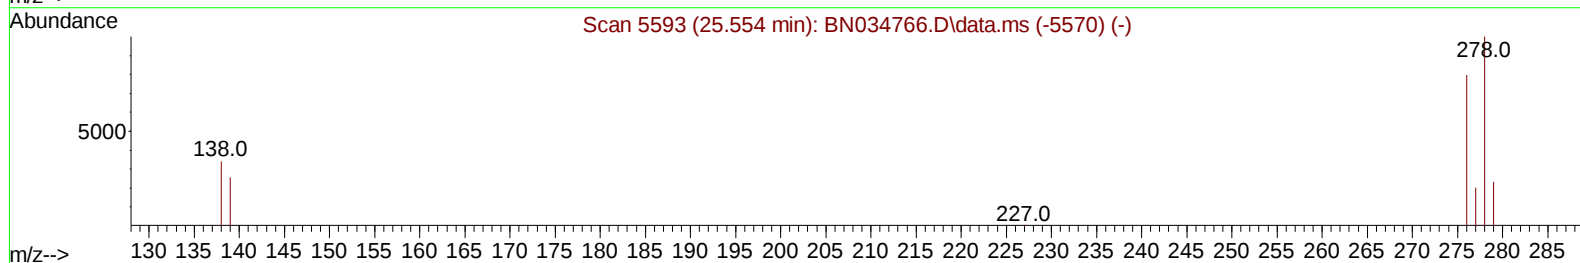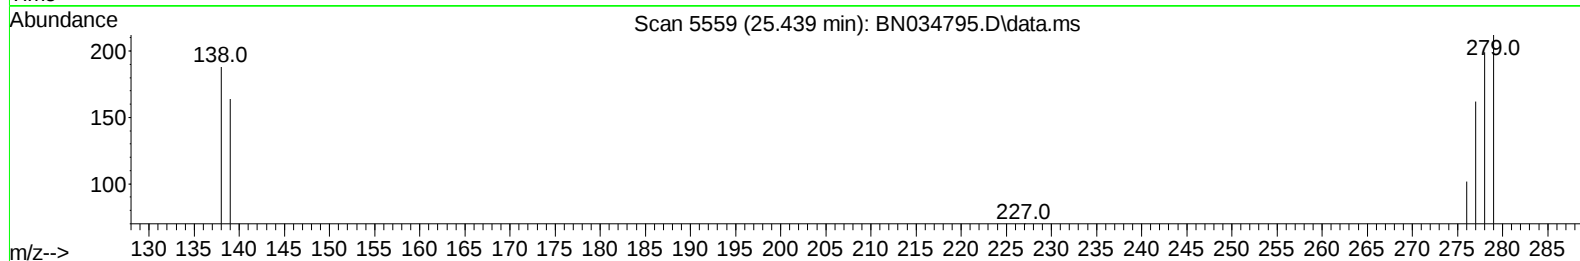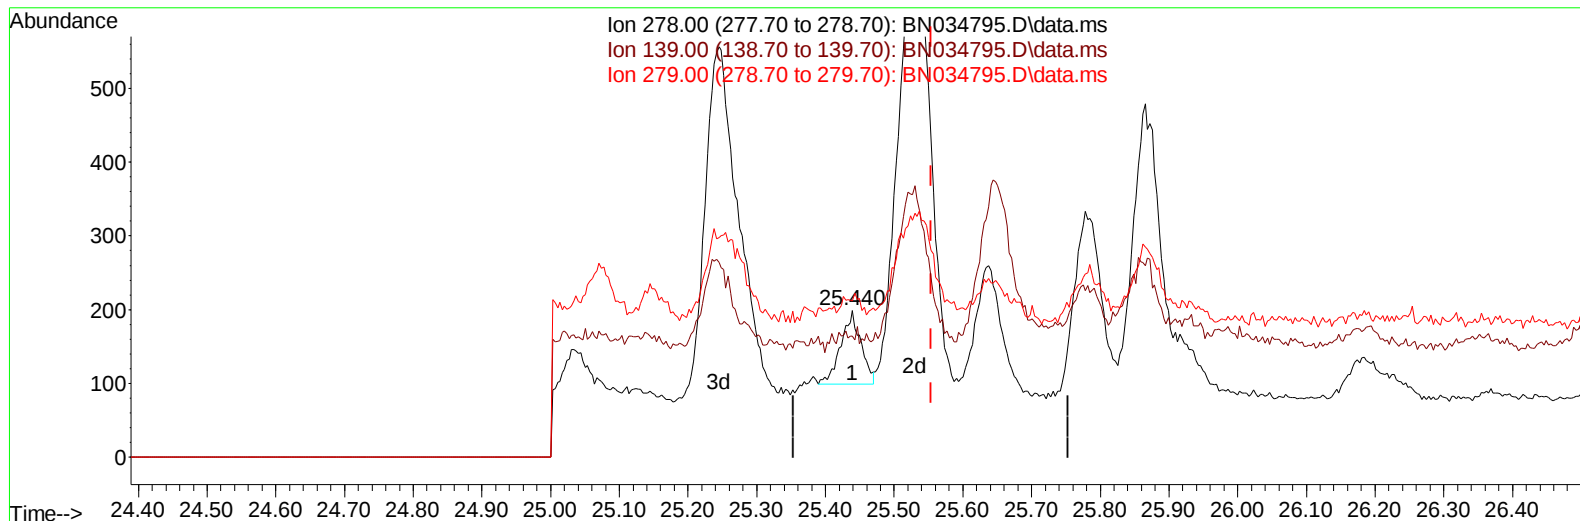

TIC: BN034795.D\data.ms

(28) Dibenzo(a,h)anthracene

25.439min (-0.114) 0.00 ng/u1

response 203

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	29.30	82.41#
279.00	25.80	106.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

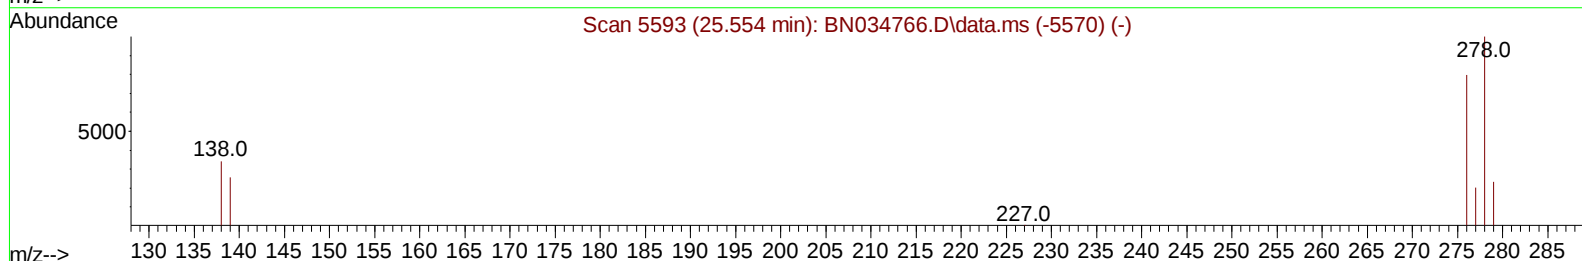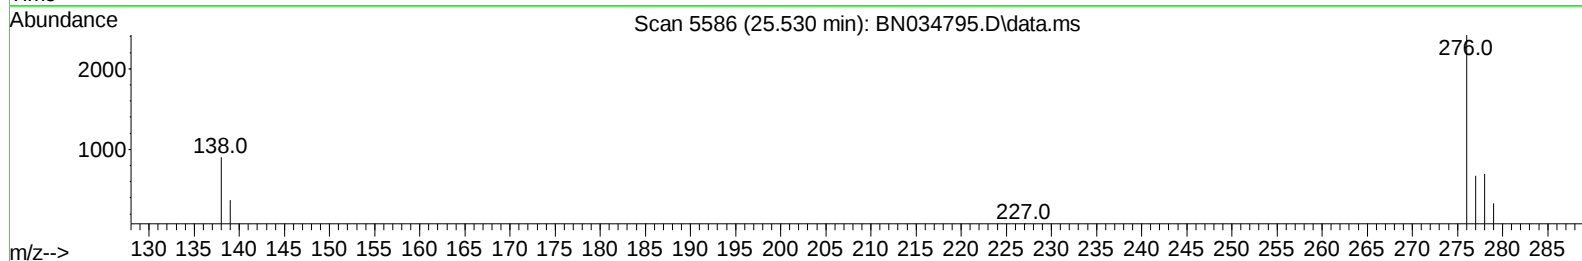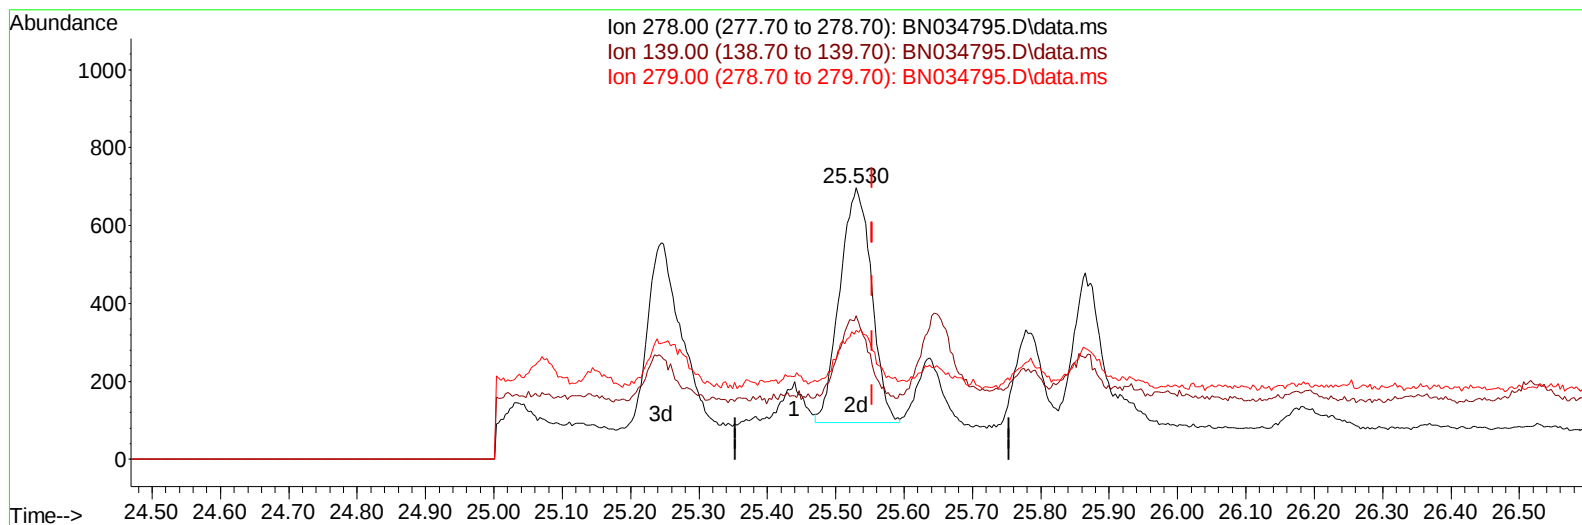

TIC: BN034795.D\data.ms

(28) Dibenzo(a,h)anthracene

25.530min (-0.024) 0.04 ng/u1 m

response 1952

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	29.30	52.80#
279.00	25.80	47.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

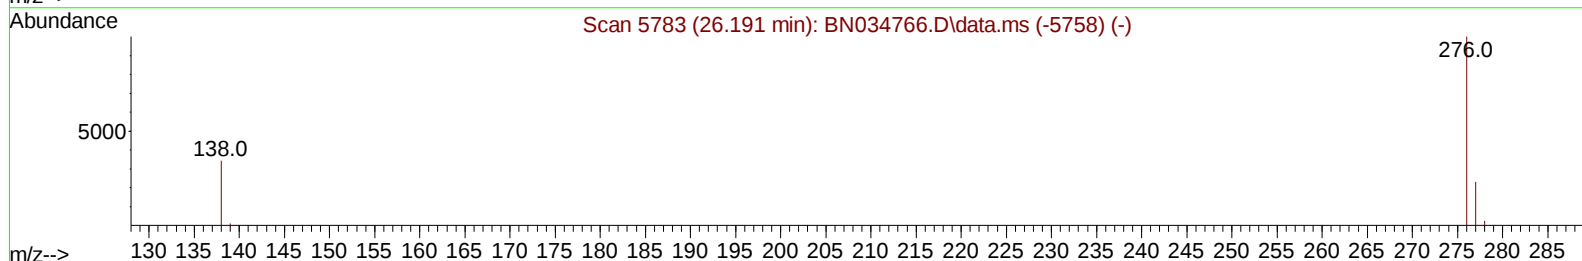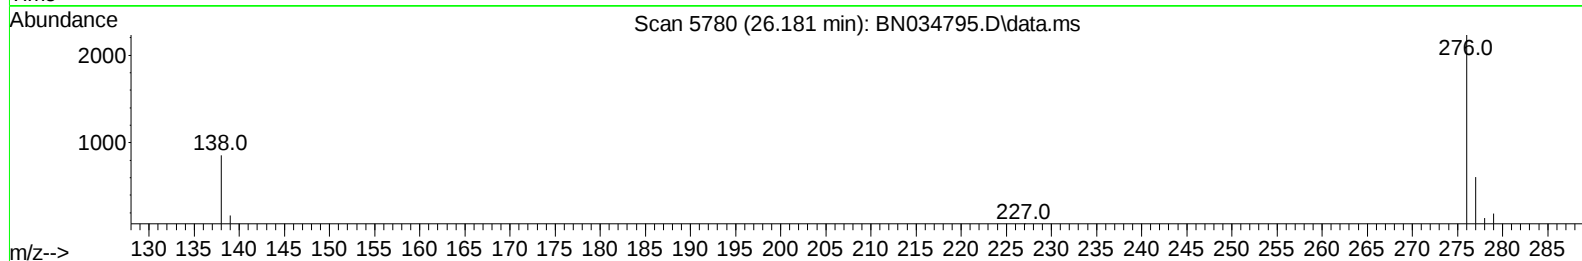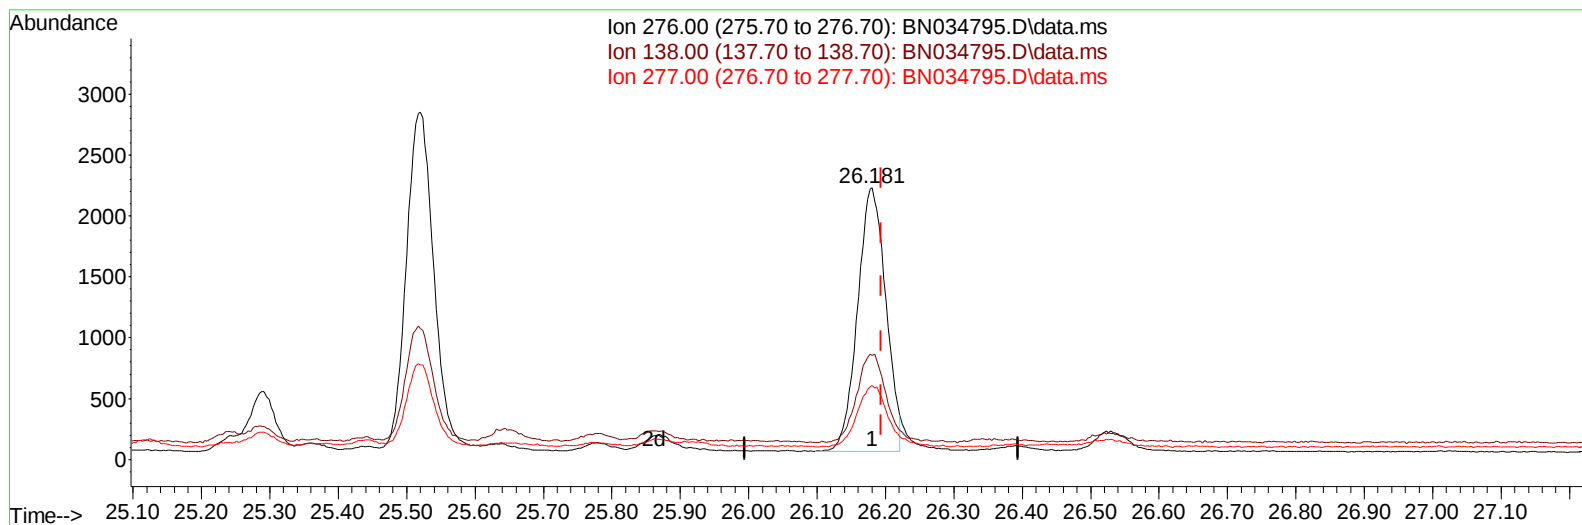

TIC: BN034795.D\data.ms

(29) Benzo(g,h,i)perylene

26.181min (-0.014) 0.12 ng/u1

response 6201

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	36.00	38.37
277.00	25.20	27.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

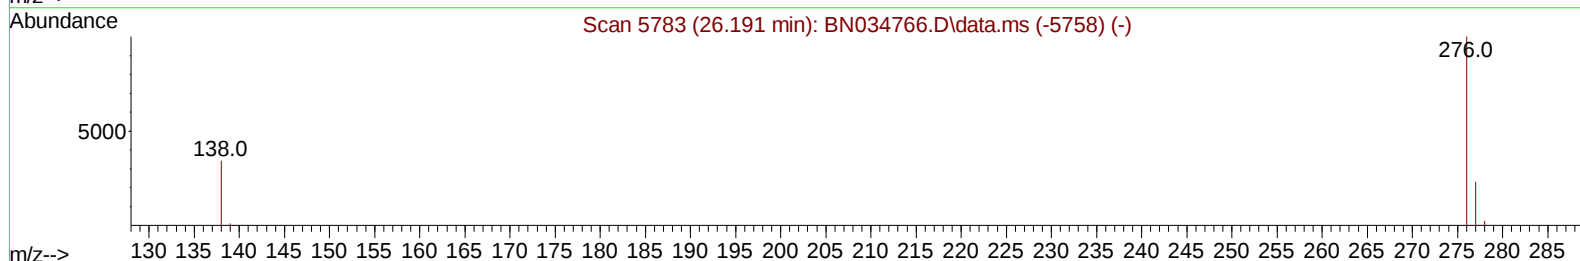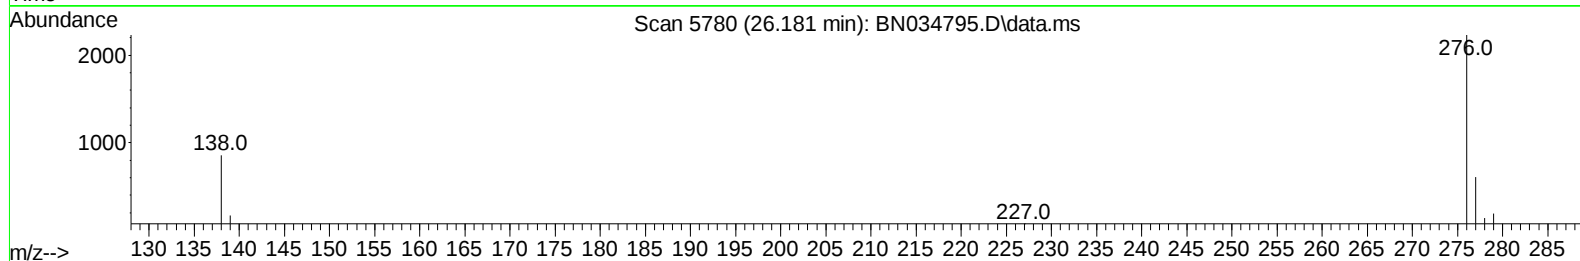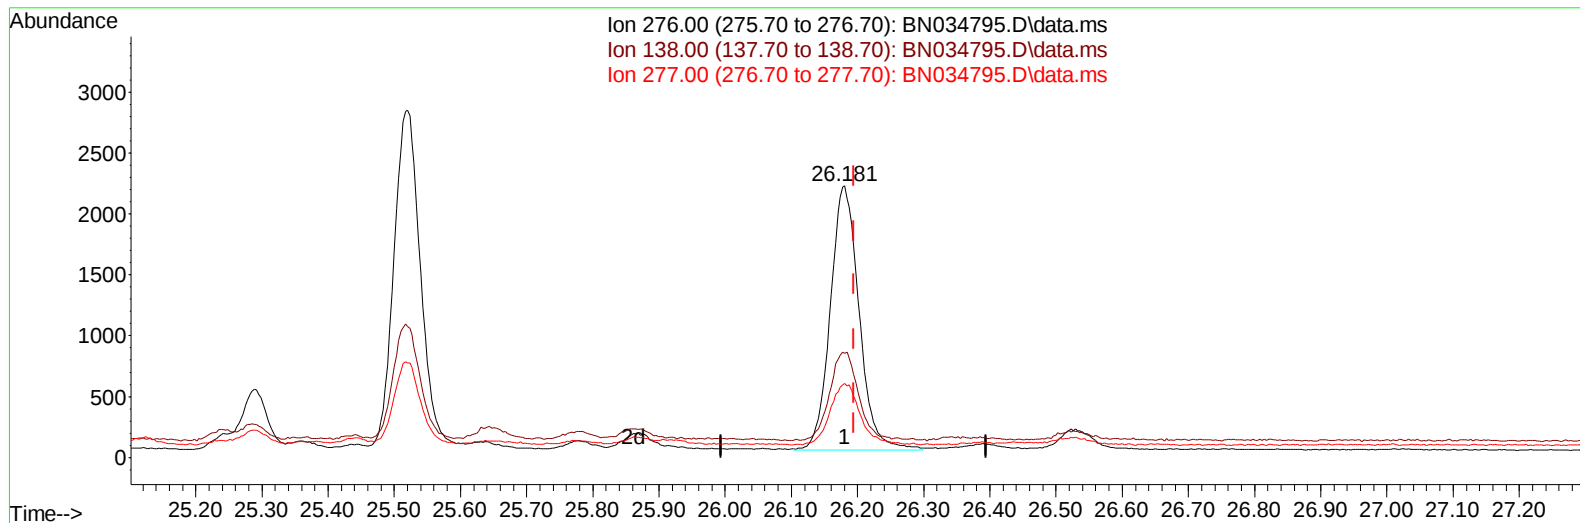

TIC: BN034795.D\data.ms

(29) Benzo(g,h,i)perylene

26.181min (-0.014) 0.13 ng/ul m

response 6529

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	36.00	38.37
277.00	25.20	27.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034795.D
 Acq On : 01 Nov 2024 09:20
 Operator : RC/JU
 Sample : P4529-17
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H45

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:25:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.600	152		8341	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136		26522	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.231	164		15130	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.979	188		30730	0.400	ng/ul	0.00
17) Chrysene-d12	21.168	240		21696	0.400	ng/ul	0.00
23) Perylene-d12	23.349	264		17478m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.170	96		35880	4.156	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152		9399	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.009	212		18651	0.264	ng/ul	0.00
Target Compounds							
							Qvalue
10) Acenaphthylene	13.949	152		3395	0.049	ng/ul#	94
15) Phenanthrene	17.017	178		3342	0.036	ng/ul#	93
16) Anthracene	17.110	178		4352	0.051	ng/ul#	94
19) Fluoranthene	19.037	202		21088	0.200	ng/ul	96
20) Pyrene	19.404	202		21787m	0.199	ng/ul	
21) Benzo(a)anthracene	21.154	228		9189m	0.106	ng/ul	
22) Chrysene	21.204	228		19016	0.219	ng/ul	98
24) Benzo(b)fluoranthene	22.700	252		31287m	0.440	ng/ul	
25) Benzo(k)fluoranthene	22.741	252		10431m	0.145	ng/ul	
26) Benzo(a)pyrene	23.255	252		11777m	0.192	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.520	276		7691m	0.118	ng/ul	
28) Dibenzo(a,h)anthracene	25.530	278		1952m	0.040	ng/ul	
29) Benzo(g,h,i)perylene	26.181	276		6529m	0.127	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034795.D
Acq On : 01 Nov 2024 09:20
Operator : RC/JU
Sample : P4529-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F7H45

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:25:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

