




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034811.D
Acq On : 01 Nov 2024 19:00
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L79

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

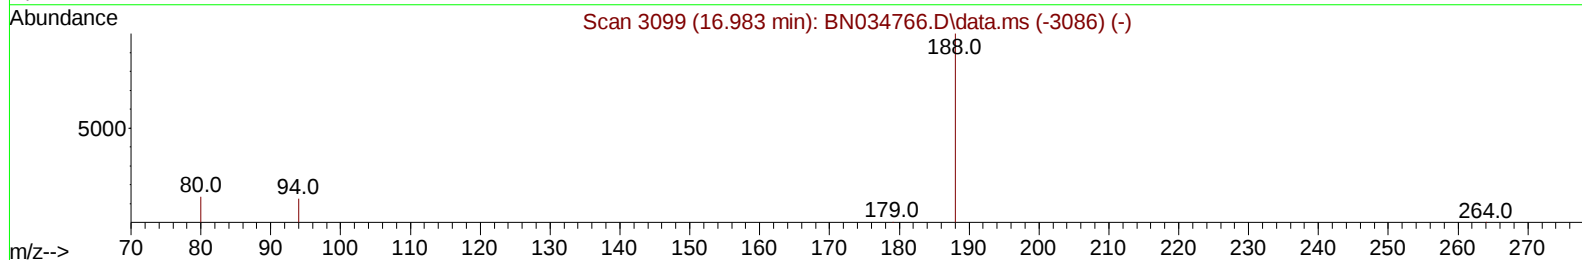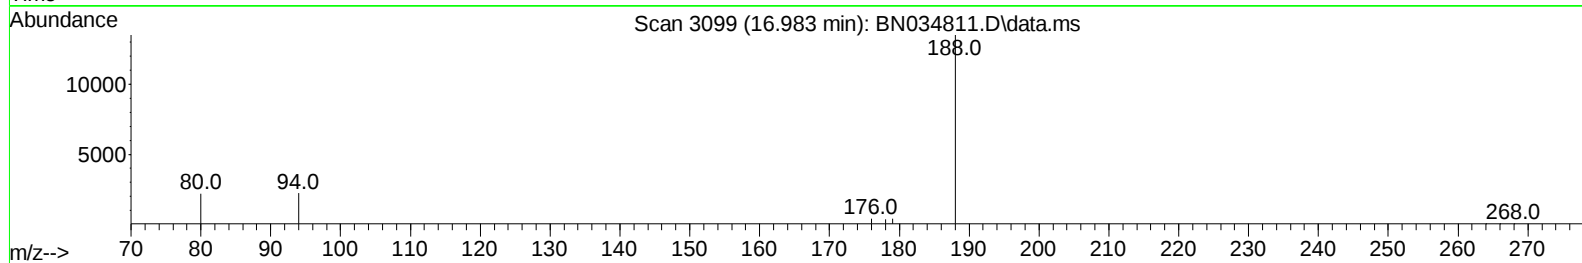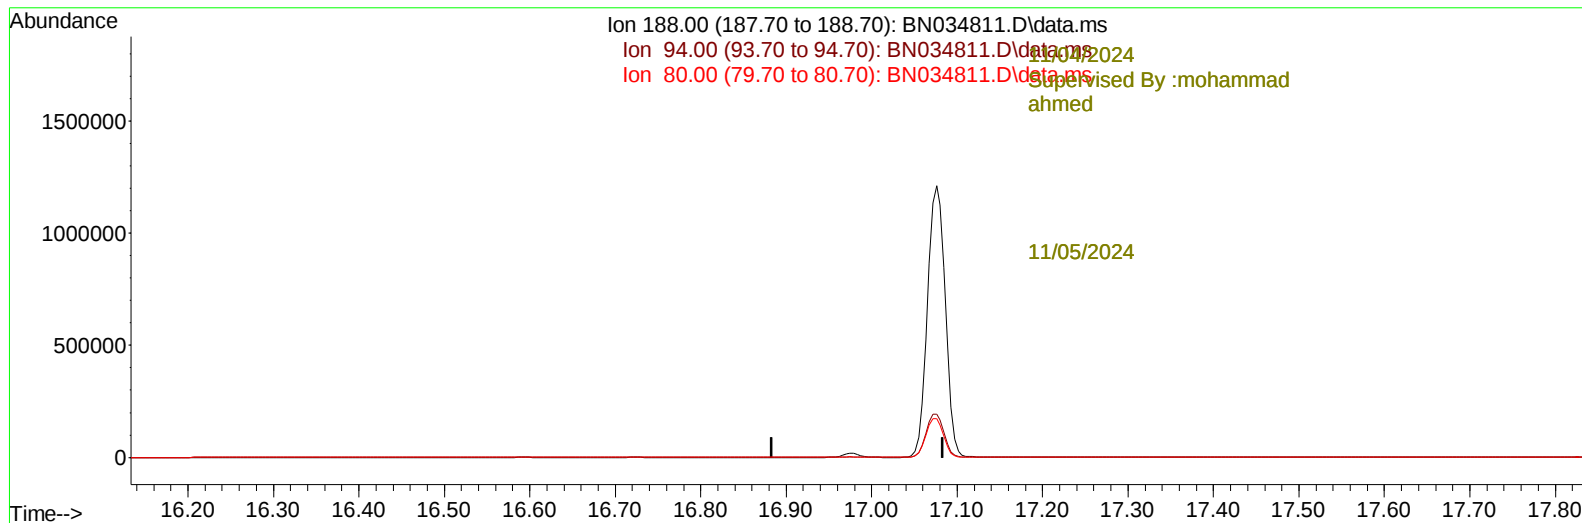

TIC: BN034811.D\data.ms

(13) Phenanthrene-d10 (I)

16.983min (-16.983) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.60	0.00#
80.00	14.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034811.D
Acq On : 01 Nov 2024 19:00
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L79

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

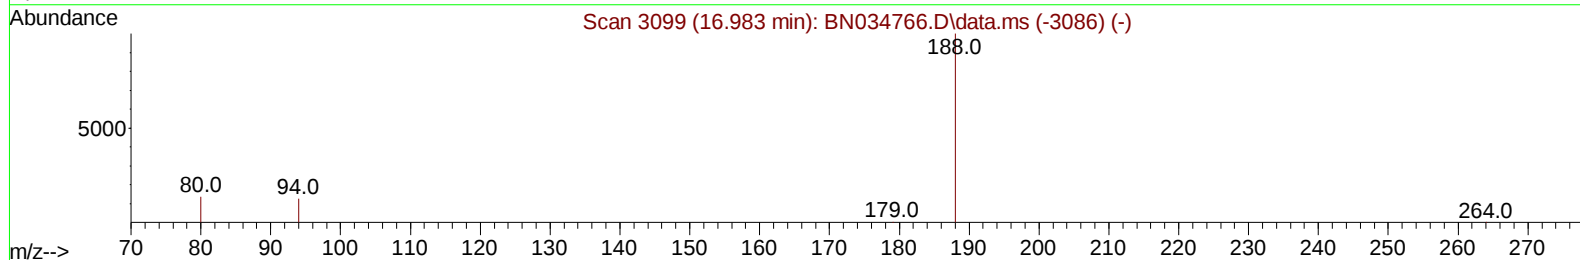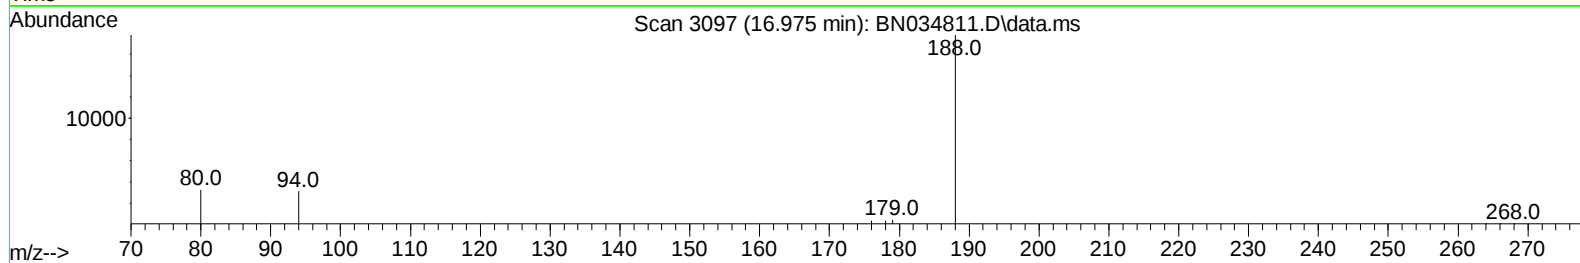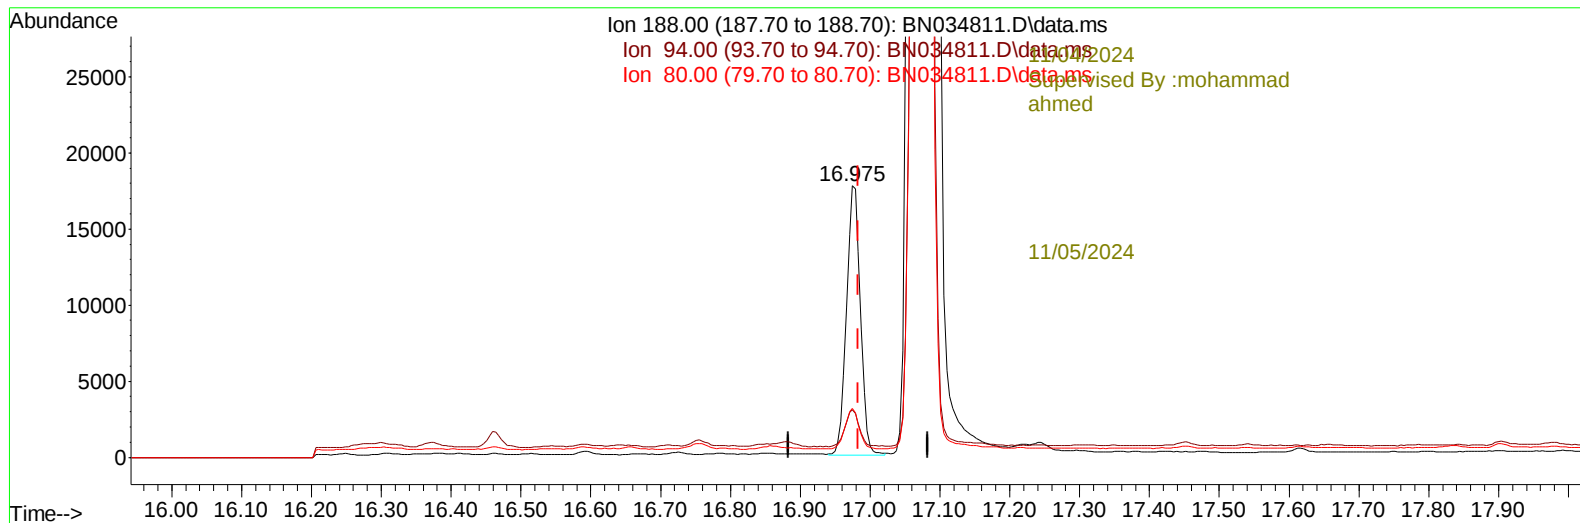

TIC: BN034811.D\data.ms

(13) Phenanthrene-d10 (I)

16.975min (-0.009) 0.40 ng/ul m

response 24483

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.60	17.52#
80.00	14.50	18.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034811.D
Acq On : 01 Nov 2024 19:00
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L79

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

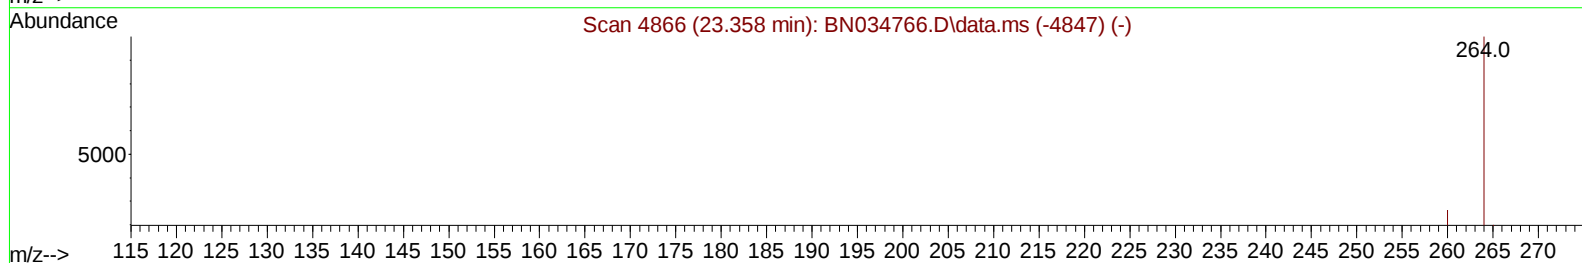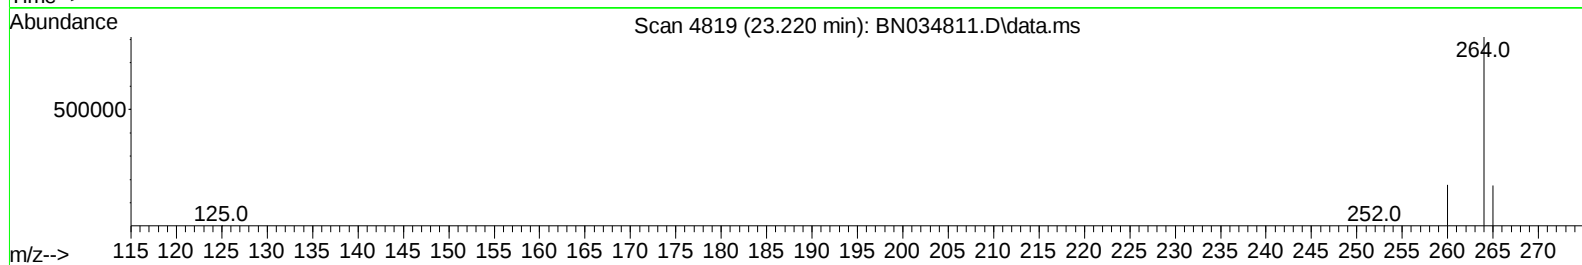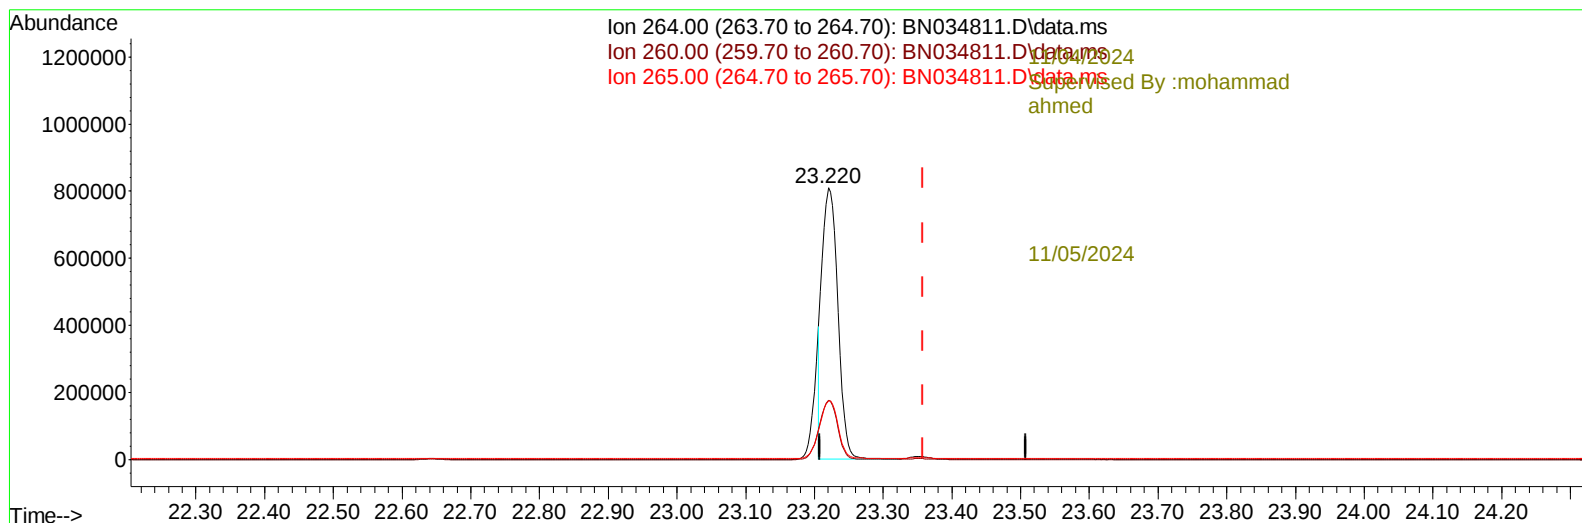

TIC: BN034811.D\data.ms

(23) Perylene-d12 (I)

23.220min (-0.138) 0.40 ng/u1

response 1301791

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	21.73#
265.00	57.90	21.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034811.D
Acq On : 01 Nov 2024 19:00
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L79

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

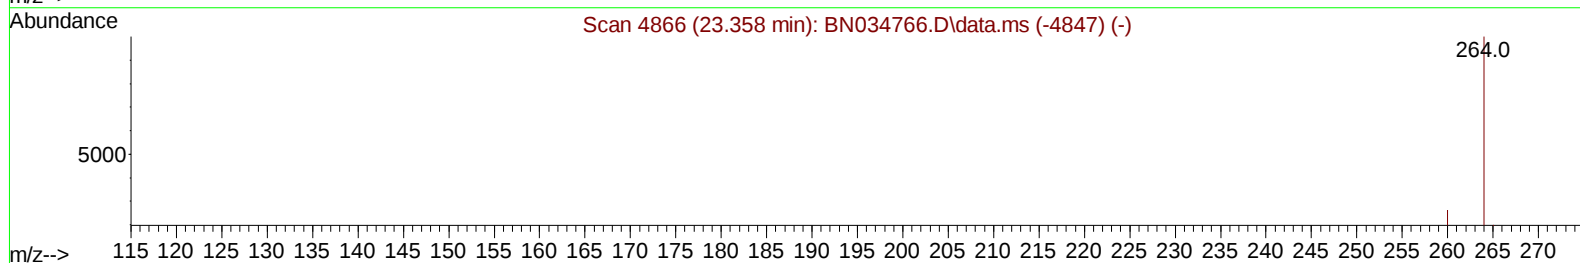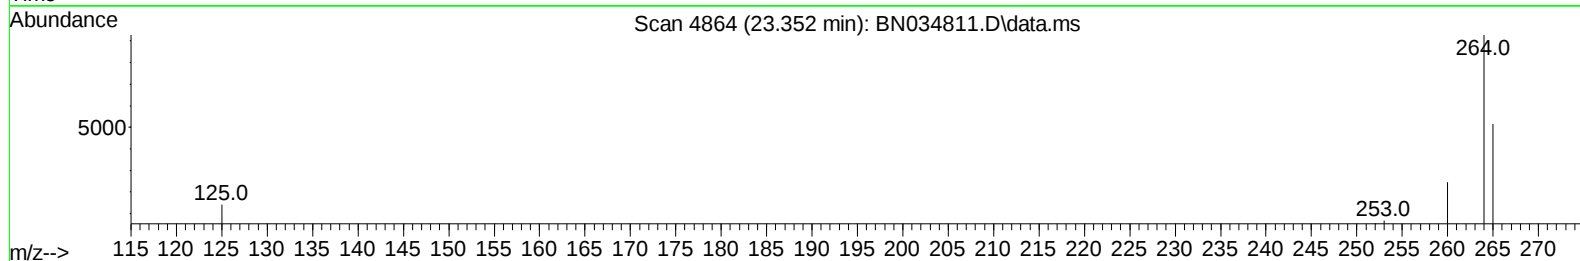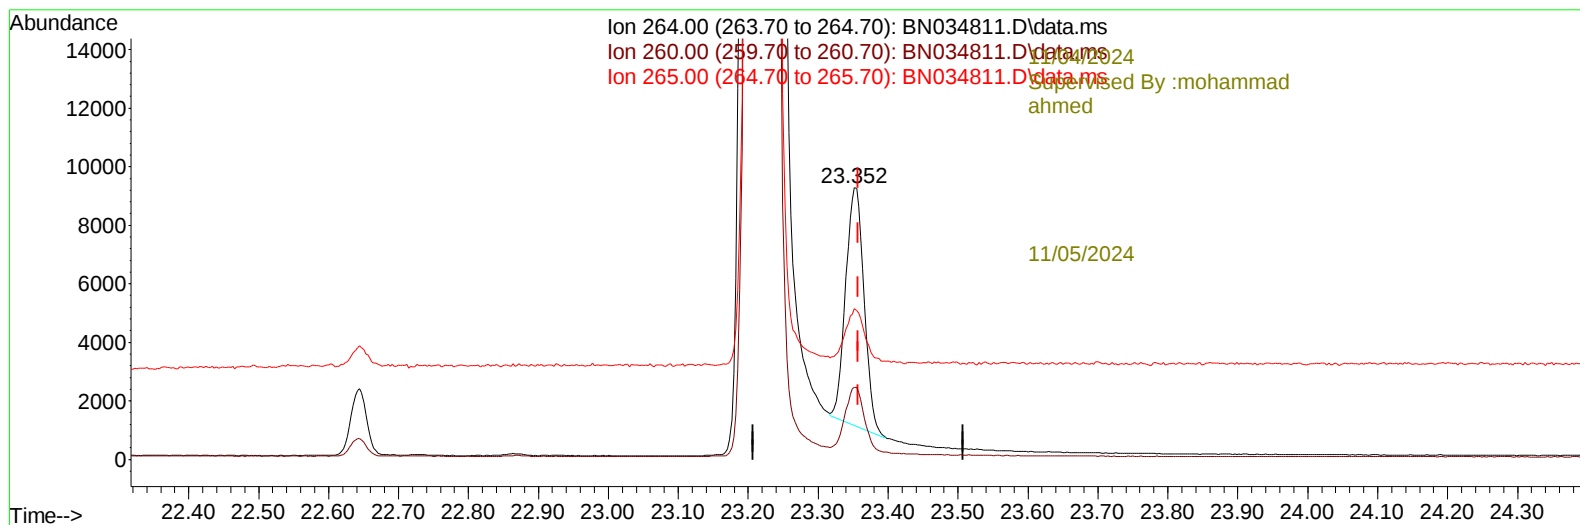

TIC: BN034811.D\data.ms

(23) Perylene-d12 (I)

23.352min (-0.006) 0.40 ng/ul m

response 14863

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	26.53
265.00	57.90	55.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034811.D
 Acq On : 01 Nov 2024 19:00
 Operator : RC/JU
 Sample : P4558-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L79

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:27:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----11/04/2024							
Supervised By :mohammad							
ahmed							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.596	152		6663	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136		20459	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164		11747	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188		24483m	0.400	ng/ul	0.00
17) Chrysene-d12	21.169	240		17618	0.400	ng/ul	0.00
23) Perylene-d12	23.352	264		14863m	0.400	ng/ul	0.00
-----05/2024							
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.165	96		29278	4.245	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152		10993	0.429	ng/ul	0.00
18) Fluoranthene-d10	19.009	212		26778	0.467	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034811.D
Acq On : 01 Nov 2024 19:00
Operator : RC/JU
Sample : P4558-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L79

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

