




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034812.D
Acq On : 01 Nov 2024 19:36
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L63

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

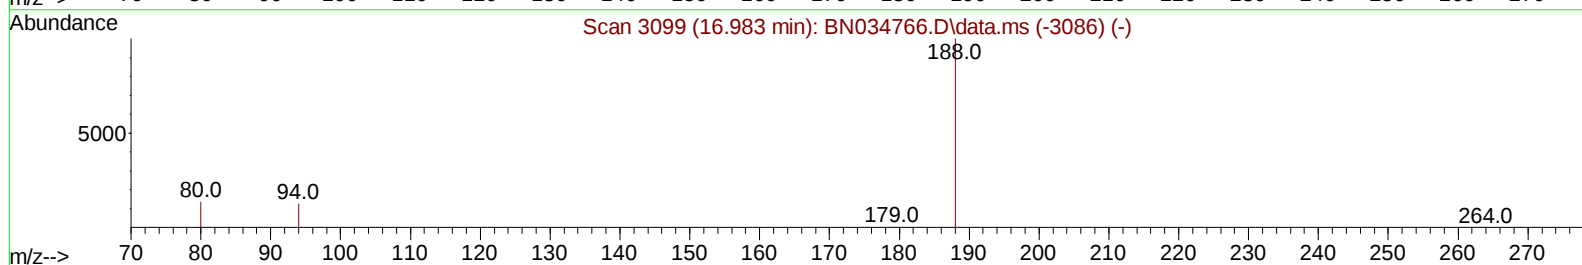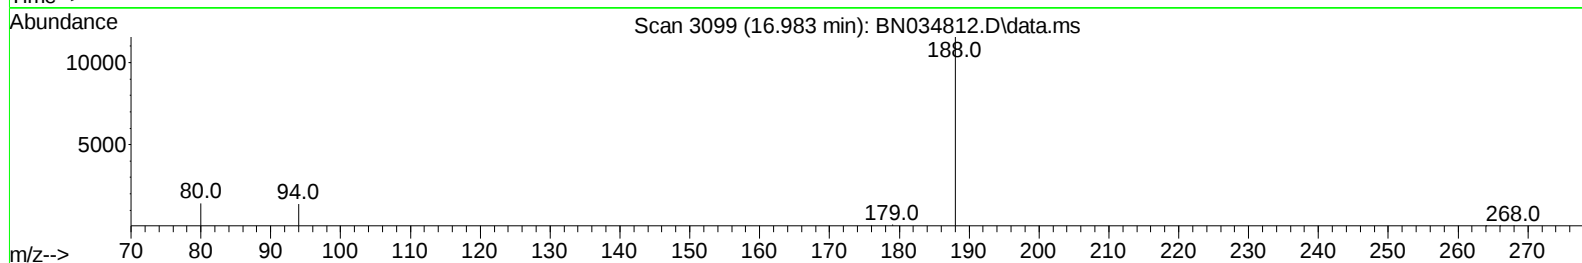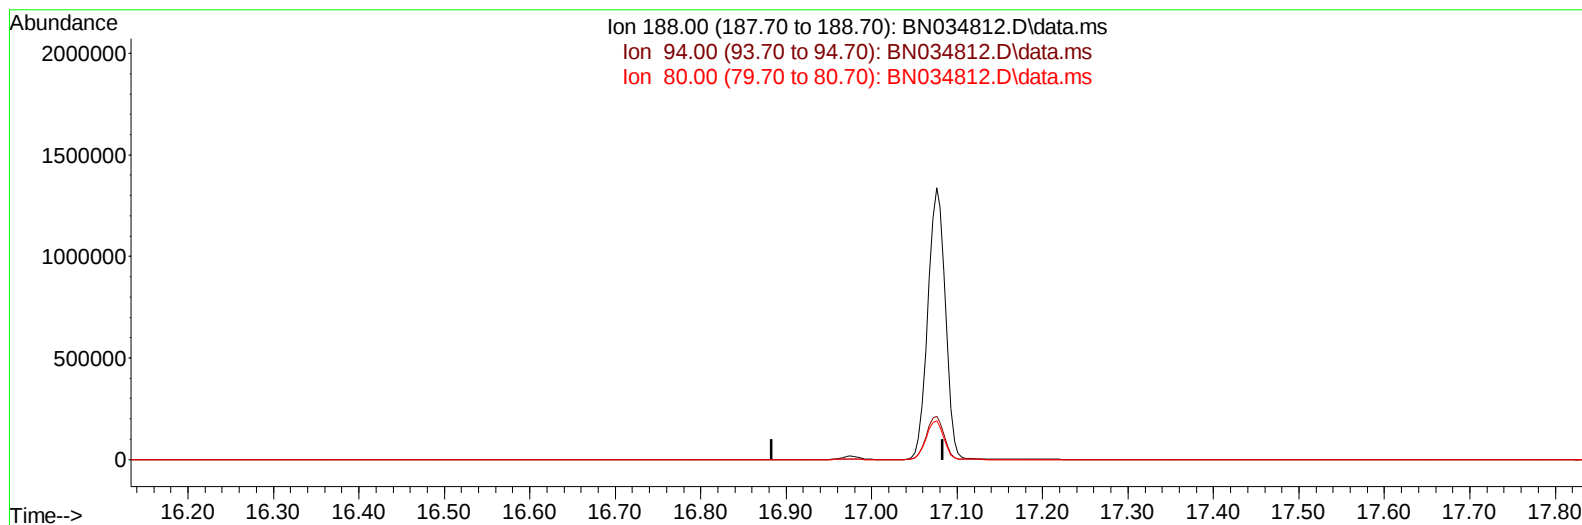

TIC: BN034812.D\data.ms

(13) Phenanthrene-d10 (I)

16.983min (-16.983) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.60	0.00#
80.00	14.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034812.D
Acq On : 01 Nov 2024 19:36
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L63

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

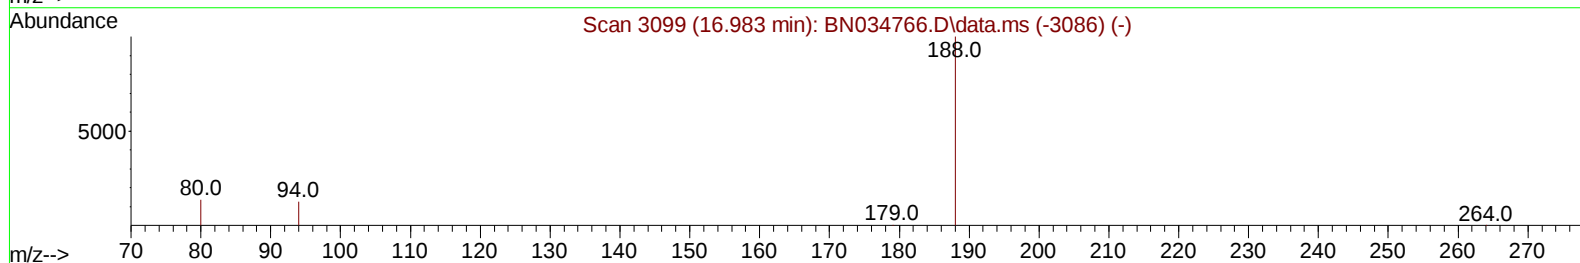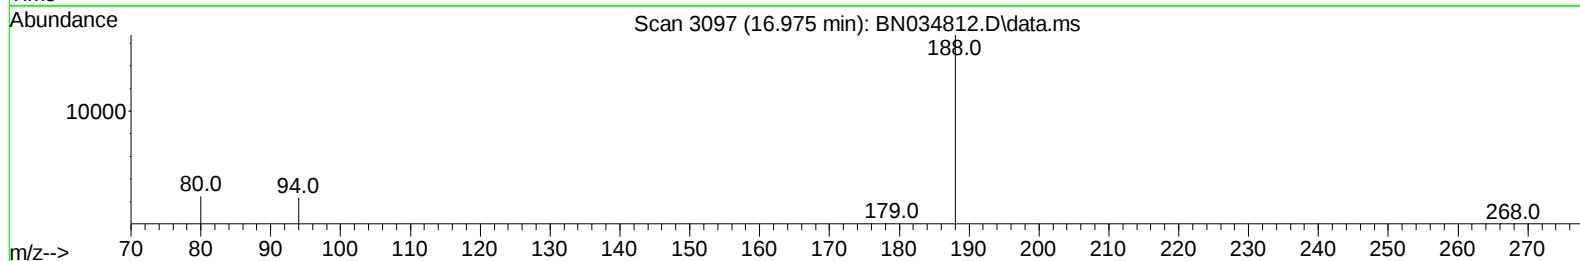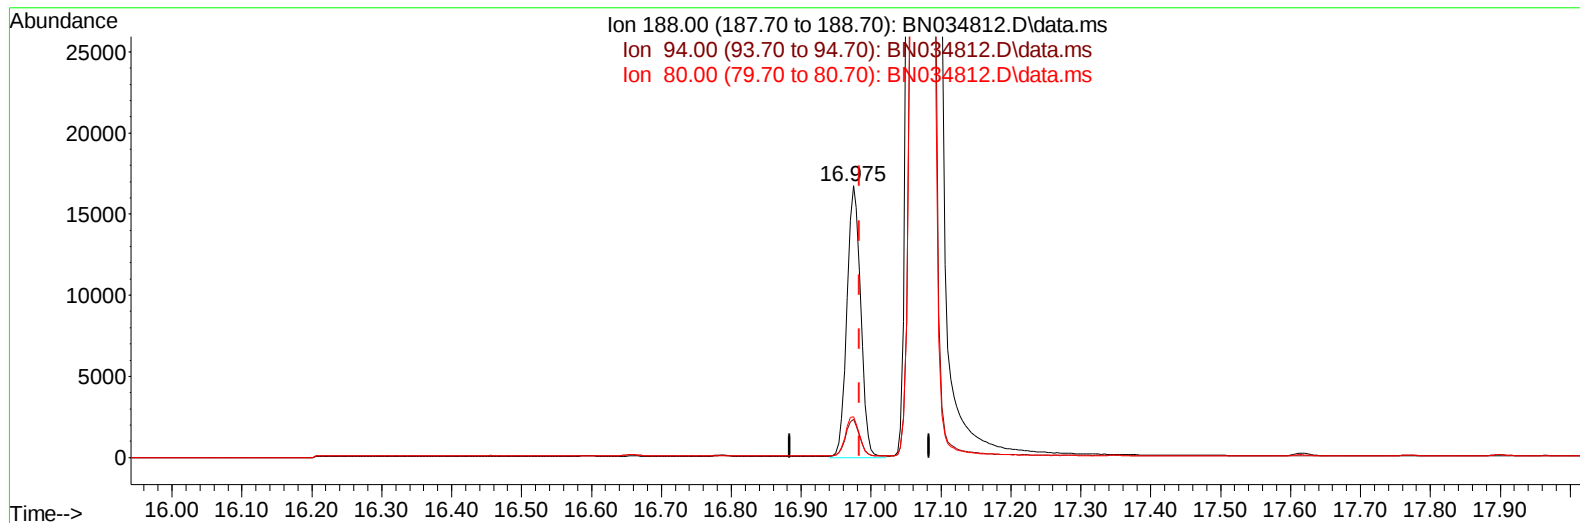

TIC: BN034812.D\data.ms

(13) Phenanthrene-d10 (I)

16.975min (-0.009) 0.40 ng/u1 m

response 22721

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.60	14.11
80.00	14.50	14.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034812.D
Acq On : 01 Nov 2024 19:36
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L63

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

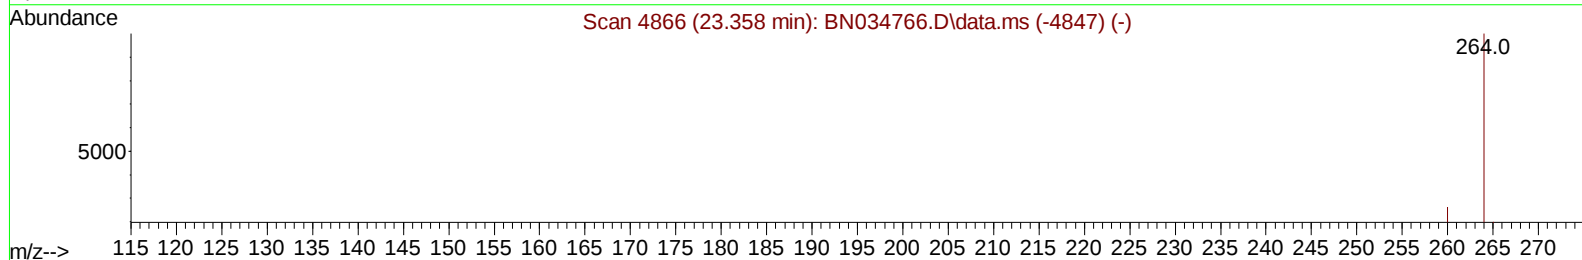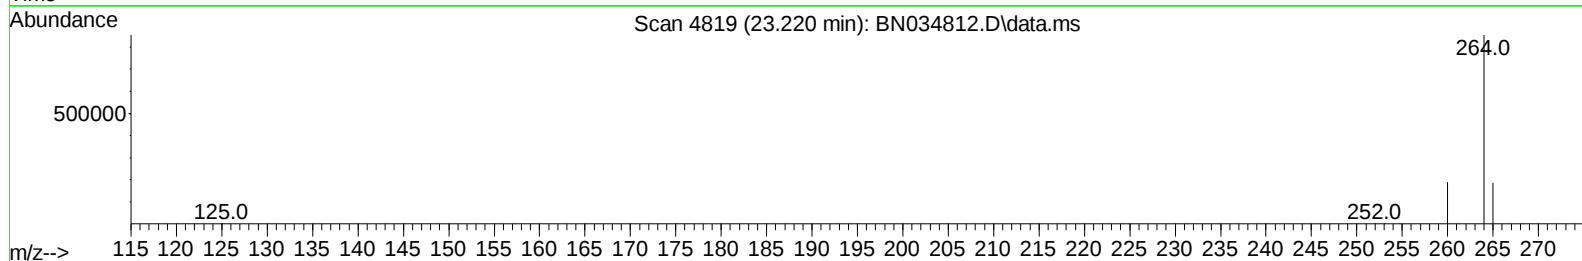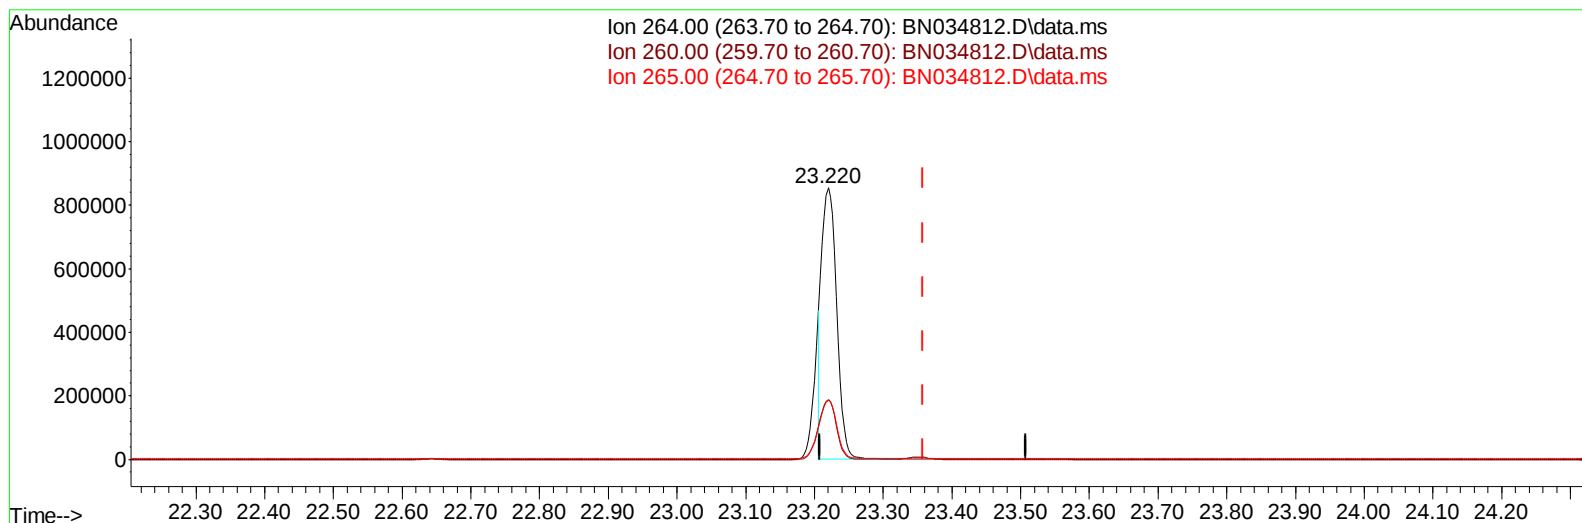

TIC: BN034812.D\data.ms

(23) Perylene-d12 (I)

23.220min (-0.138) 0.40 ng/u1

response 1312708

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	22.01#
265.00	57.90	21.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034812.D
Acq On : 01 Nov 2024 19:36
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L63

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

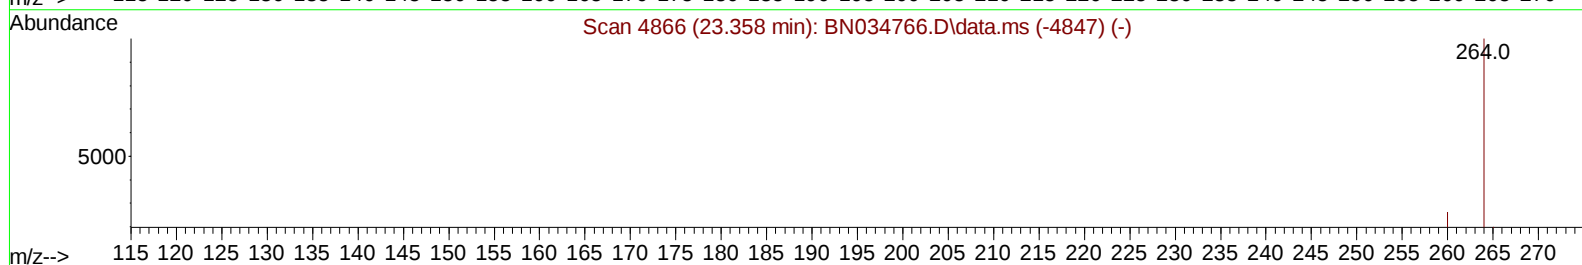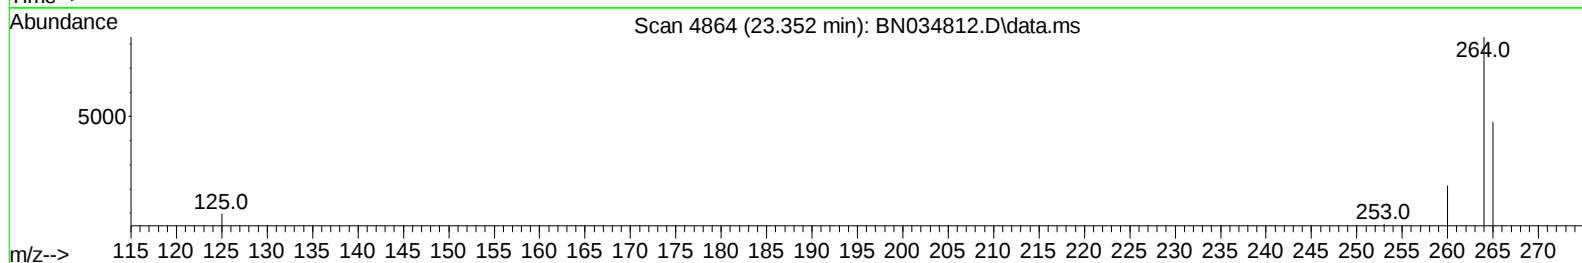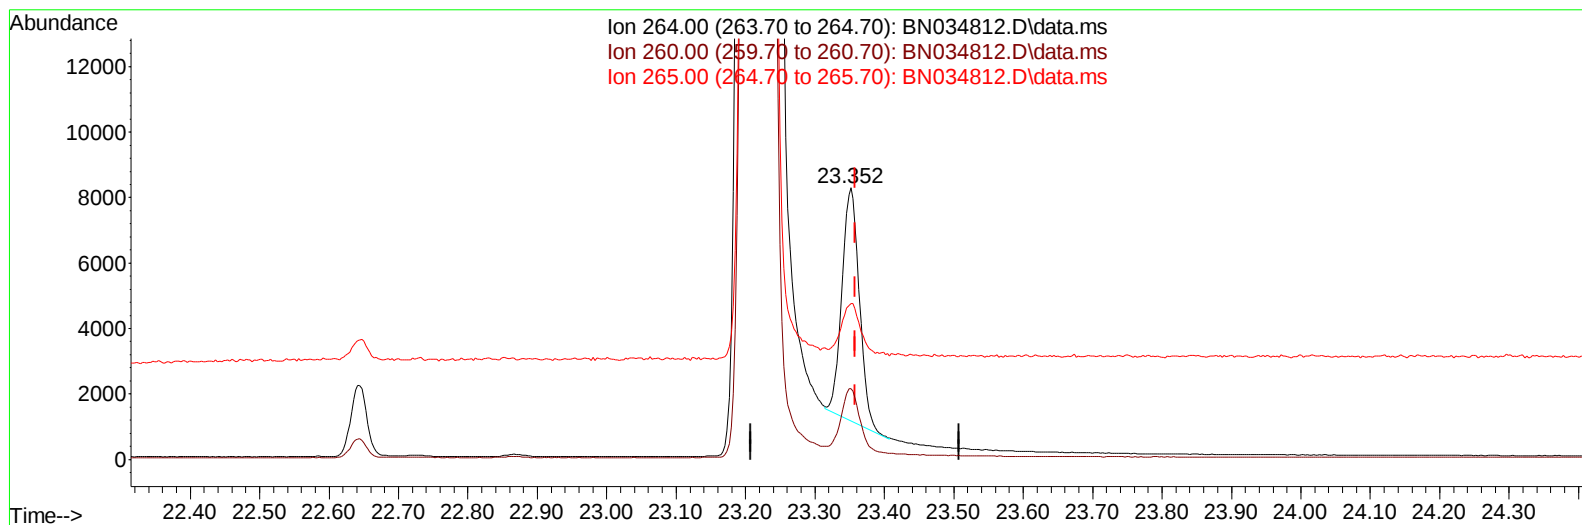

TIC: BN034812.D\data.ms

(23) Perylene-d12 (I)

23.352min (-0.006) 0.40 ng/ul m

response 12367

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	25.99
265.00	57.90	57.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034812.D
 Acq On : 01 Nov 2024 19:36
 Operator : RC/JU
 Sample : P4534-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L63

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:27:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	6530	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	19933	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	11249	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	22721m	0.400	ng/ul	0.00
17) Chrysene-d12	21.168	240	15537	0.400	ng/ul	0.00
23) Perylene-d12	23.352	264	12367m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	39078	5.781	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.955	152	10175	0.407	ng/ul	-0.01
18) Fluoranthene-d10	19.004	212	26805	0.530	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034812.D
Acq On : 01 Nov 2024 19:36
Operator : RC/JU
Sample : P4534-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L63

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:27:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

