




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034821.D
 Acq On : 02 Nov 2024 01:37
 Operator : RC/JU
 Sample : P4534-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L84

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:29:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

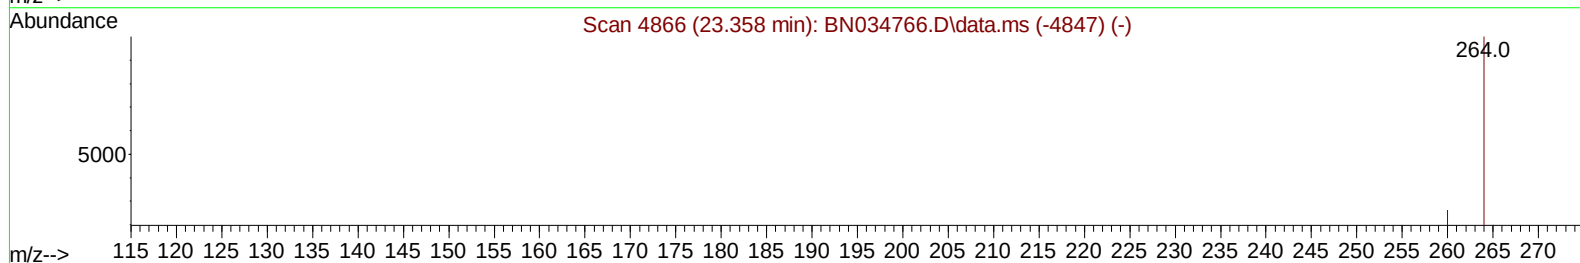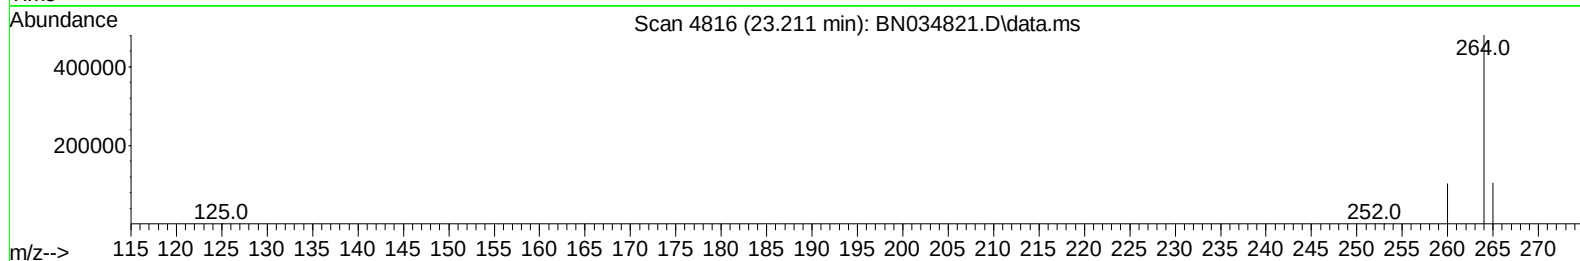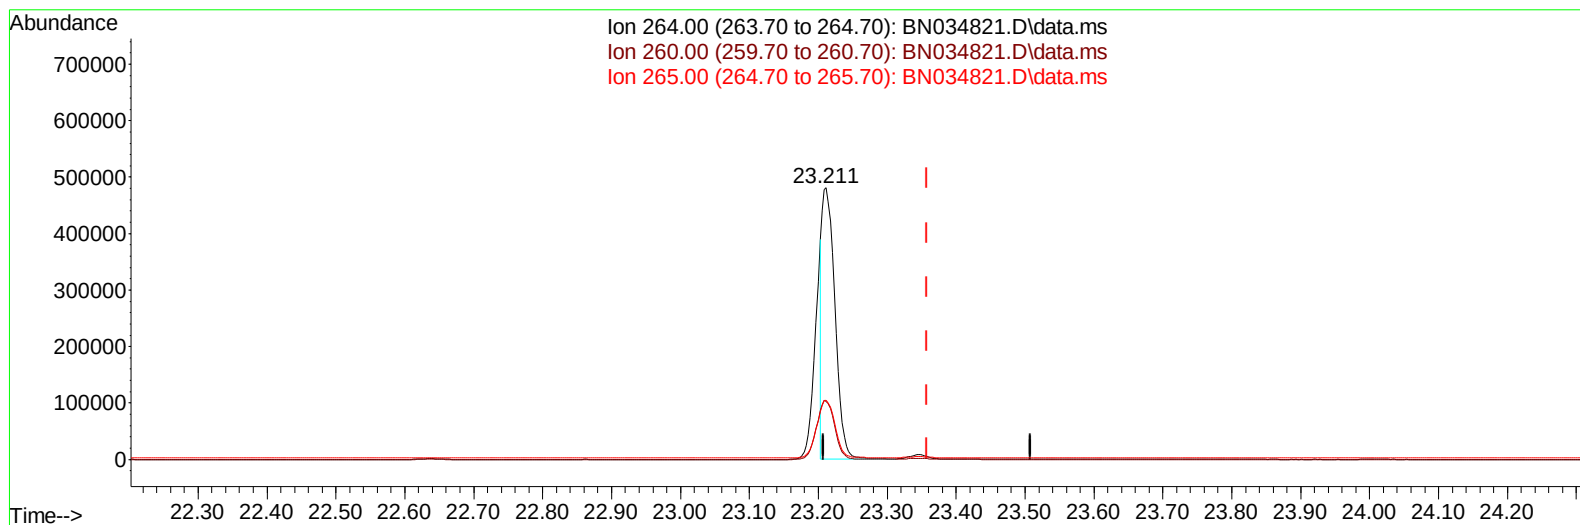

TIC: BN034821.D\data.ms

(23) Perylene-d12 (I)

23.211min (-0.146) 0.40 ng/u1

response 629472

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	21.45#
265.00	57.90	21.94#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034821.D
Acq On : 02 Nov 2024 01:37
Operator : RC/JU
Sample : P4534-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L84

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:29:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

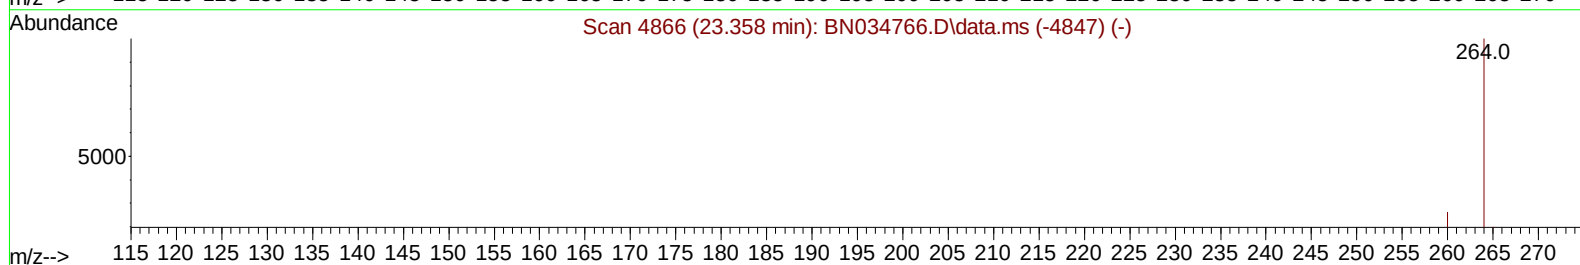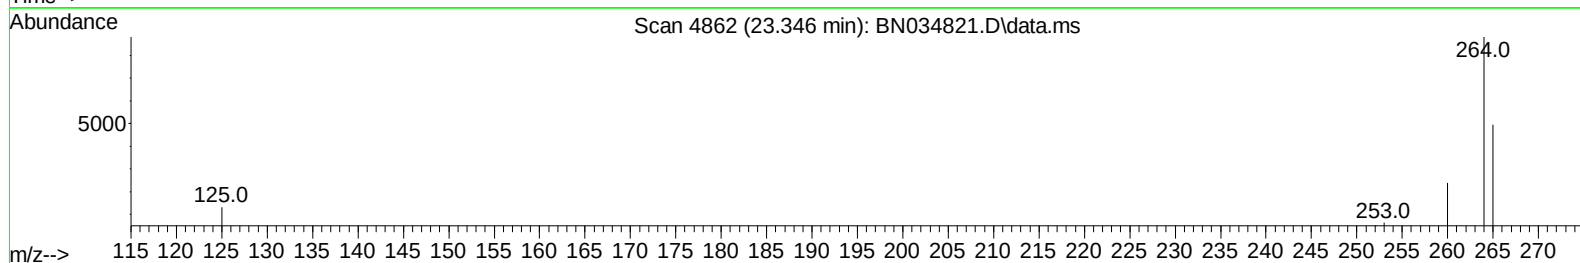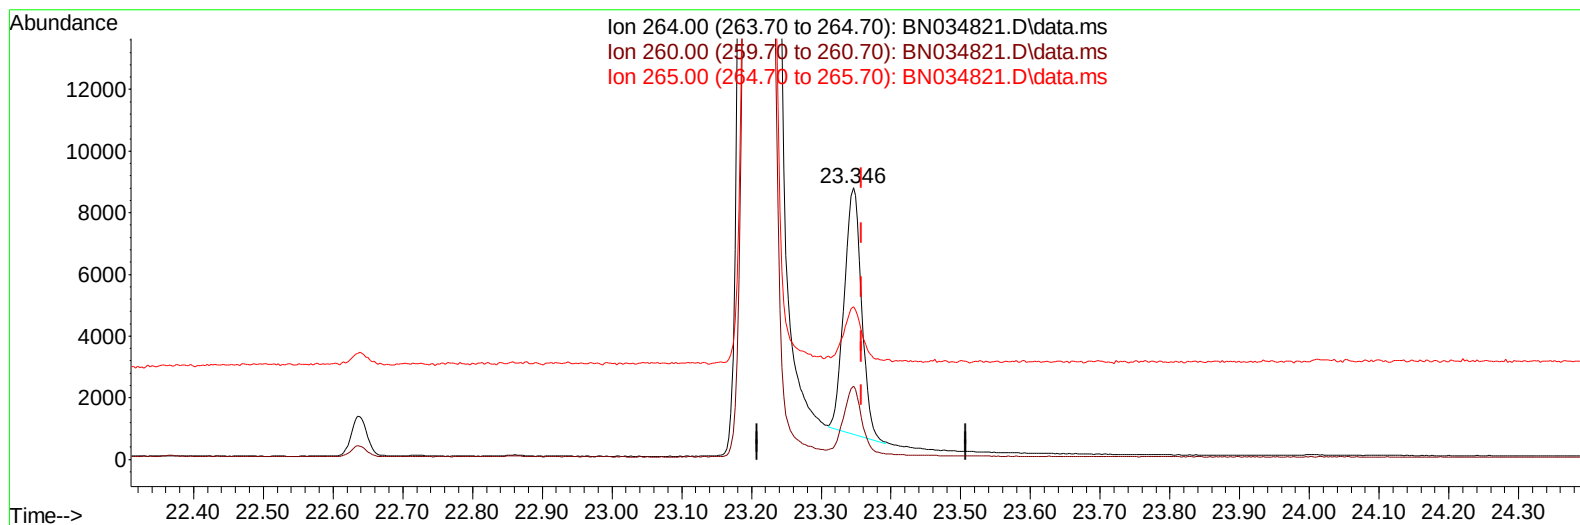

TIC: BN034821.D\data.ms

(23) Perylene-d12 (I)

23.346min (-0.012) 0.40 ng/ul m

response 13789

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	27.00
265.00	57.90	56.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034821.D
 Acq On : 02 Nov 2024 01:37
 Operator : RC/JU
 Sample : P4534-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L84

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:29:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	7946	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	24472	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	13716	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	27599	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.166	240	18550	0.400	ng/ul	0.00
23) Perylene-d12	23.346	264	13789m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	27138	3.299	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	8304	0.271	ng/ul	-0.01
18) Fluoranthene-d10	19.004	212	17903	0.297	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034821.D
Acq On : 02 Nov 2024 01:37
Operator : RC/JU
Sample : P4534-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1L84

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:29:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

