




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034829.D
Acq On : 02 Nov 2024 06:26
Operator : RC/JU
Sample : PB164449BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:29:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

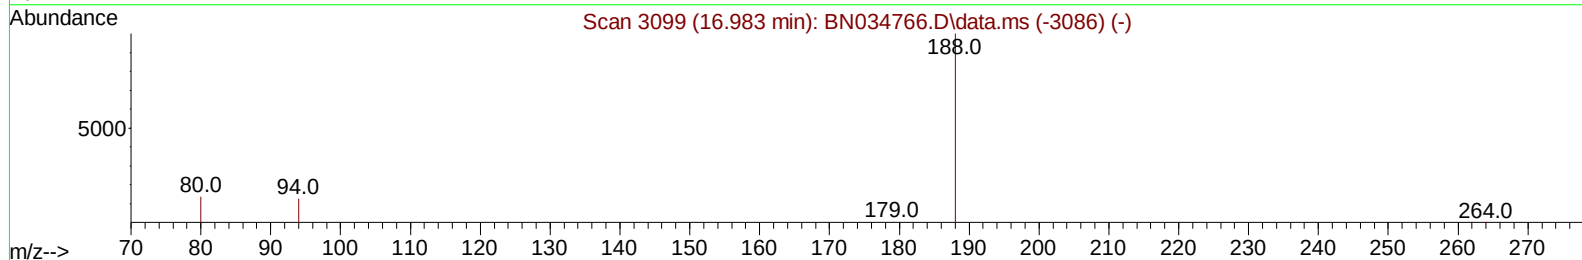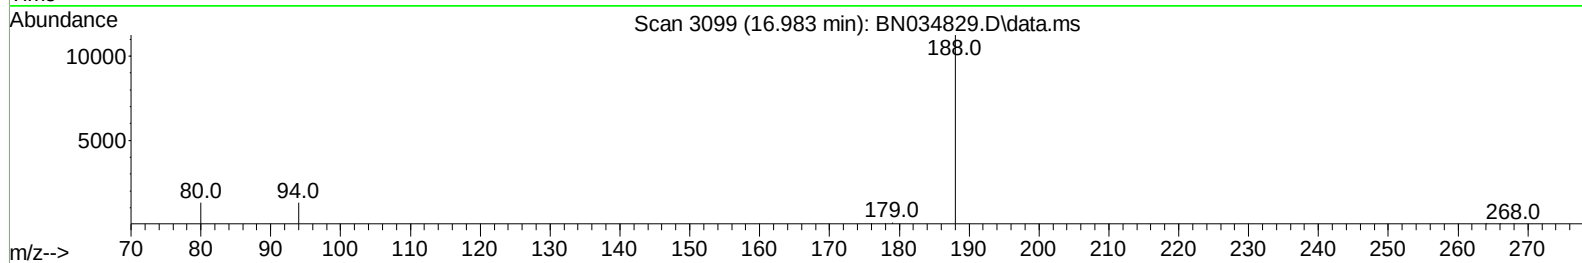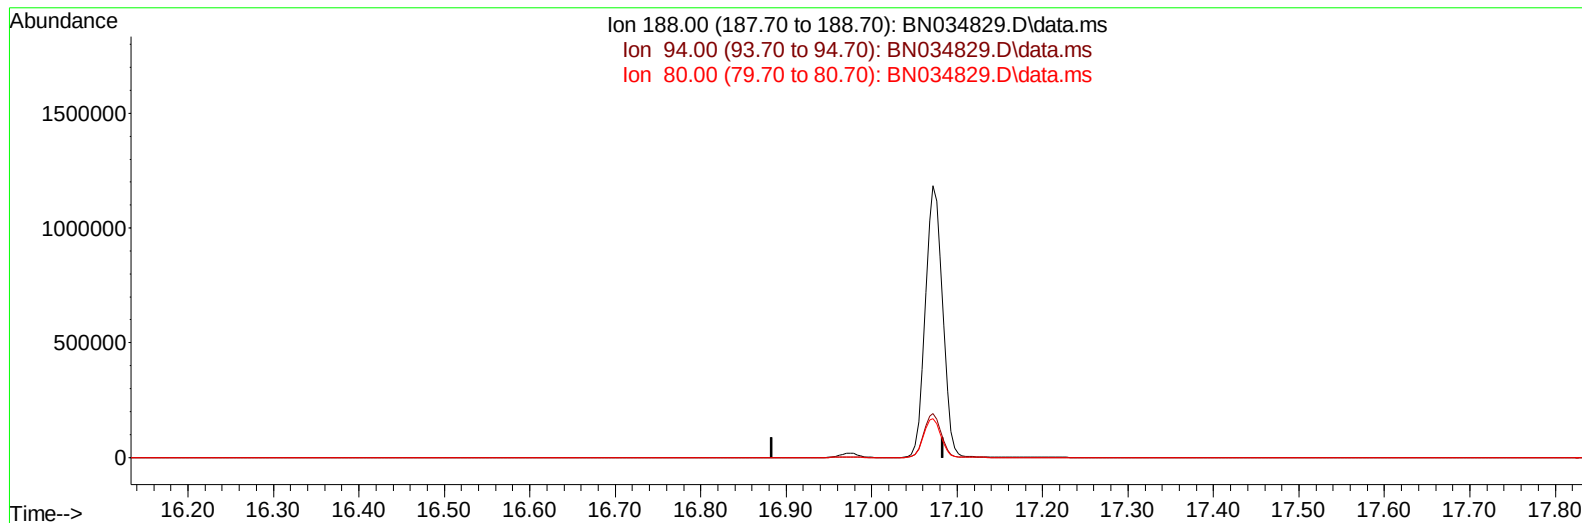

TIC: BN034829.D\data.ms

(13) Phenanthrene-d10 (I)

16.983min (-16.983) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.60	0.00#
80.00	14.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034829.D
Acq On : 02 Nov 2024 06:26
Operator : RC/JU
Sample : PB164449BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:29:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

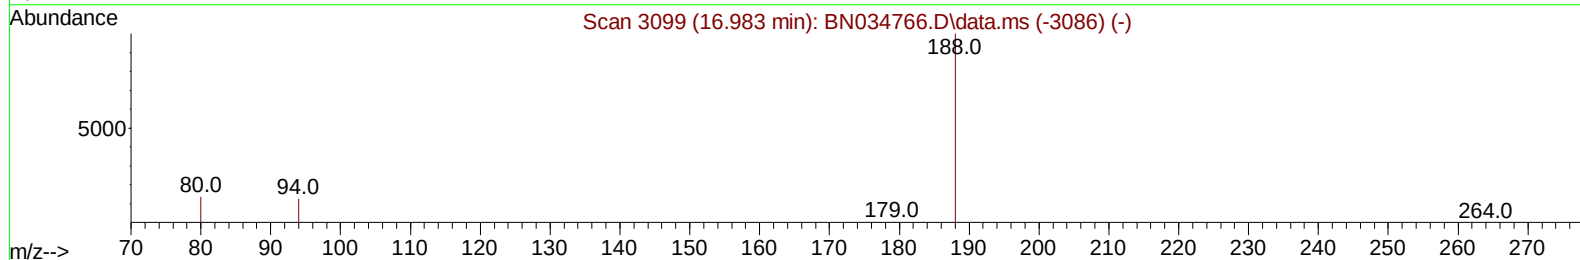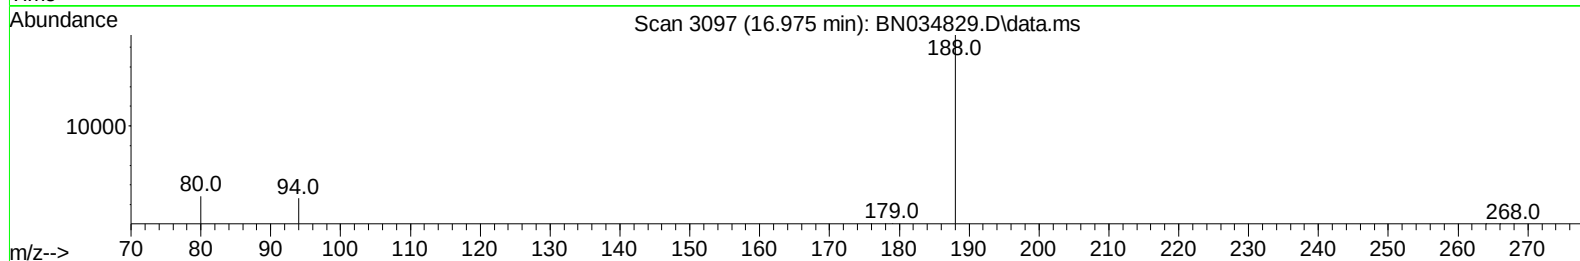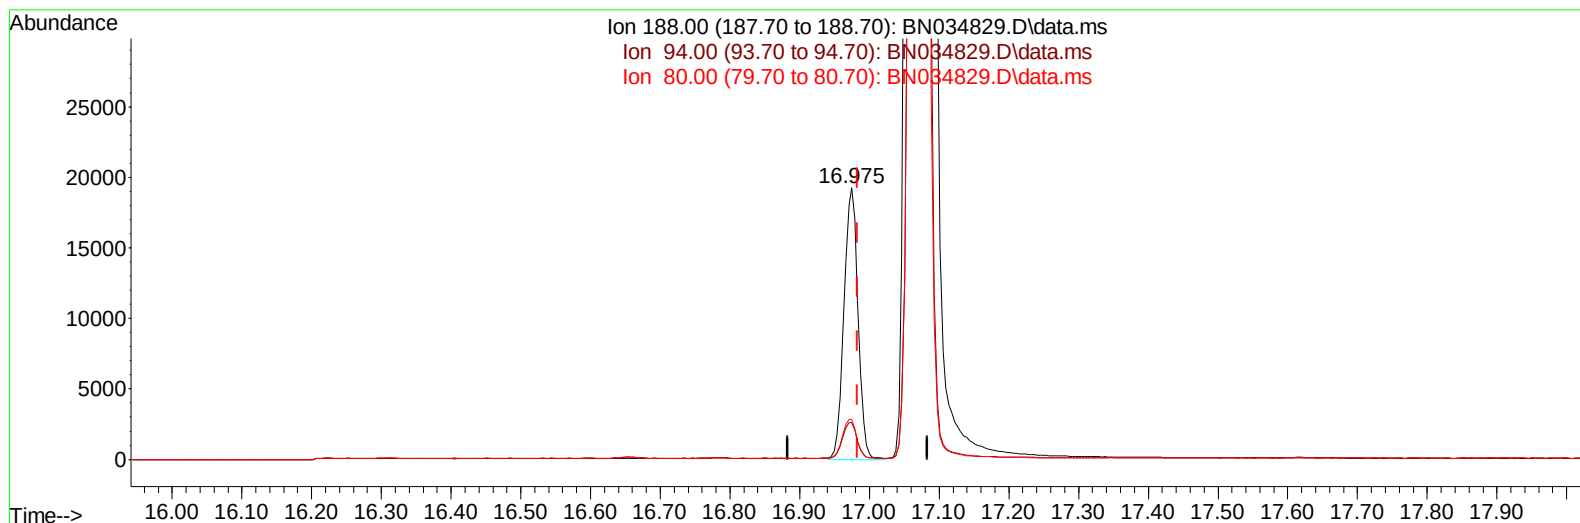

TIC: BN034829.D\data.ms

(13) Phenanthrene-d10 (I)

16.975min (-0.009) 0.40 ng/ul m

response 26894

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.60	13.63
80.00	14.50	14.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034829.D
Acq On : 02 Nov 2024 06:26
Operator : RC/JU
Sample : PB164449BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:29:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

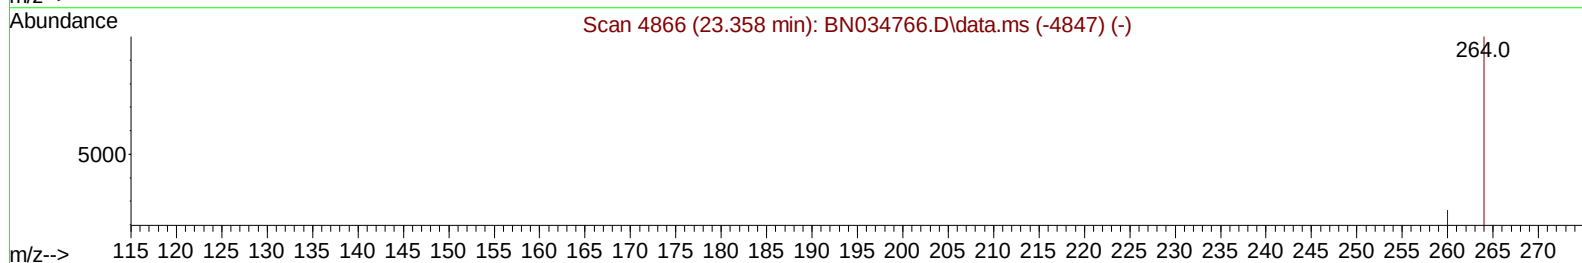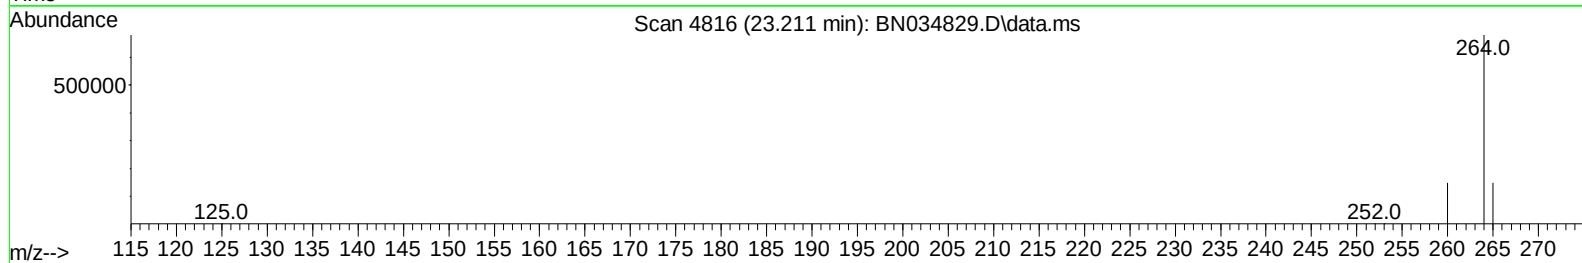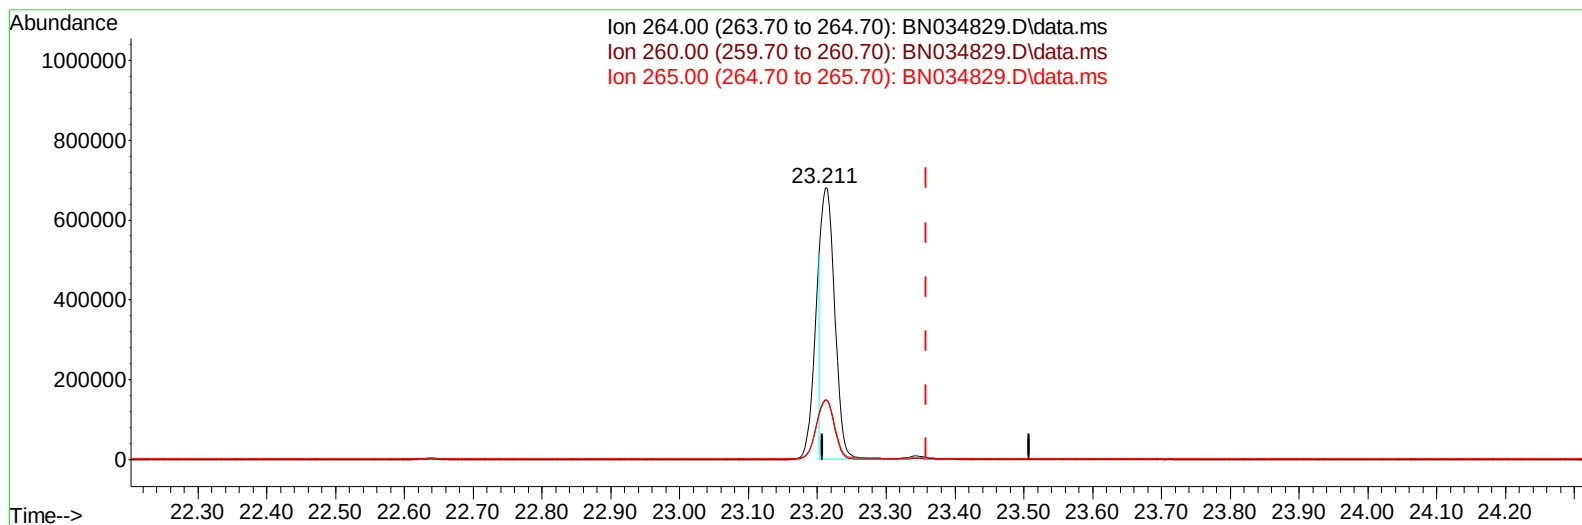

TIC: BN034829.D\data.ms

(23) Perylene-d12 (I)

23.211min (-0.146) 0.40 ng/u1

response 927588

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	21.95#
265.00	57.90	21.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034829.D
Acq On : 02 Nov 2024 06:26
Operator : RC/JU
Sample : PB164449BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:29:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

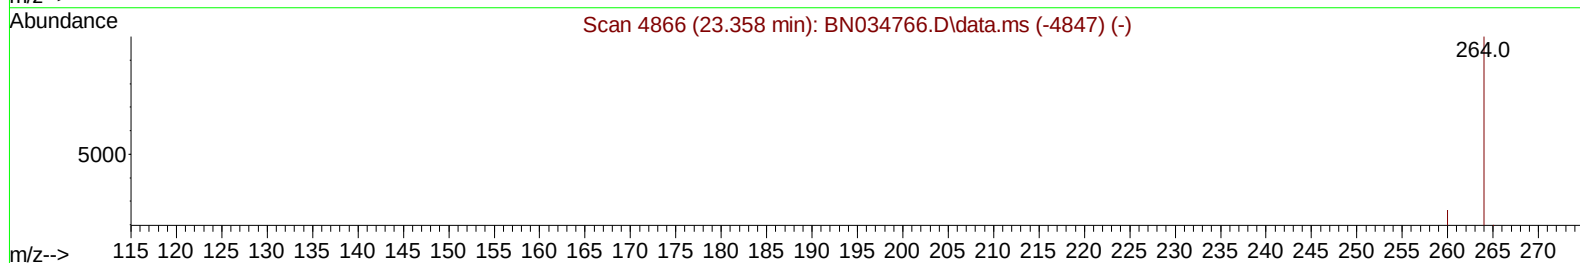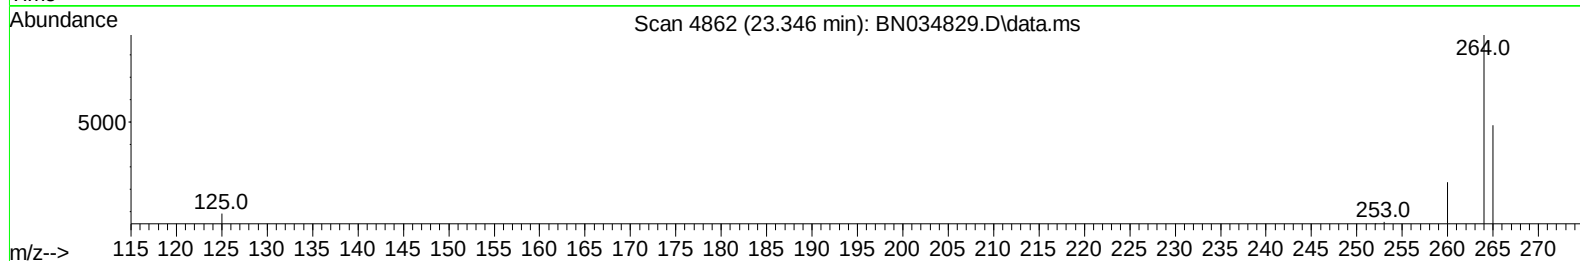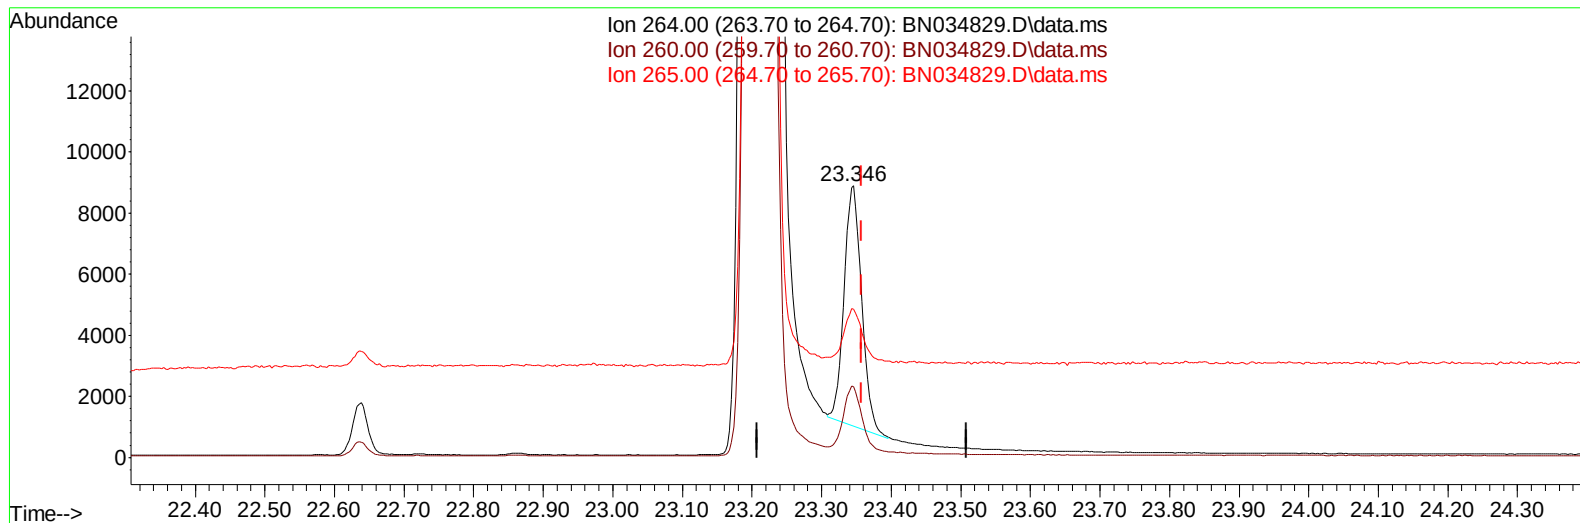

TIC: BN034829.D\data.ms

(23) Perylene-d12 (I)

23.346min (-0.012) 0.40 ng/ul m

response 13752

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.60	25.96
265.00	57.90	54.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034829.D
 Acq On : 02 Nov 2024 06:26
 Operator : RC/JU
 Sample : PB164449BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK449

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:29:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	7761	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	23853	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.226	164	13321	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	26894m	0.400	ng/ul	0.00
17) Chrysene-d12	21.166	240	17173	0.400	ng/ul	0.00
23) Perylene-d12	23.346	264	13752m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	52189	6.496	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	11710	0.392	ng/ul	-0.01
18) Fluoranthene-d10	19.005	212	22514	0.403	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034829.D
Acq On : 02 Nov 2024 06:26
Operator : RC/JU
Sample : PB164449BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK449

Manual IntegrationsAPPROVED

Quant Time: Nov 03 23:29:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

