

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034792.D
 Acq On : 01 Nov 2024 07:31
 Operator : RC/JU
 Sample : P4529-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H35

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:25:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	8085	0.400	ng/ul	0.00
4) Naphthalene-d8	10.367	136	25582	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.231	164	14853	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.979	188	31002m	0.400	ng/ul	0.00
17) Chrysene-d12	21.172	240	21516	0.400	ng/ul	0.00
23) Perylene-d12	23.355	264	17732m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	36235	4.330	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	10017	0.312	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	21155	0.302	ng/ul	0.00
Target Compounds						Qvalue
15) Phenanthrene	17.017	178	2978	0.032	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034792.D
Acq On : 01 Nov 2024 07:31
Operator : RC/JU
Sample : P4529-14
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F7H35

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024


Quant Time: Nov 03 23:25:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

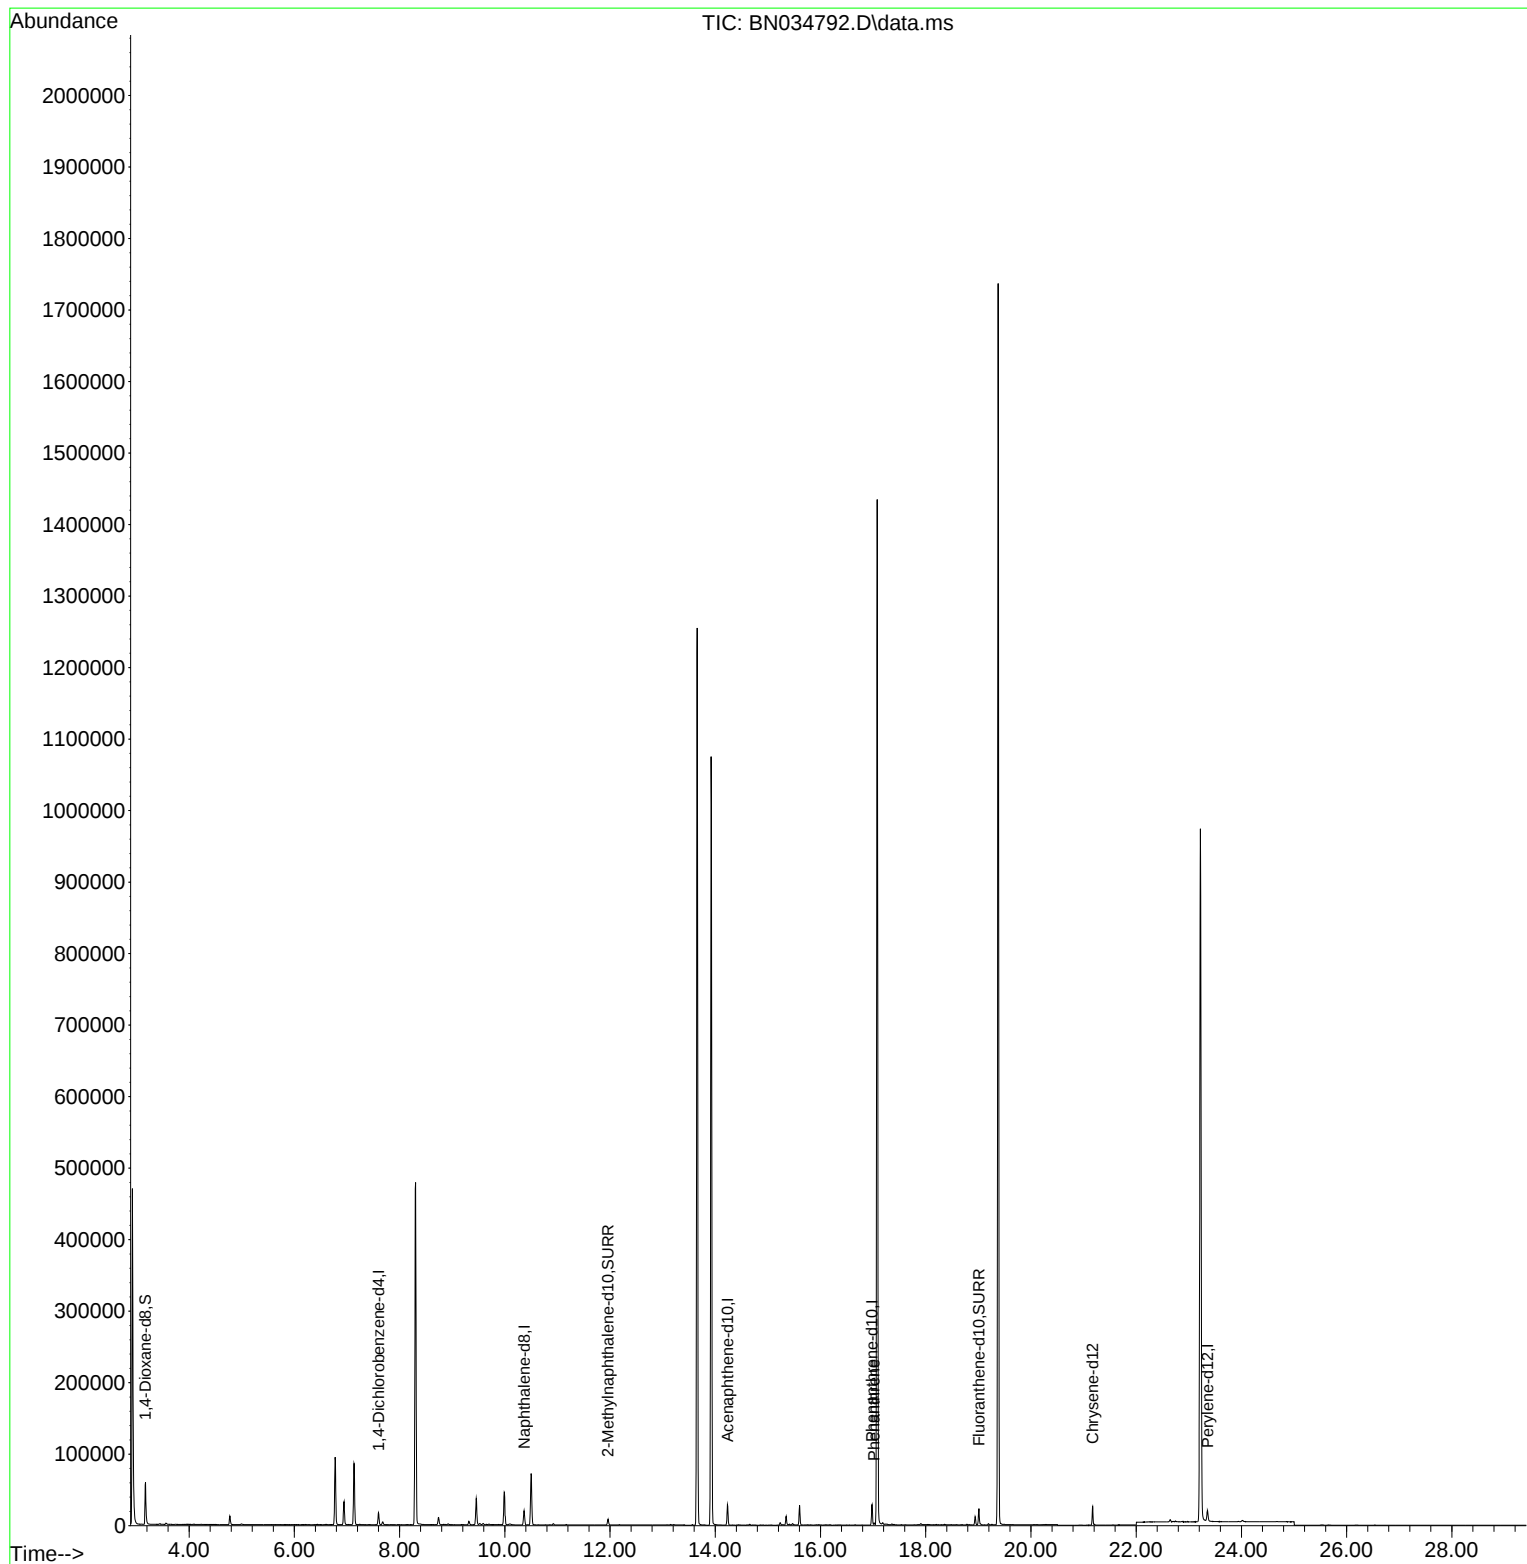

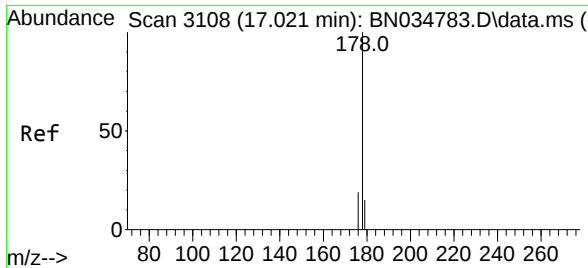

#15
 Phenanthrene
 Concen: 0.032 ng/ul
 RT: 17.017 min Scan# 3107
 Delta R.T. -0.008 min
 Lab File: BN034792.D
 Acq: 01 Nov 2024 07:31

Instrument :
 BNA_N
 ClientSampleId :
 F7H35

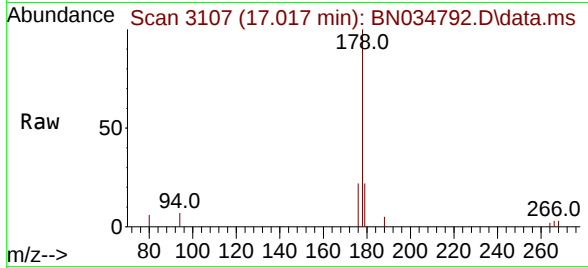

Tgt Ion:	178	Resp:	2978
Ion	Ratio	Lower	Upper
178	100		
179	22.4	12.4	18.6
176	22.1	15.4	23.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

