

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034794.D
 Acq On : 01 Nov 2024 08:44
 Operator : RC/JU
 Sample : P4529-16
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H37

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:25:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.600	152	9752	0.400	ng/u1	0.00
4) Naphthalene-d8	10.366	136	31272	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.231	164	17992	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.979	188	36126m	0.400	ng/u1	0.00
17) Chrysene-d12	21.169	240	24194	0.400	ng/u1	0.00
23) Perylene-d12	23.352	264	18721m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	60483	5.991	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.961	152	17155	0.437	ng/u1	0.00
18) Fluoranthene-d10	19.009	212	34864	0.443	ng/u1	0.00
Target Compounds						Qvalue
24) Benzo(b)fluoranthene	22.700	252	2183m	0.029	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034794.D
Acq On : 01 Nov 2024 08:44
Operator : RC/JU
Sample : P4529-16
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F7H37

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024


Quant Time: Nov 03 23:25:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

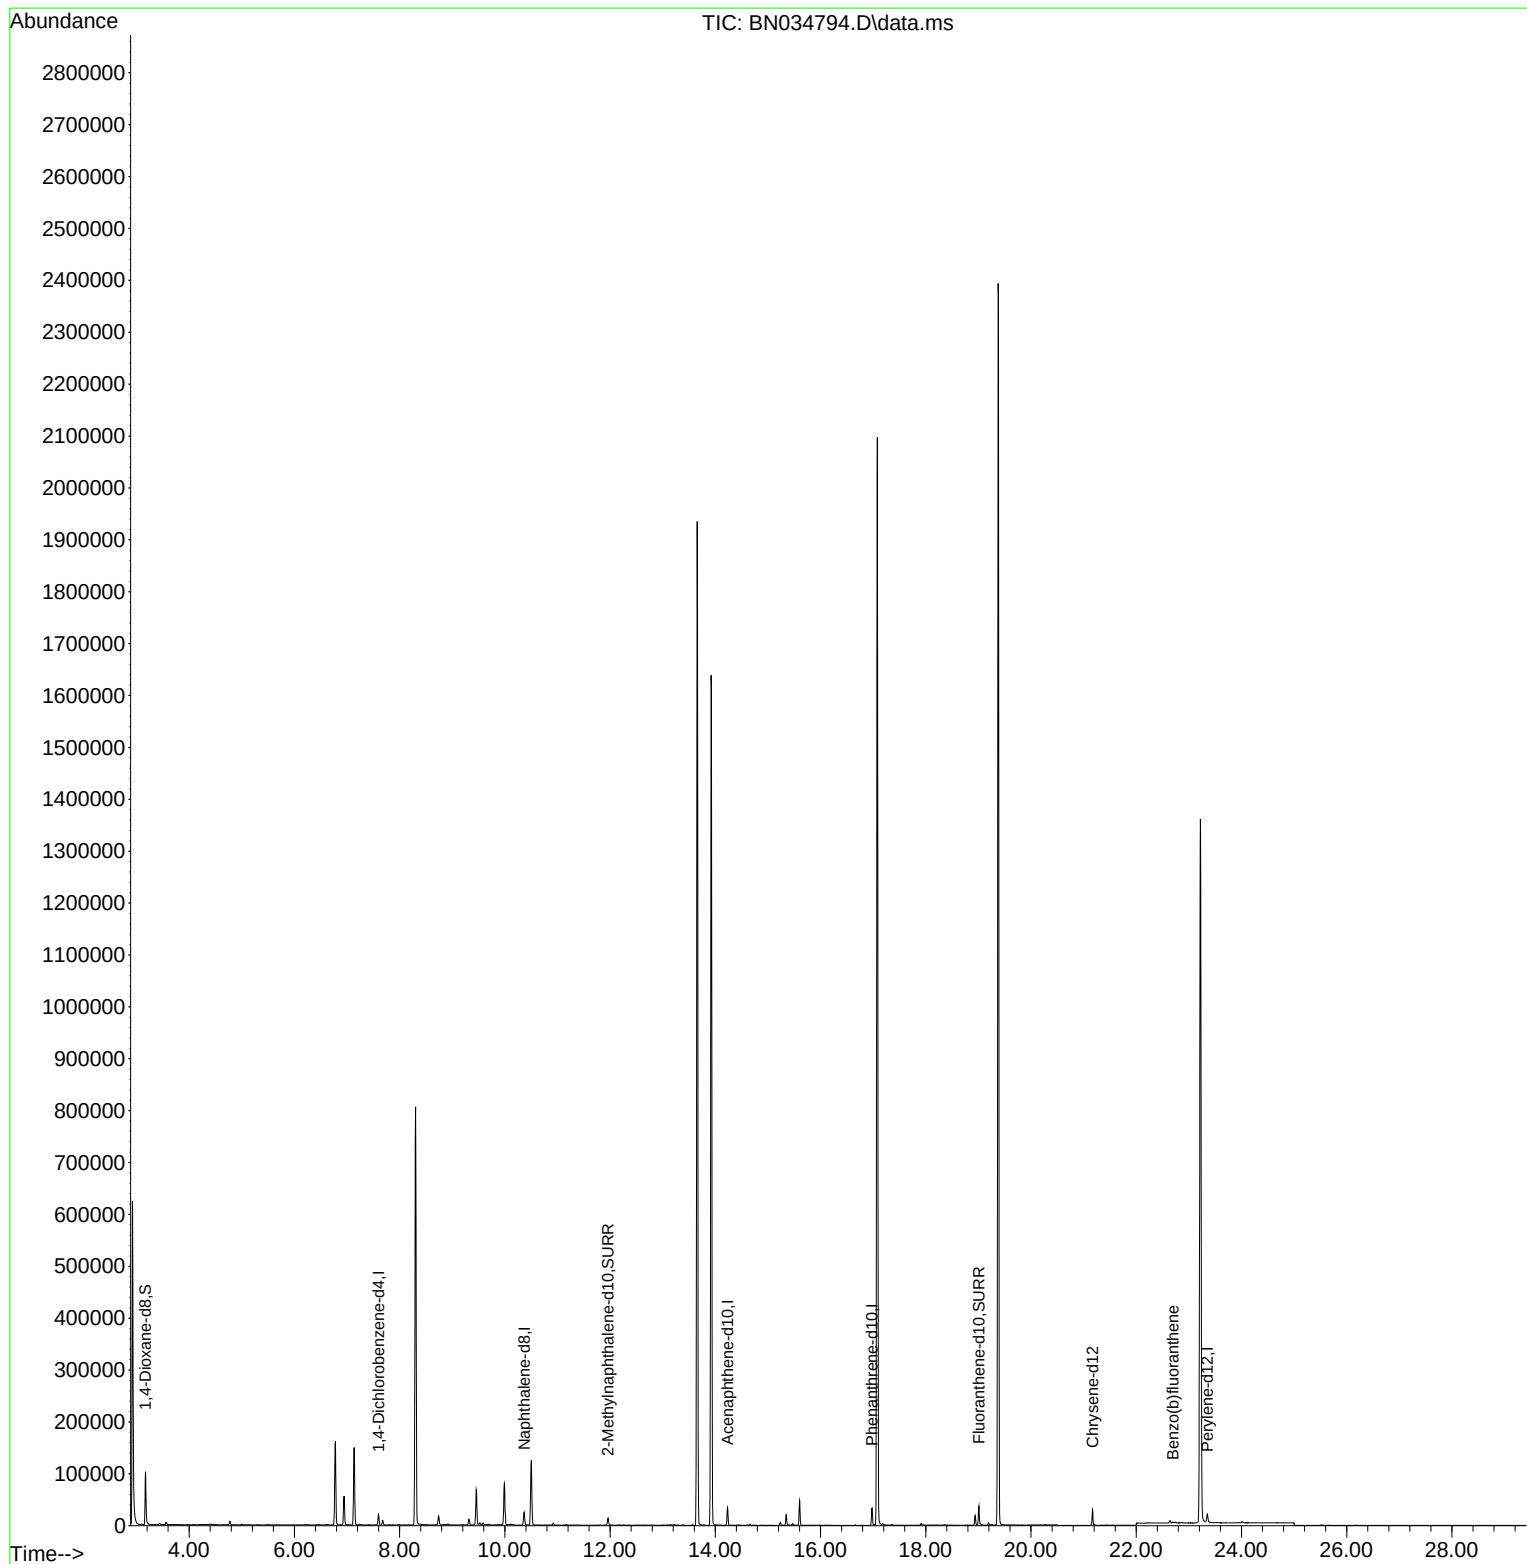

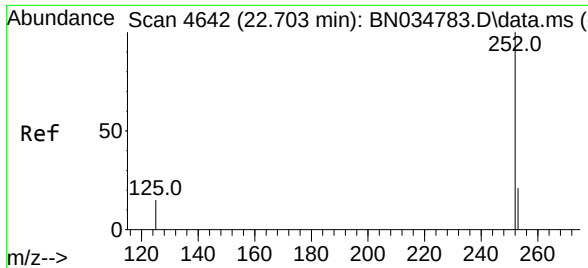

#24
Benzo(b)fluoranthene
Concen: 0.029 ng/ul m
RT: 22.700 min Scan# 4641
Delta R.T. -0.009 min
Lab File: BN034794.D
Acq: 01 Nov 2024 08:44

Instrument :
BNA_N
ClientSampleId :
F7H37

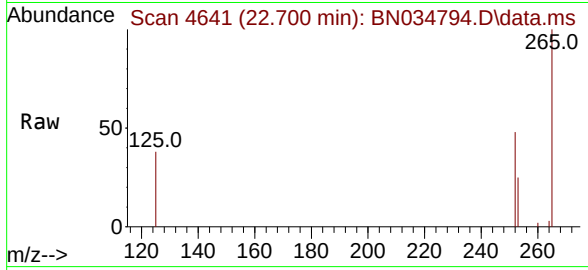

Tgt Ion:252 Resp: 2183
Ion Ratio Lower Upper
252 100
253 51.9 0.0 47.6
125 79.4 0.0 41.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

