

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034804.D
 Acq On : 01 Nov 2024 14:46
 Operator : RC/JU
 Sample : P4530-18
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F7H50

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:26:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	6927	0.400	ng/ul	0.00
4) Naphthalene-d8	10.366	136	21578	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.231	164	12011	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.979	188	24202m	0.400	ng/ul	0.00
17) Chrysene-d12	21.169	240	16086	0.400	ng/ul	0.00
23) Perylene-d12	23.352	264	12785m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	36639	5.110	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	10001	0.370	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	24640	0.471	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.410	128	2113	0.037	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034804.D
Acq On : 01 Nov 2024 14:46
Operator : RC/JU
Sample : P4530-18
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F7H50

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024


Quant Time: Nov 03 23:26:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

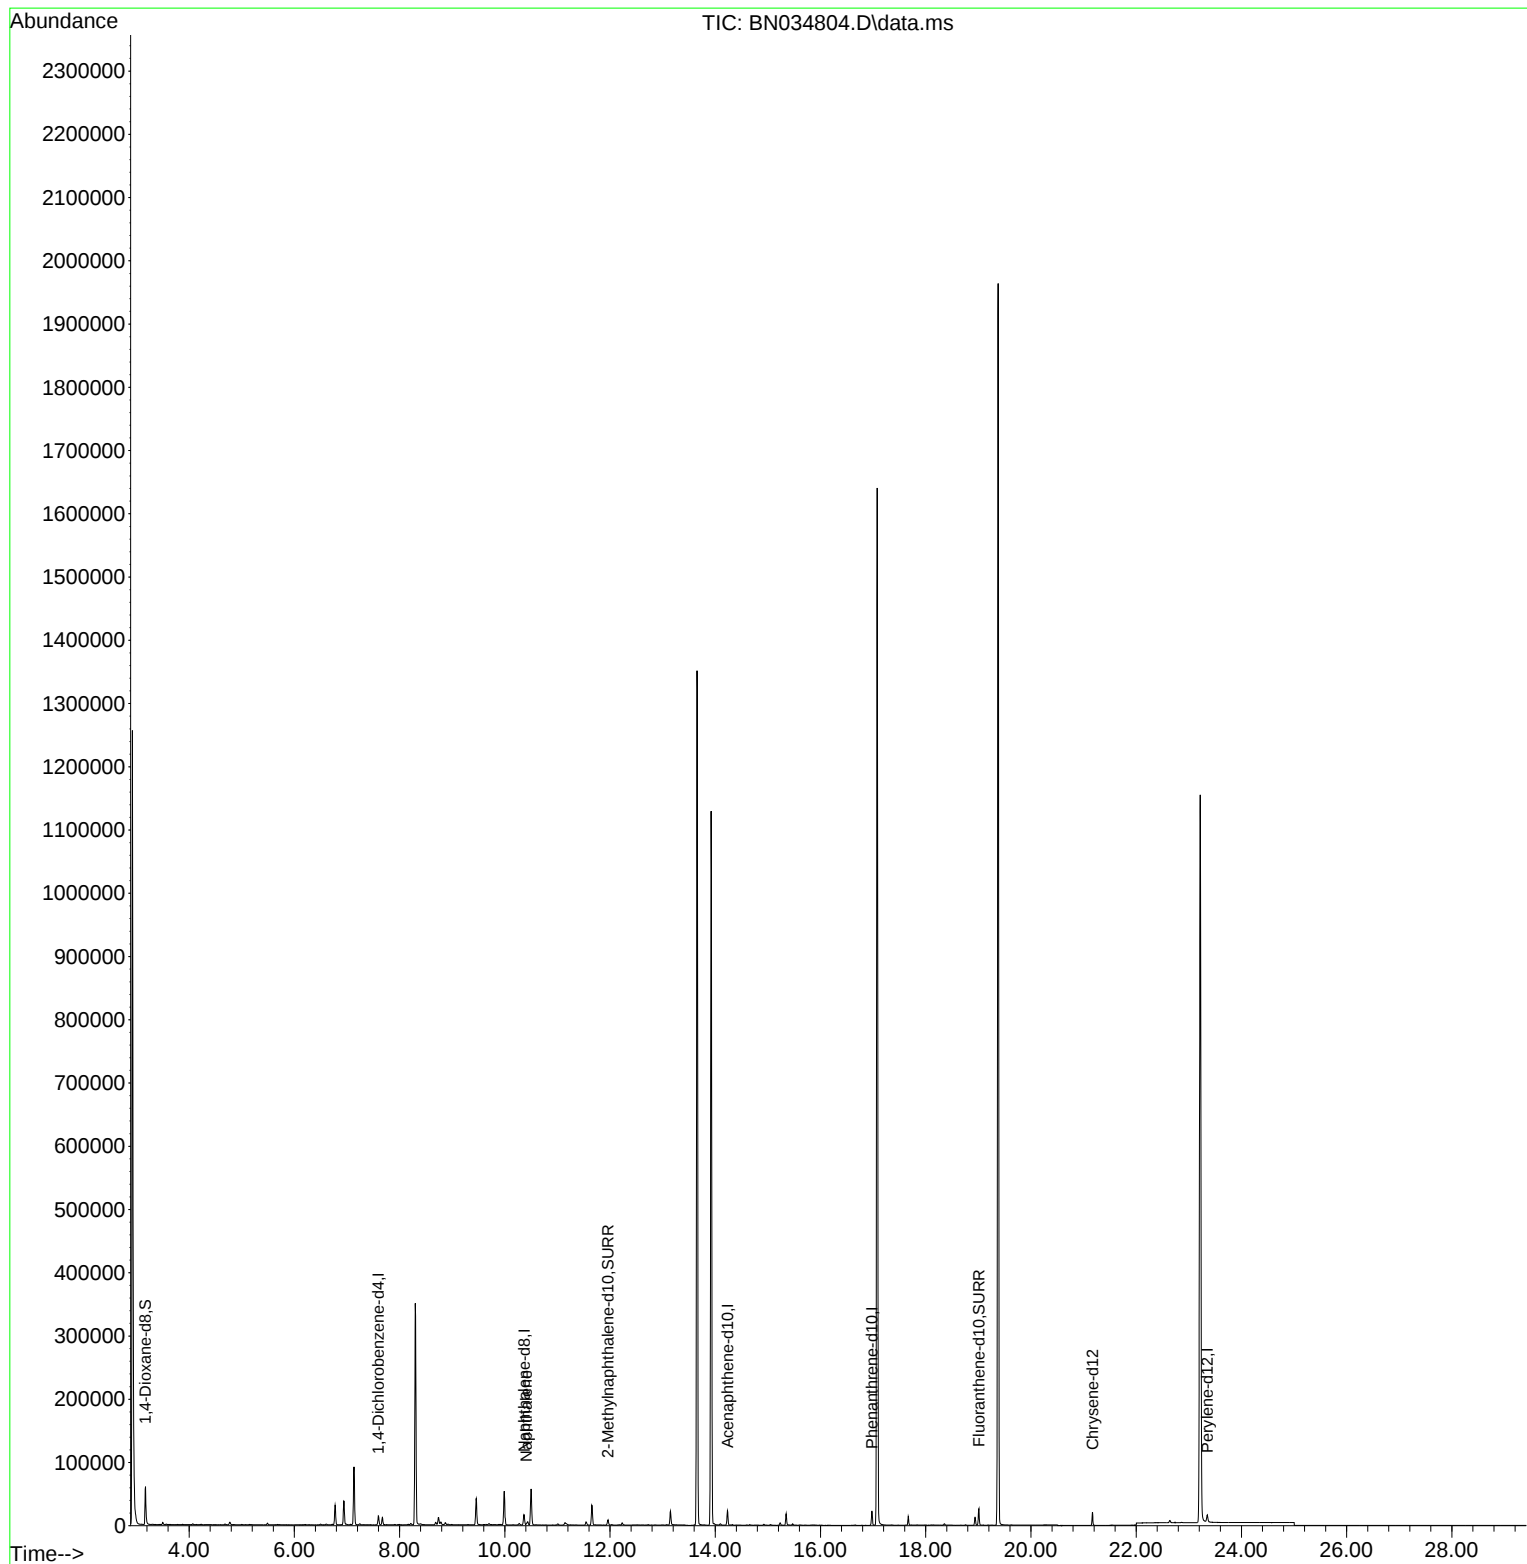

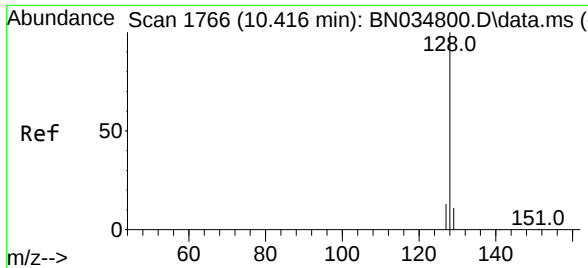

#5
Naphthalene
Concen: 0.037 ng/ul
RT: 10.410 min Scan# 1766
Delta R.T. -0.011 min
Lab File: BN034804.D
Acq: 01 Nov 2024 14:46

Instrument :
BNA_N
ClientSampleId :
F7H50

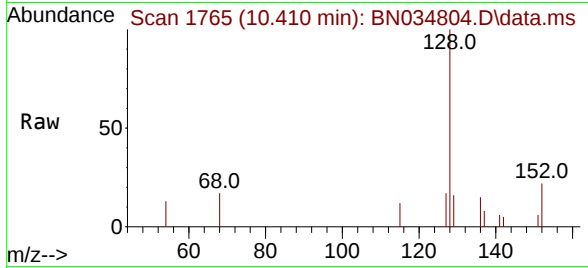

Tgt Ion:128 Resp: 211
Ion Ratio Lower Upper
128 100
129 16.3 9.1 13.7
127 17.3 10.5 15.7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

