

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034810.D
 Acq On : 01 Nov 2024 18:24
 Operator : RC/JU
 Sample : P4558-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L77

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:27:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	7304	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	22370	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	12533	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	26050m	0.400	ng/ul	0.00
17) Chrysene-d12	21.169	240	17891	0.400	ng/ul	0.00
23) Perylene-d12	23.352	264	14823m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.166	96	31004	4.101	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.961	152	10521	0.375	ng/ul	0.00
18) Fluoranthene-d10	19.009	212	23781	0.408	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.203	88	870	0.105	ng/ul#	32

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034810.D
Acq On : 01 Nov 2024 18:24
Operator : RC/JU
Sample : P4558-01
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1L77

Quant Time: Nov 03 23:27:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/04/2024
Supervised By :mohammad ahmed 11/05/2024

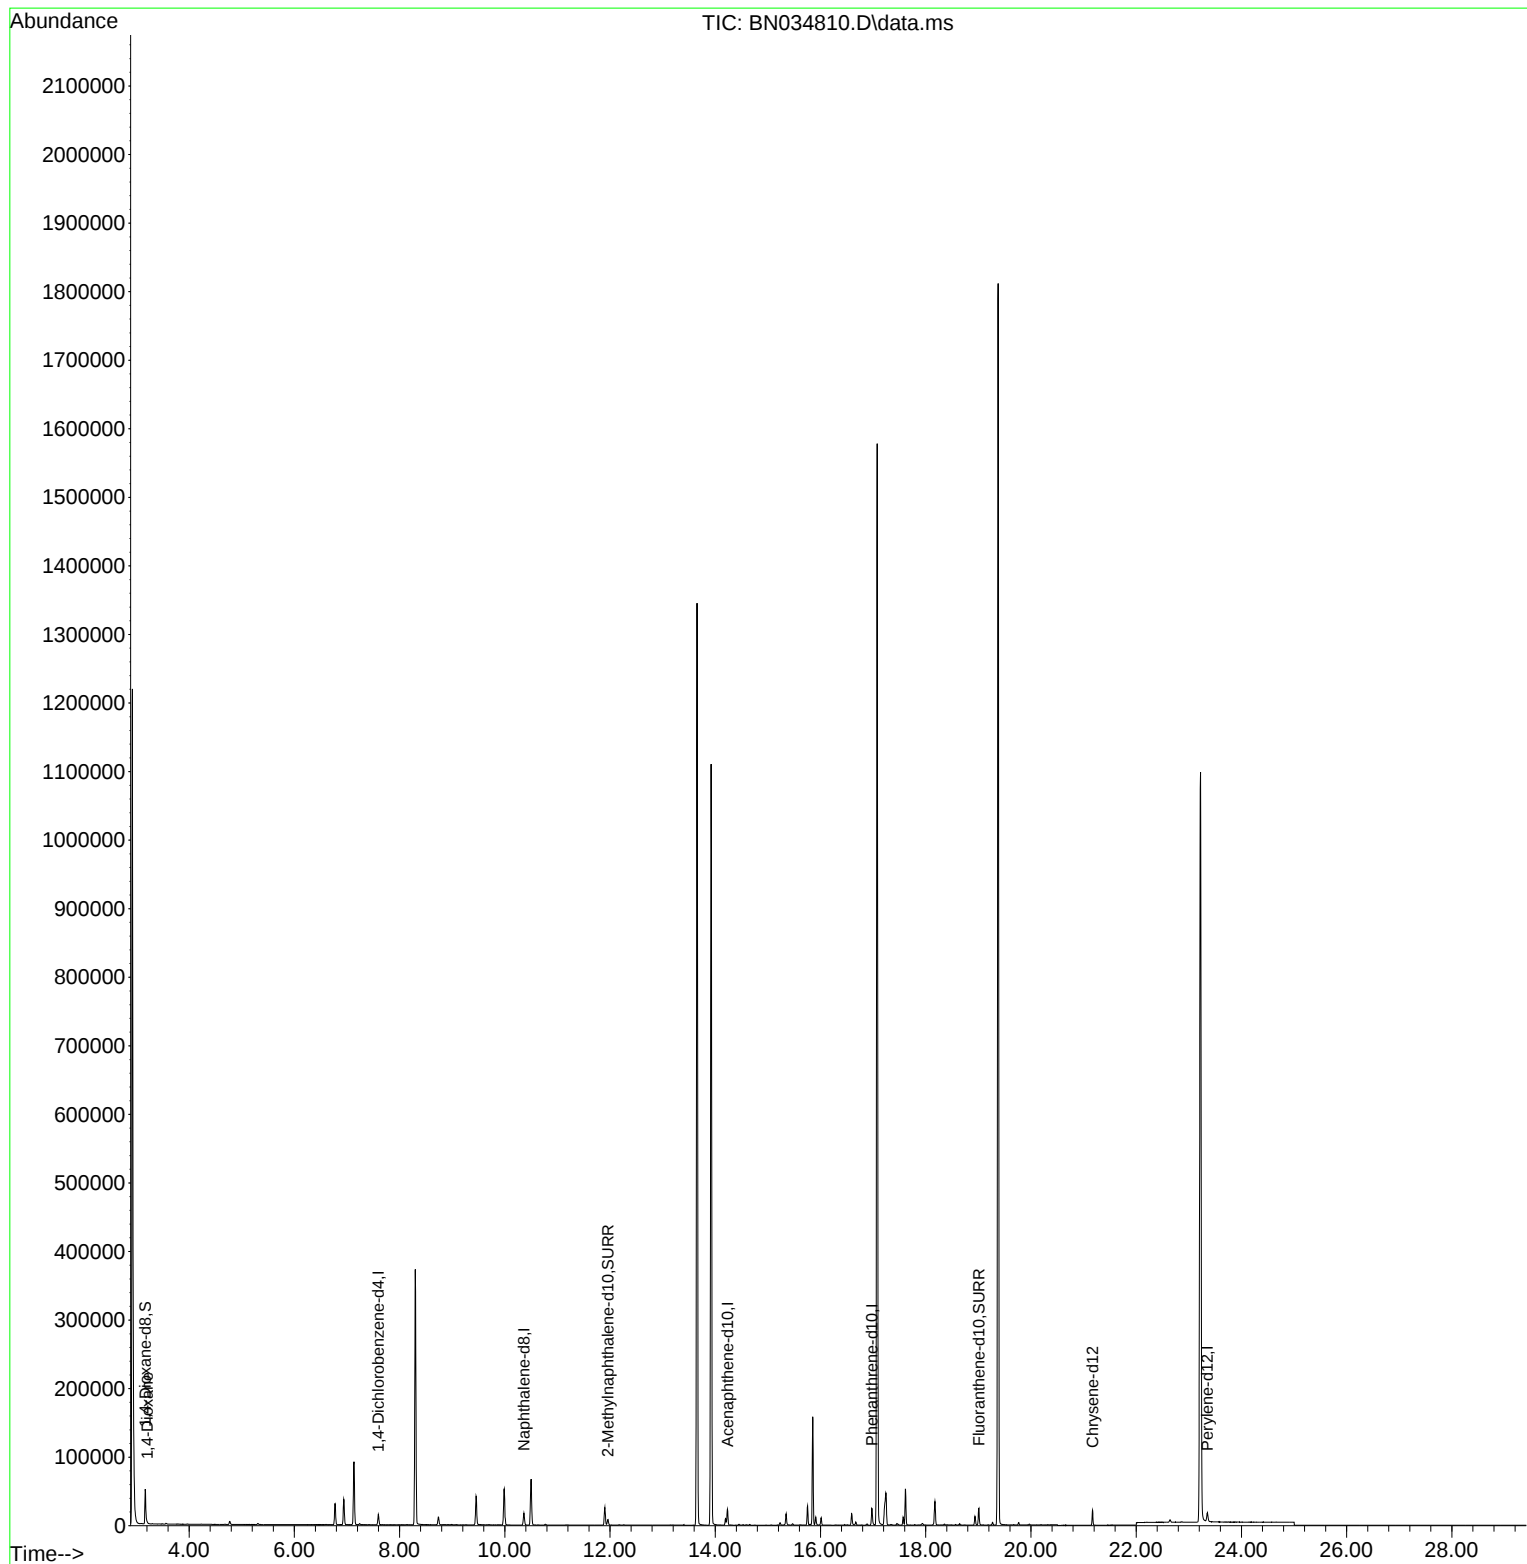

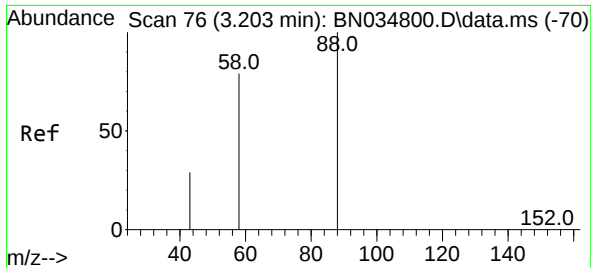

#2
 1,4-Dioxane
 Concen: 0.105 ng/ul
 RT: 3.203 min Scan# 70
 Delta R.T. -0.004 min
 Lab File: BN034810.D
 Acq: 01 Nov 2024 18:24

Instrument :
 BNA_N
 ClientSampleId :
 E1L77

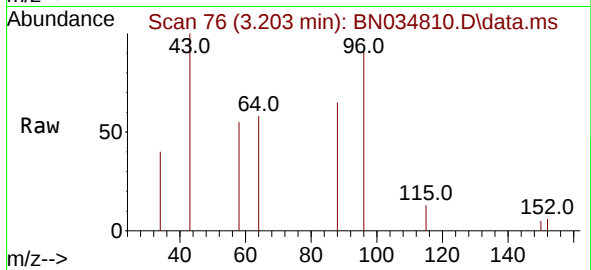

Tgt Ion: 88 Resp: 870

Ion	Ratio	Lower	Upper
88	100		
43	152.7	41.9	62.9
58	83.9	57.5	86.3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

