

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
 Data File : BN034822.D
 Acq On : 02 Nov 2024 02:13
 Operator : RC/JU
 Sample : P4534-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1L86

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

Quant Time: Nov 03 23:29:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 31 11:13:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.596	152	7696	0.400	ng/ul	0.00
4) Naphthalene-d8	10.361	136	22269	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.231	164	12319	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	25102m	0.400	ng/ul	0.00
17) Chrysene-d12	21.166	240	17728	0.400	ng/ul	0.00
23) Perylene-d12	23.346	264	15572m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	32537	4.084	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.956	152	9631	0.345	ng/ul	-0.01
18) Fluoranthene-d10	19.005	212	21117	0.366	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.199	88	278	0.032	ng/ul#	44

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN103124\
Data File : BN034822.D
Acq On : 02 Nov 2024 02:13
Operator : RC/JU
Sample : P4534-14
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1L86

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
Supervised By :mohammad ahmed 11/05/2024


Quant Time: Nov 03 23:29:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 31 11:13:08 2024
Response via : Initial Calibration

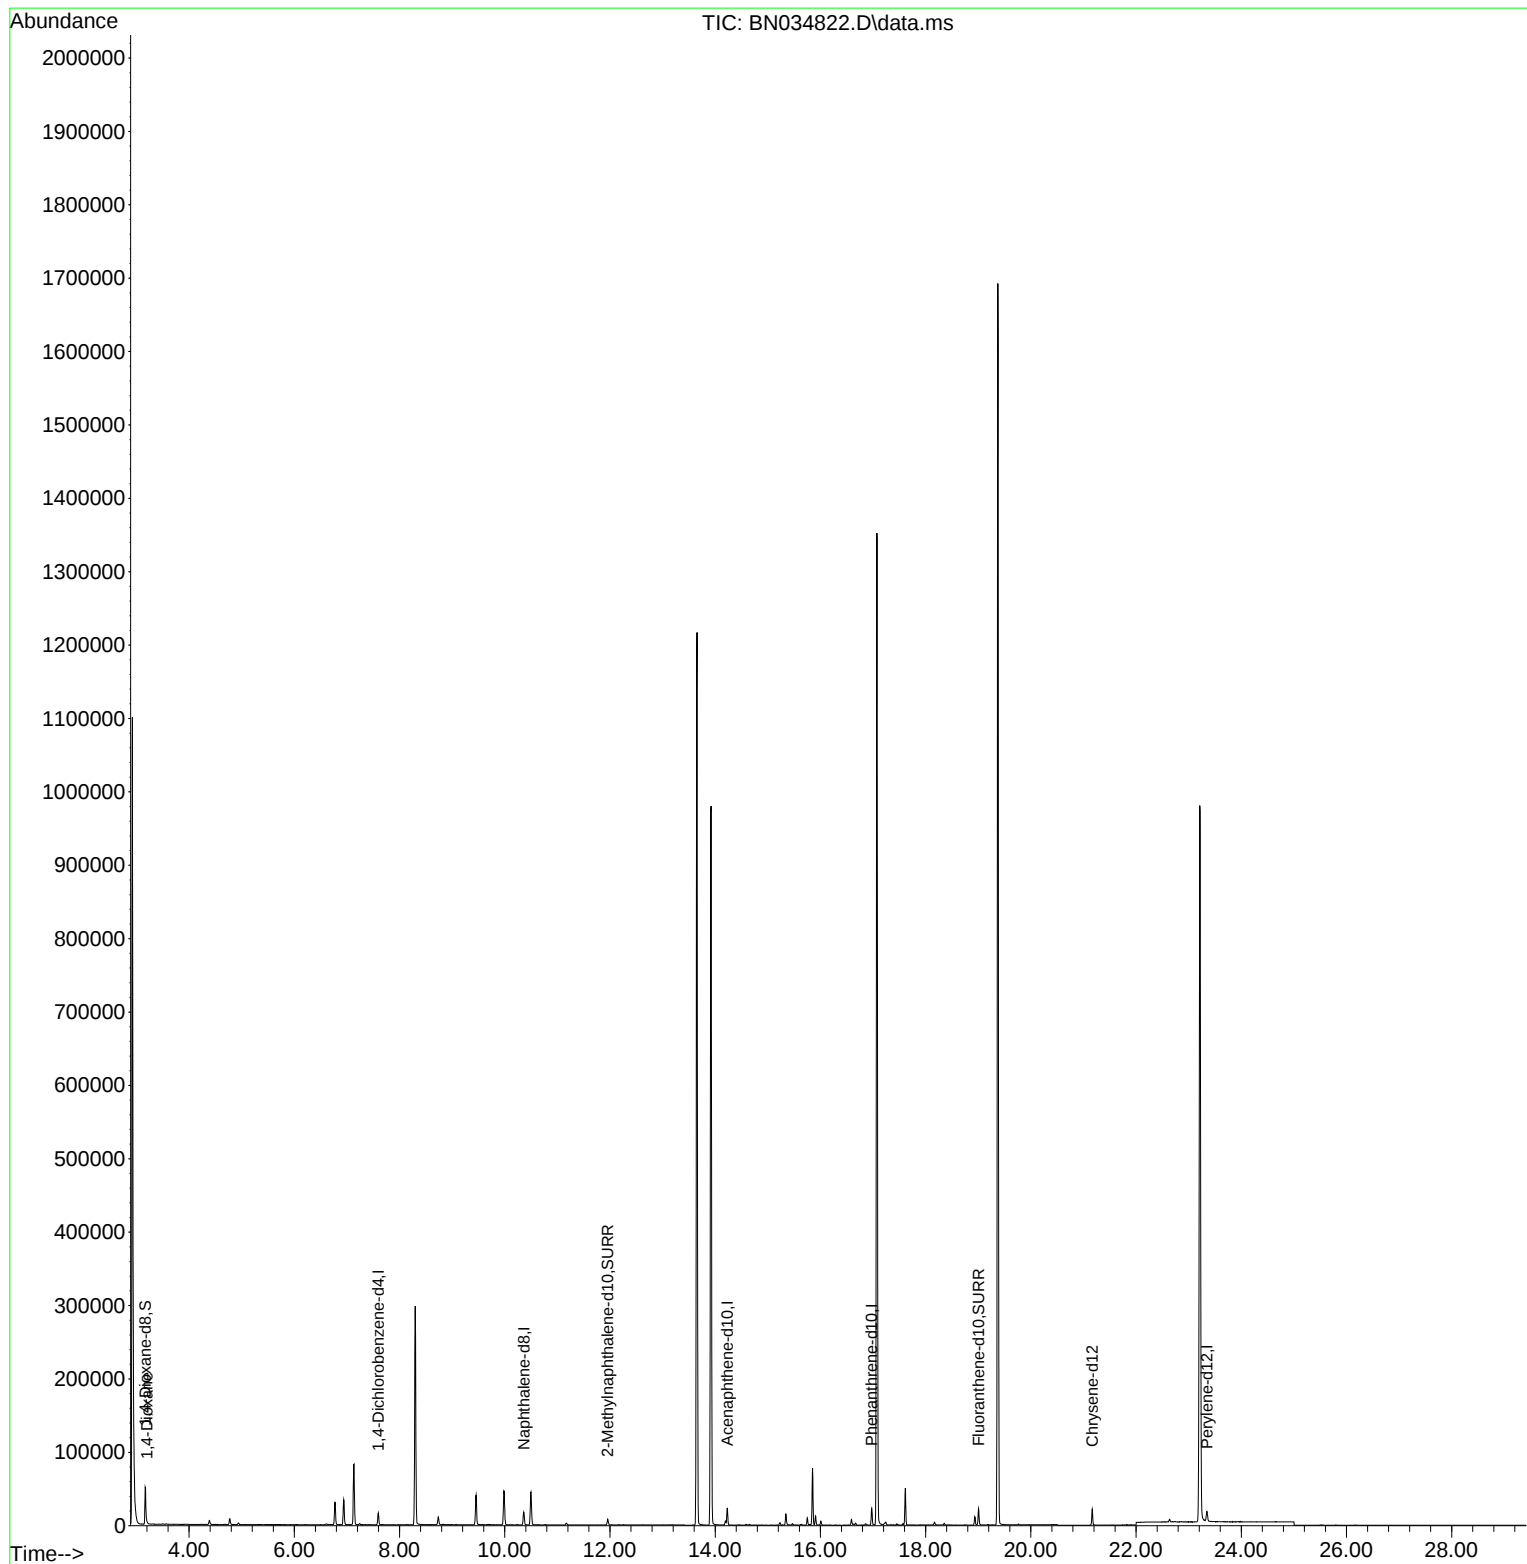

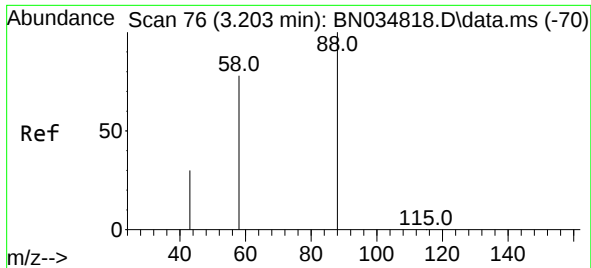

#2
 1,4-Dioxane
 Concen: 0.032 ng/ul
 RT: 3.199 min Scan# 70
 Delta R.T. -0.009 min
 Lab File: BN034822.D
 Acq: 02 Nov 2024 02:13

Instrument :
 BNA_N
 ClientSampleId :
 E1L86

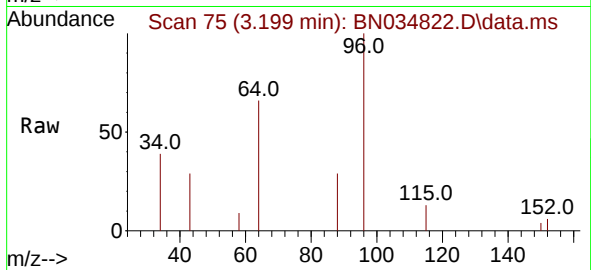

Tgt Ion: 88 Resp: 278

Ion	Ratio	Lower	Upper
88	100		
43	99.3	41.9	62.9
58	31.9	57.5	86.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/04/2024
 Supervised By :mohammad ahmed 11/05/2024

