
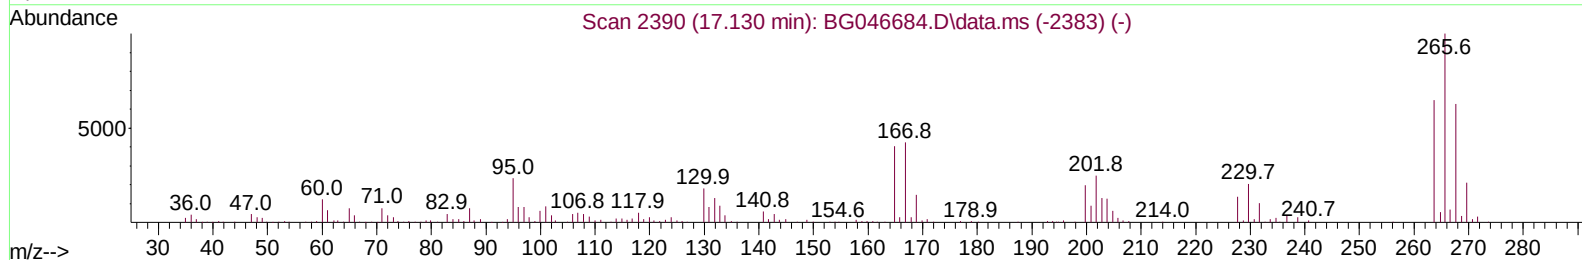
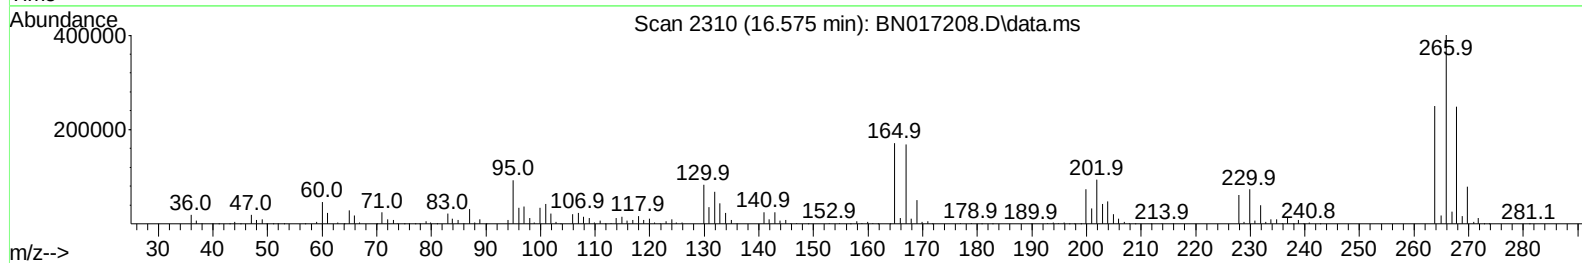


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\  
Data File : BN017208.D  
Acq On    : 01 Nov 2021  11:58  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Nov 01 19:03:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

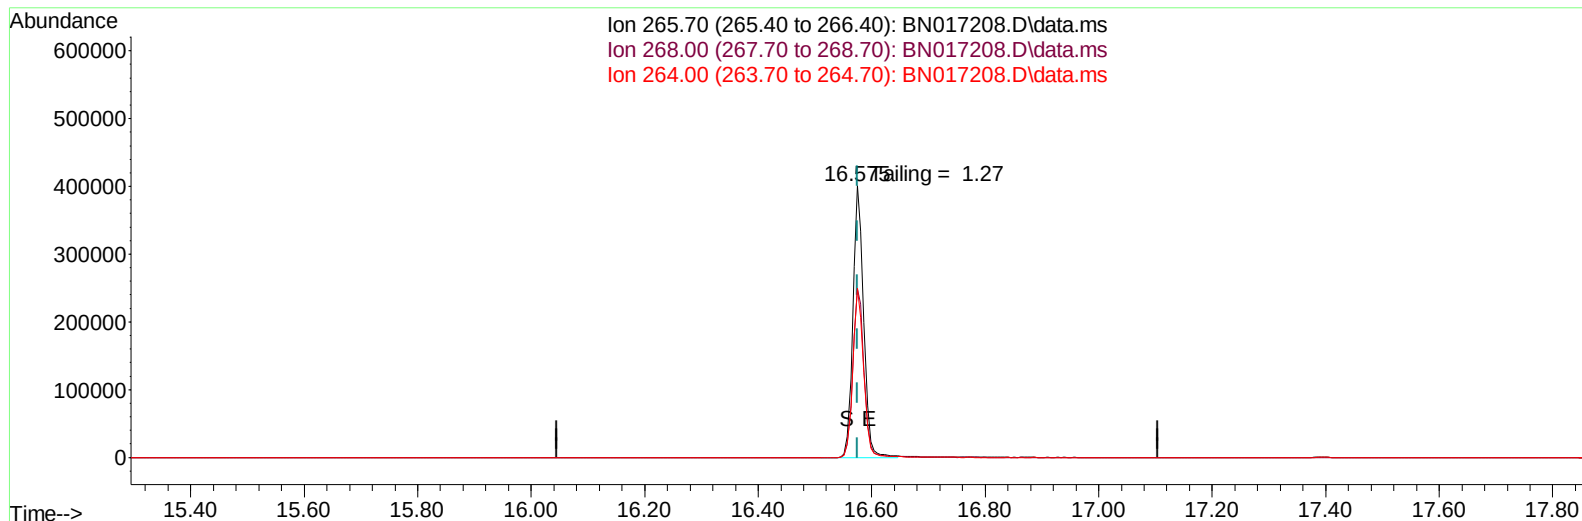

TIC: BN017208.D\data.ms

(70) Pentachlorophenol (C)




16.575min (0.000) 21974.76 ng

response **535982**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.16
264.00	61.60	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
 Data File : BN017208.D
 Acq On : 01 Nov 2021 11:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 19:03:02 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 01 19:02:51 2021
 Response via : Initial Calibration

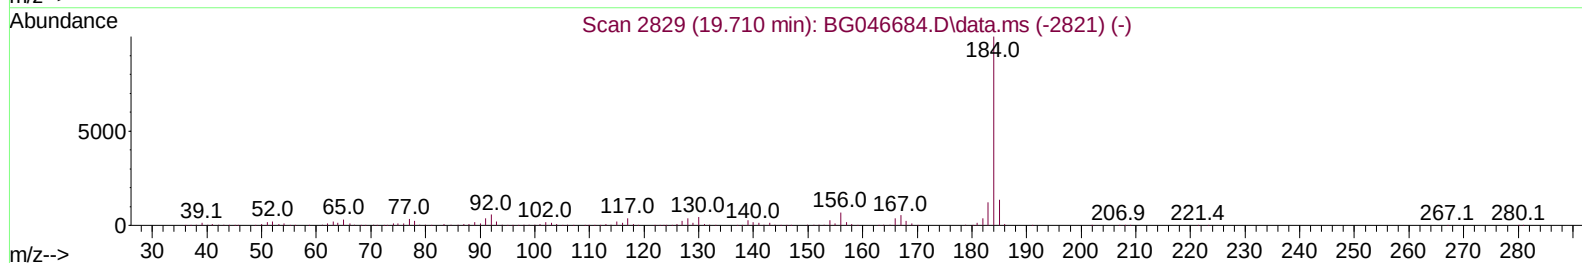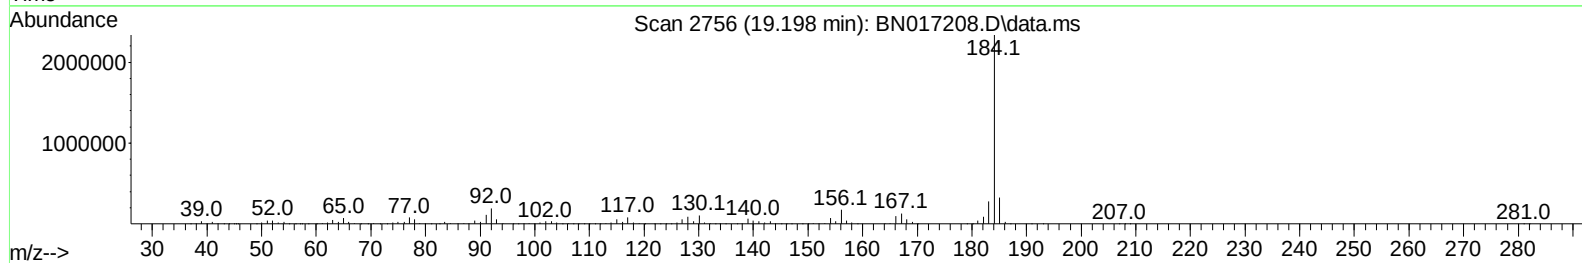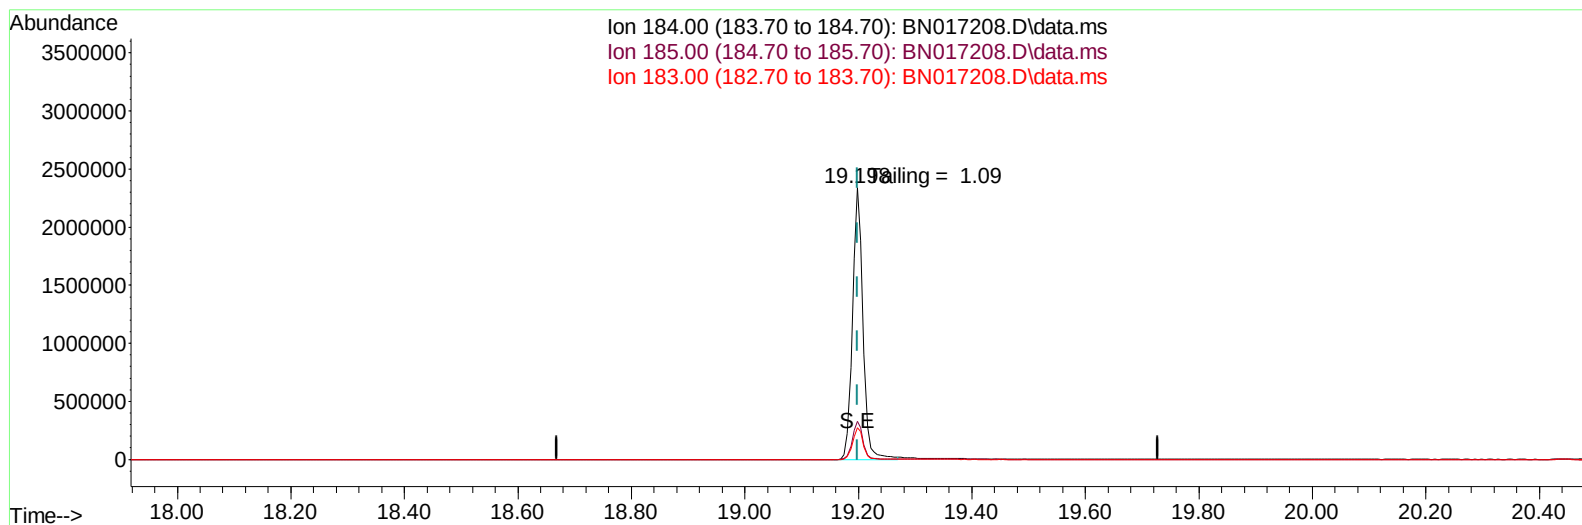

TIC: BN017208.D\data.ms

(77) Benzidine**19.198min (0.000) 0.00 ng****response 3081328**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.76
0.00	0.00	0.00