
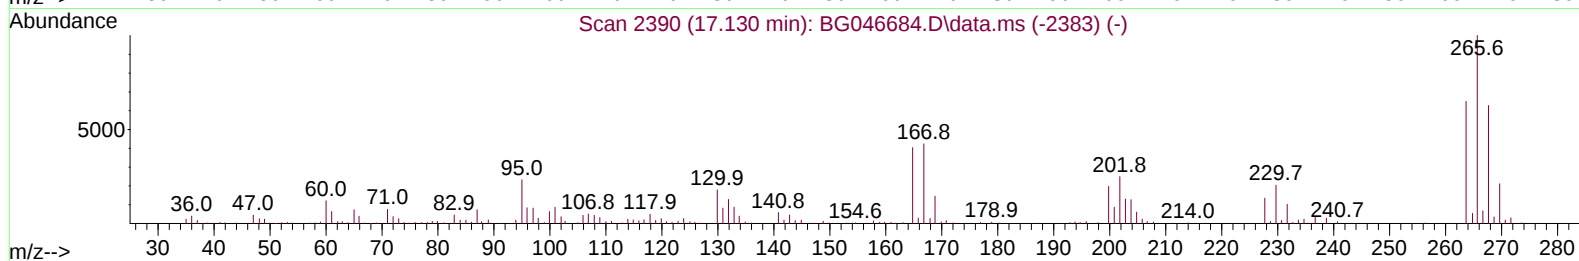
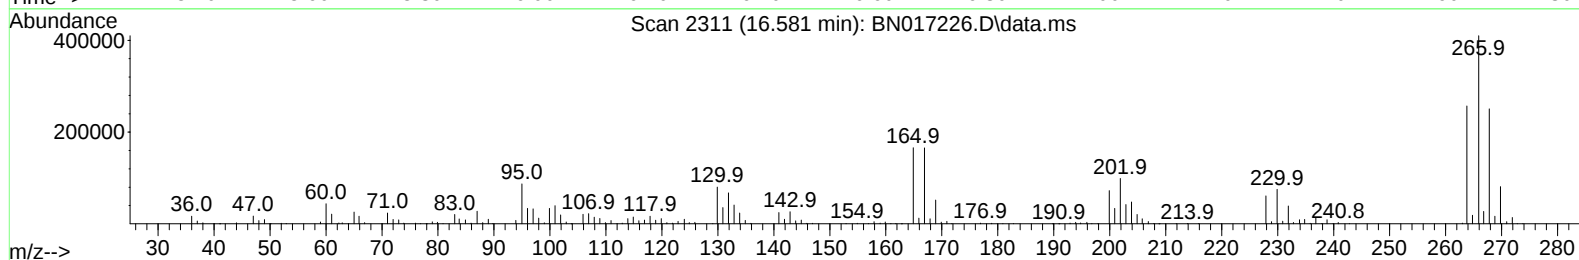


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
 Data File : BN017226.D
 Acq On : 02 Nov 2021 00:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 05:25:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 01 19:02:51 2021
 Response via : Initial Calibration

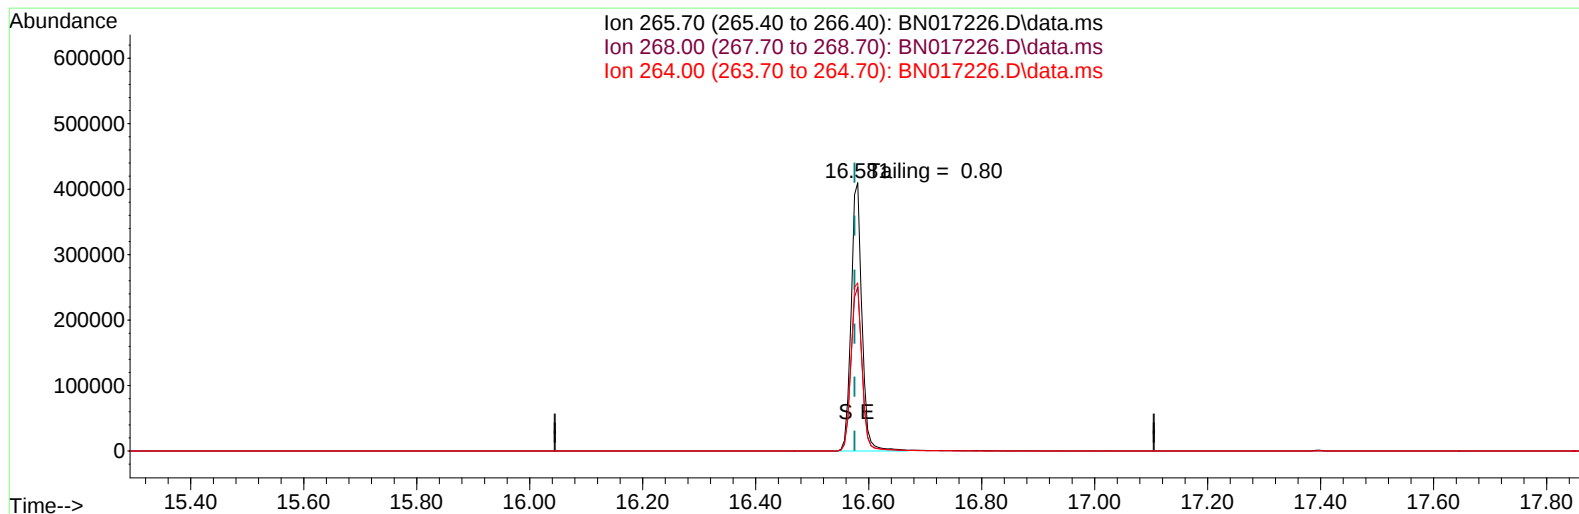

TIC: BN017226.D\data.ms

(70) Pentachlorophenol (C)




16.581min (+ 0.006) 23431.32 ng

response 549075

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.18
264.00	61.60	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
Data File : BN017226.D
Acq On : 02 Nov 2021 00:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 05:25:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

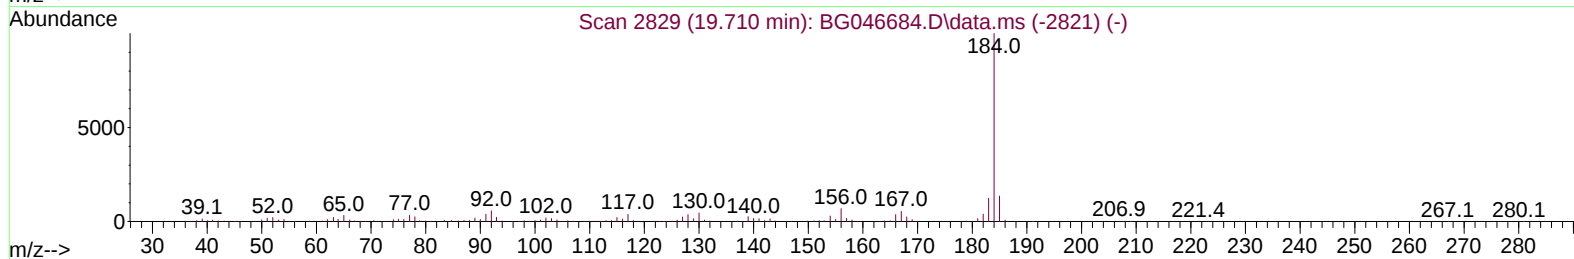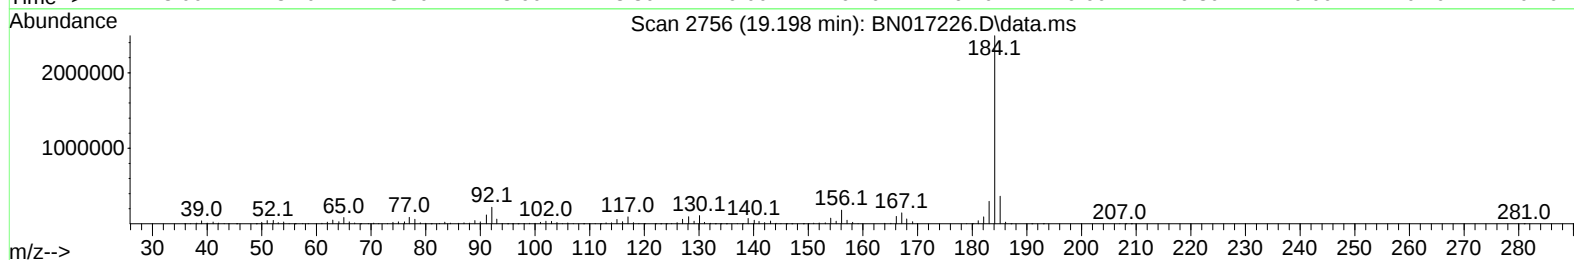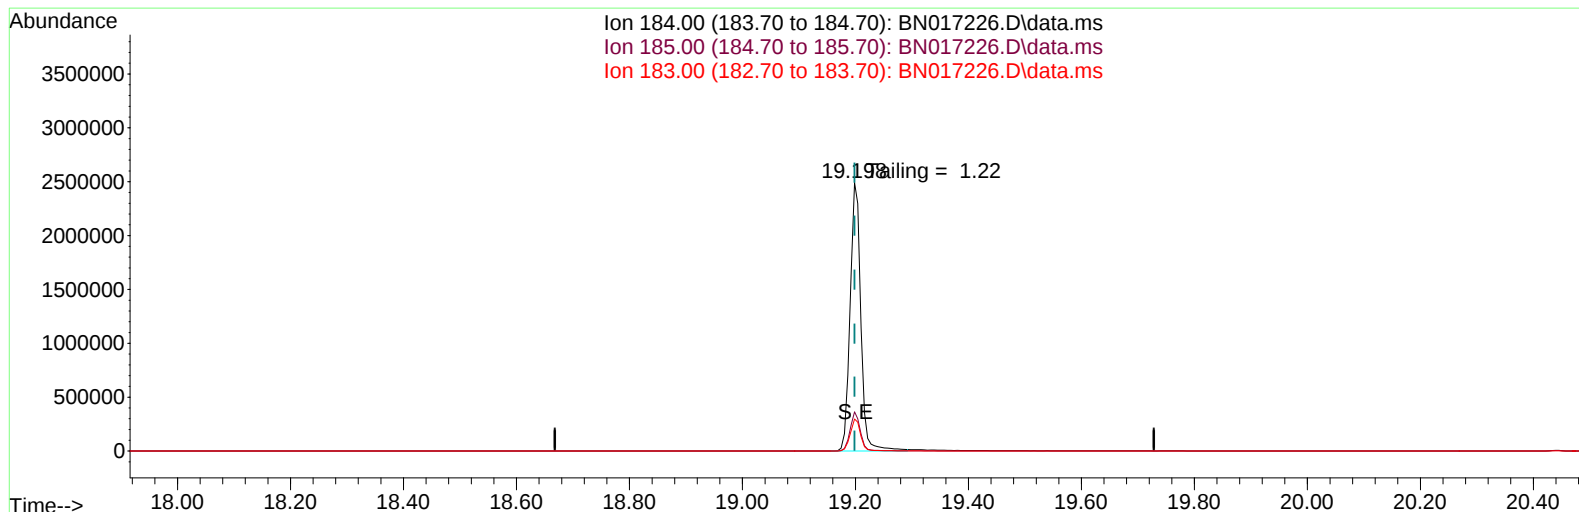

TIC: BN017226.D\data.ms

(77) Benzidine

19.198min (+ 0.000) 0.00 ng

response 3347172

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.63
183.00	13.20	11.93
0.00	0.00	0.00