


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
 Data File : BN017208.D
 Acq On : 01 Nov 2021 11:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 01 17:00:24 2021

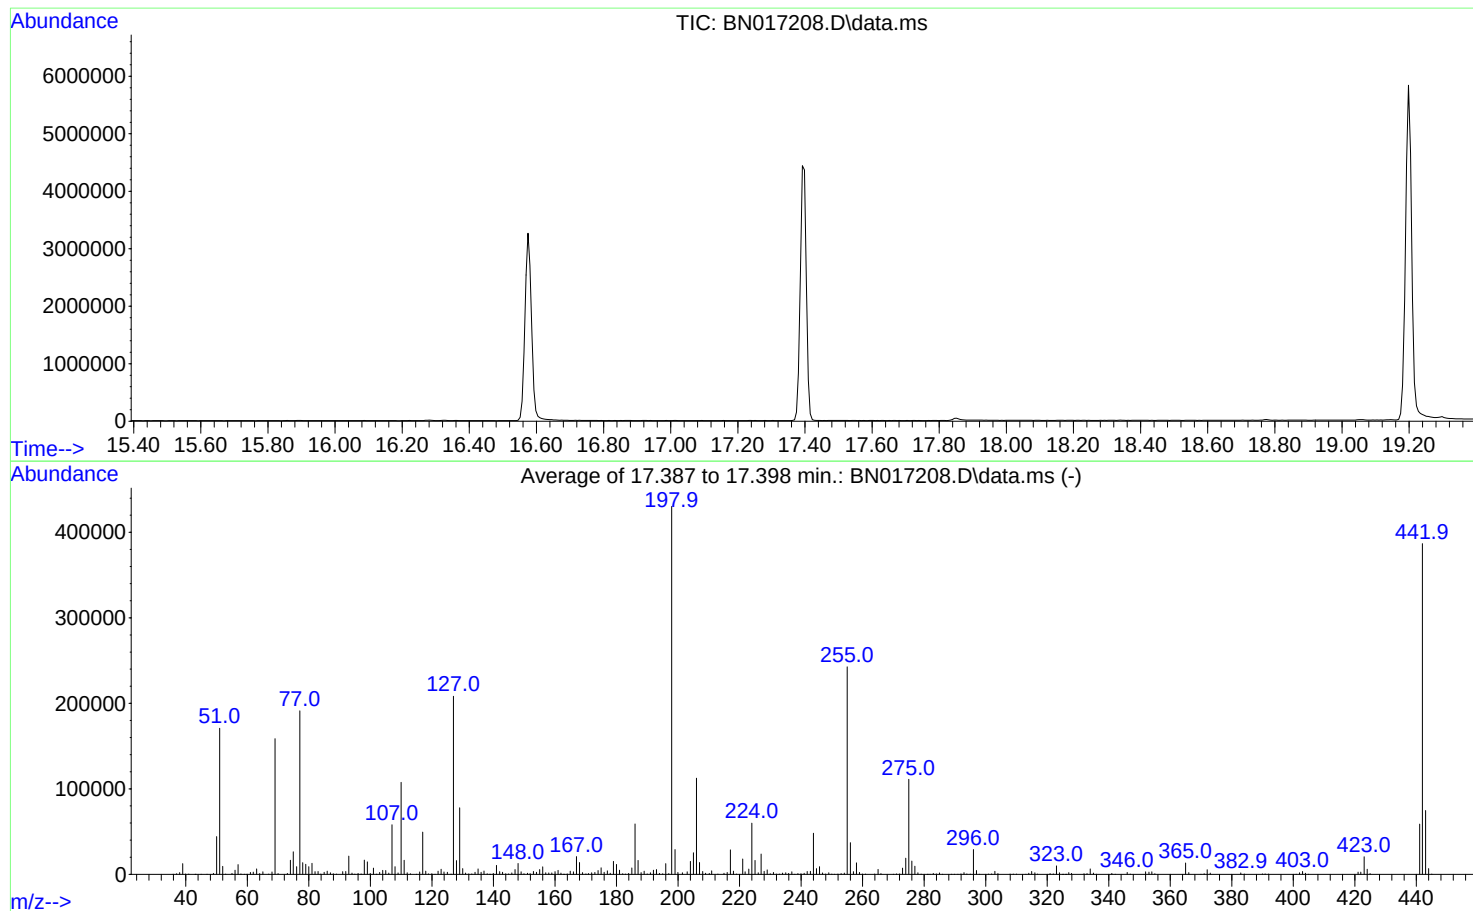




AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	170837	PASS
68	69	0.00	2	1.8	2852	PASS
69	198	0.00	100	36.9	158741	PASS
70	69	0.00	2	0.6	893	PASS
127	198	10	80	48.4	208363	PASS
197	198	0.00	2	0.2	1017	PASS
198	198	100	100	100.0	430187	PASS
199	198	5	9	6.8	29088	PASS
275	198	10	60	25.8	111120	PASS
365	198	1	100	3.1	13315	PASS
441	198	0.01	100	13.7	58832	PASS
442	442	50	100	100.0	386795	PASS
443	442	15	24	19.3	74755	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
Data File : BN017208.D
Acq On : 01 Nov 2021 11:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 01 19:03:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

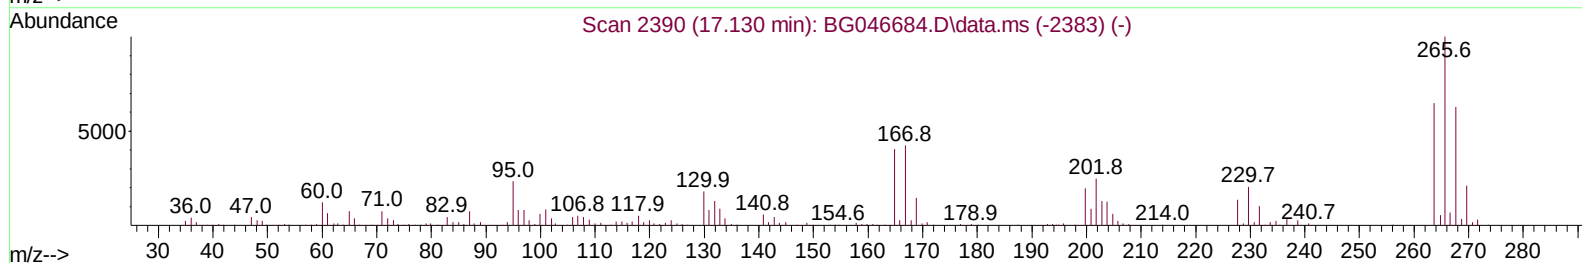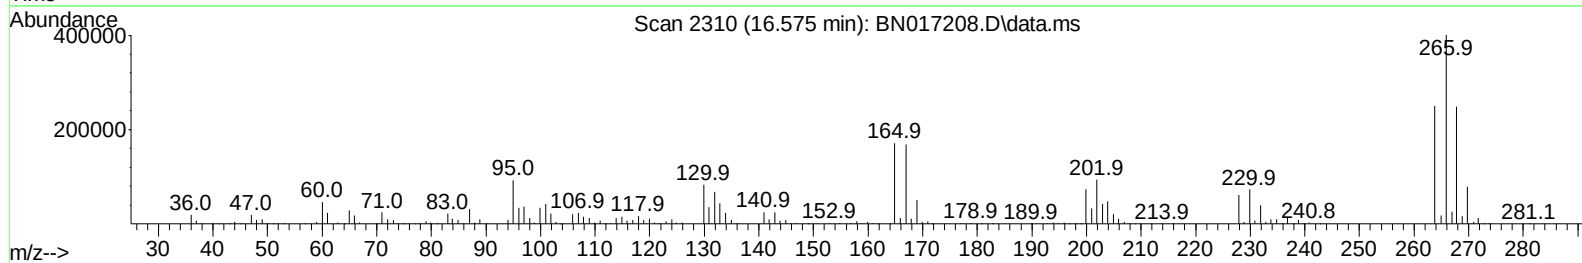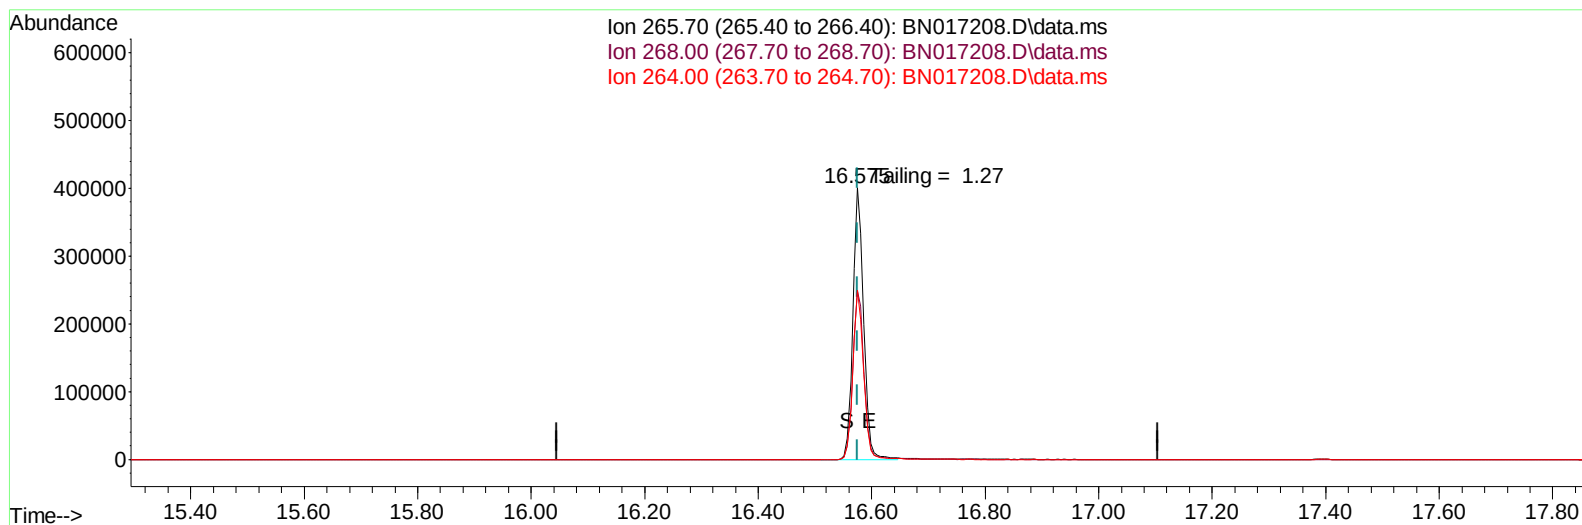

TIC: BN017208.D\data.ms

(70) Pentachlorophenol (C)

16.575min (0.000) 21974.76 ng




response 535982

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.16
264.00	61.60	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
Data File : BN017208.D
Acq On : 01 Nov 2021 11:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 01 19:03:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

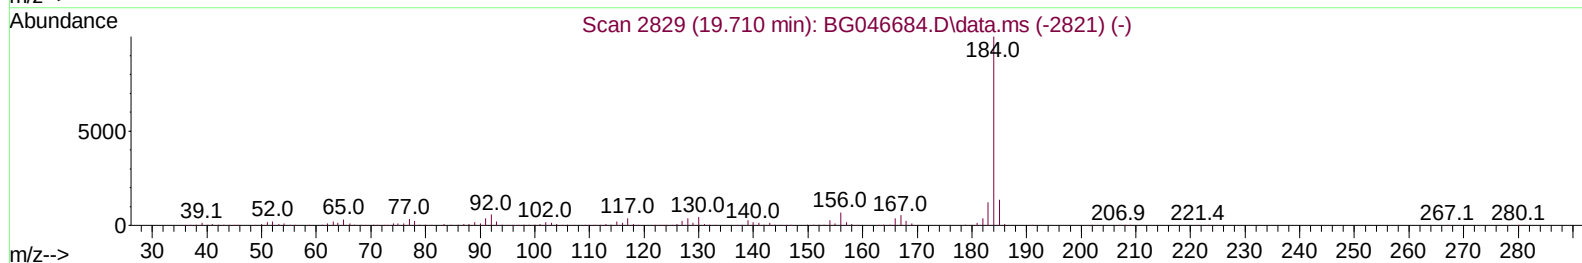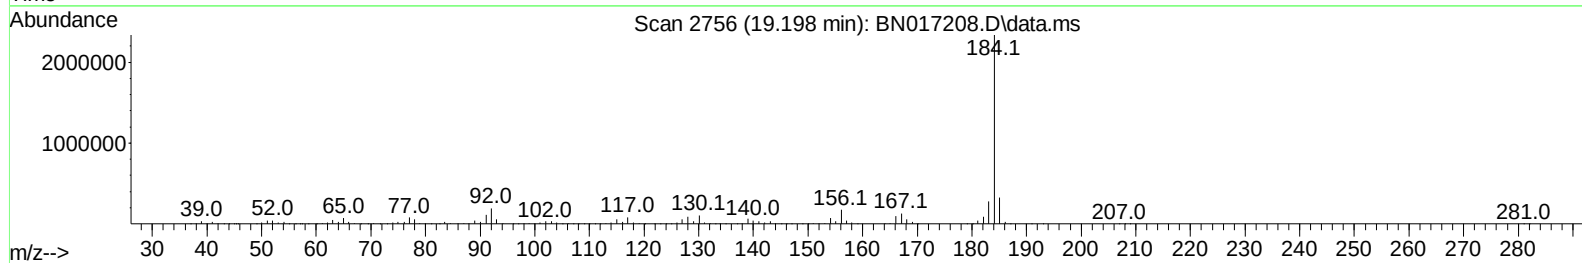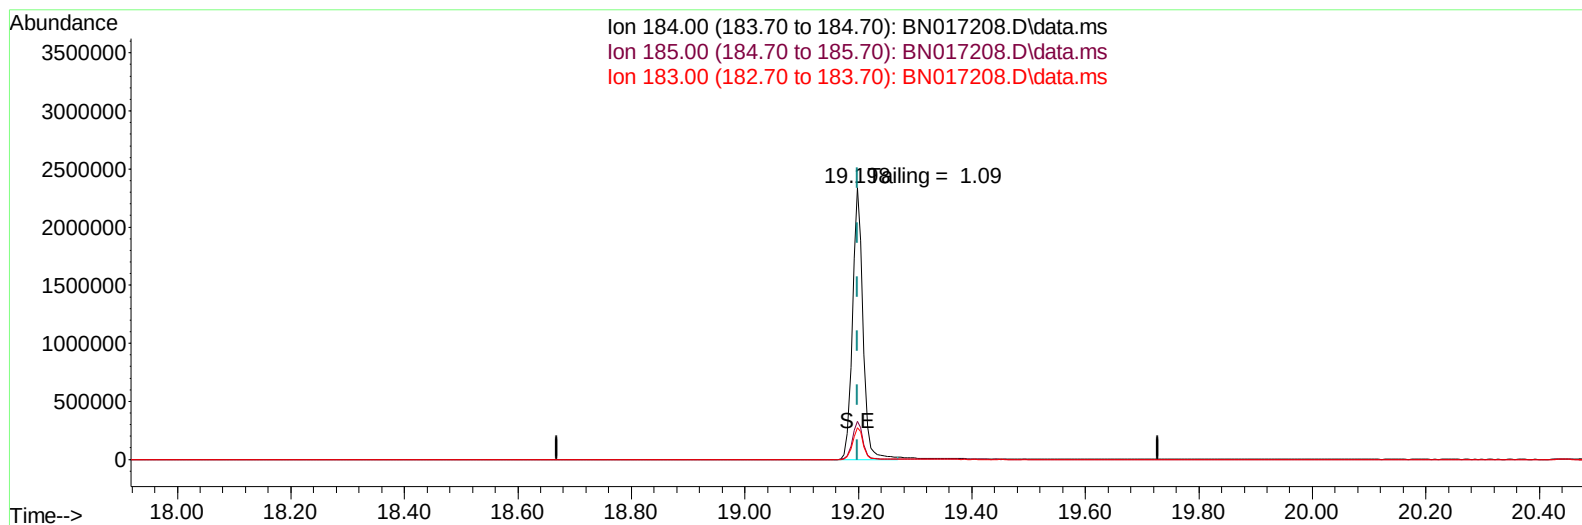

TIC: BN017208.D\data.ms

(77) Benzidine

19.198min (0.000) 0.00 ng

response 3081328

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2021	BNA_N	BN017208.D
Compound Name	Response	Retention Time
DDT	1571268	20.445
DDD	9308	19.998
DDE	123	19.486
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9431	1580699	0.60

Instrument :
BNA_N
ClientSampleId :
DFTPP