
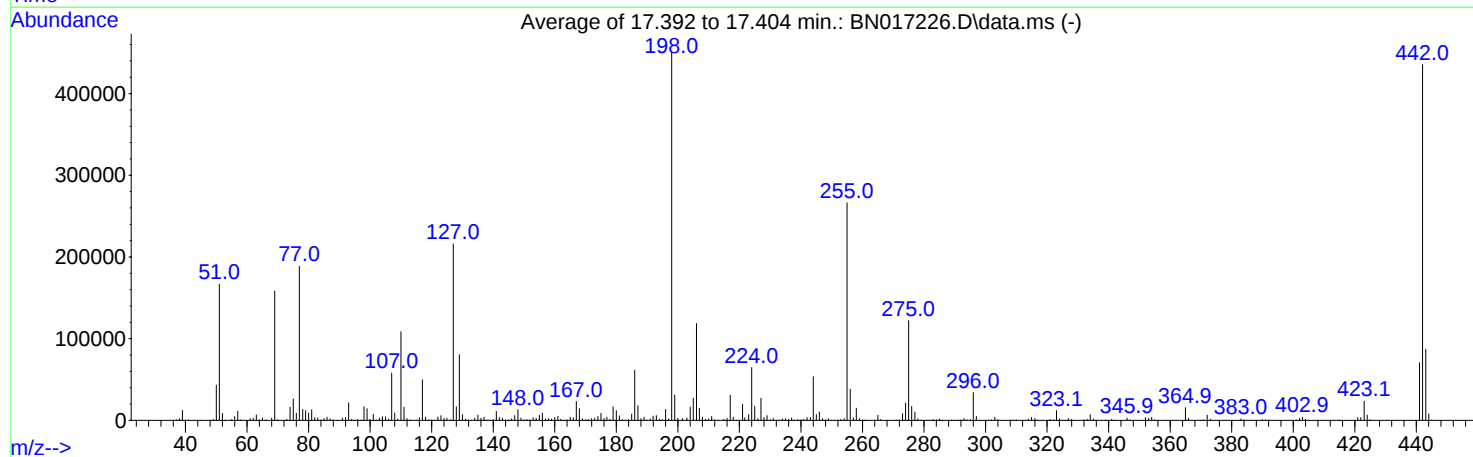


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
 Data File : BN017226.D
 Acq On : 02 Nov 2021 00:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 01 17:00:24 2021

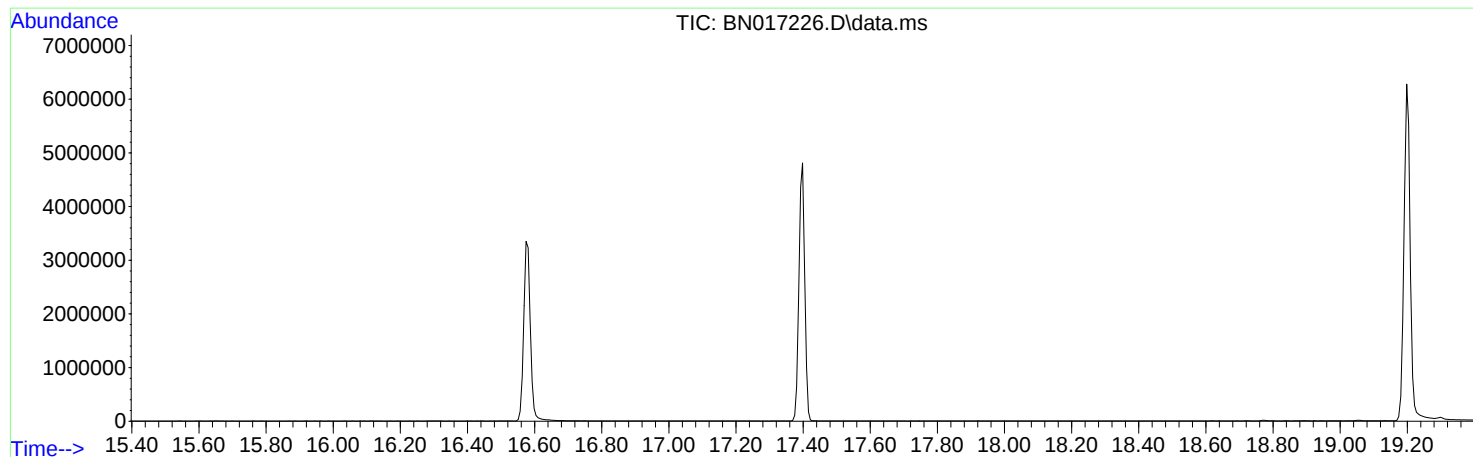




AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	166955	PASS
68	69	0.00	2	1.8	2834	PASS
69	198	0.00	100	35.2	158328	PASS
70	69	0.00	2	0.5	820	PASS
127	198	10	80	48.0	215979	PASS
197	198	0.00	2	0.3	1555	PASS
198	198	100	100	100.0	450261	PASS
199	198	5	9	6.9	30947	PASS
275	198	10	60	27.1	122029	PASS
365	198	1	100	3.4	15446	PASS
441	198	0.01	100	15.6	70419	PASS
442	442	50	100	100.0	435541	PASS
443	442	15	24	20.0	87080	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
 Data File : BN017226.D
 Acq On : 02 Nov 2021 00:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 02 05:25:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 01 19:02:51 2021
 Response via : Initial Calibration

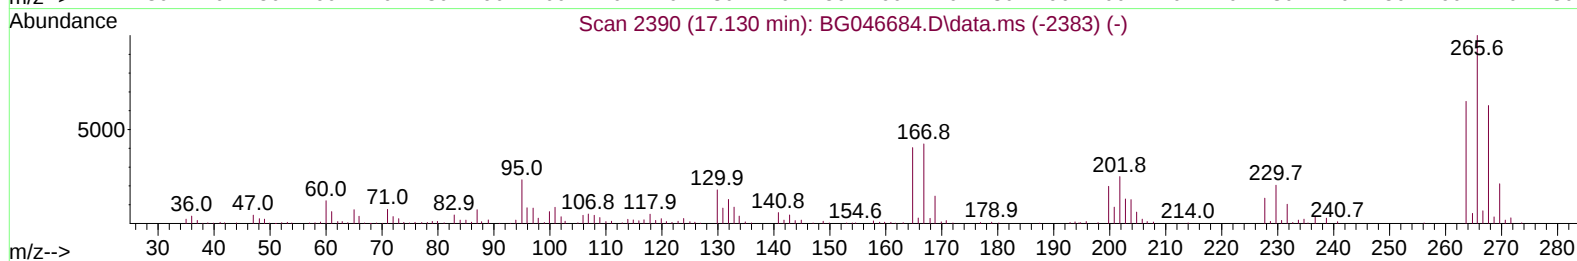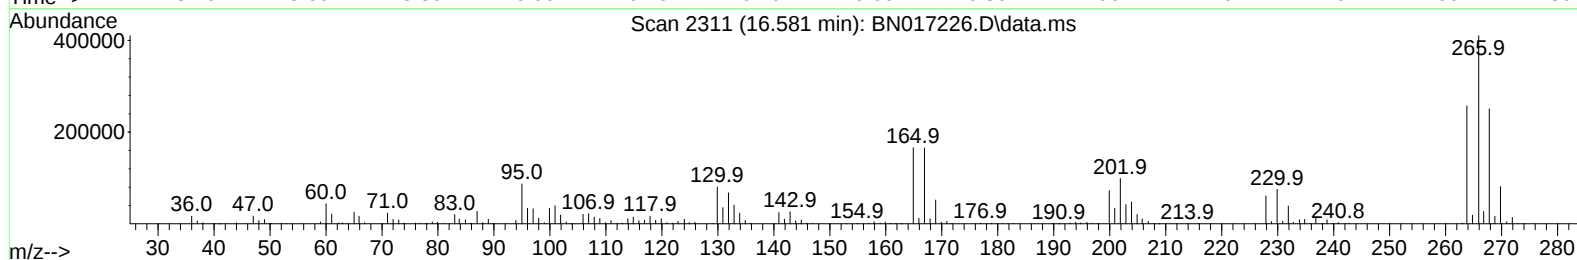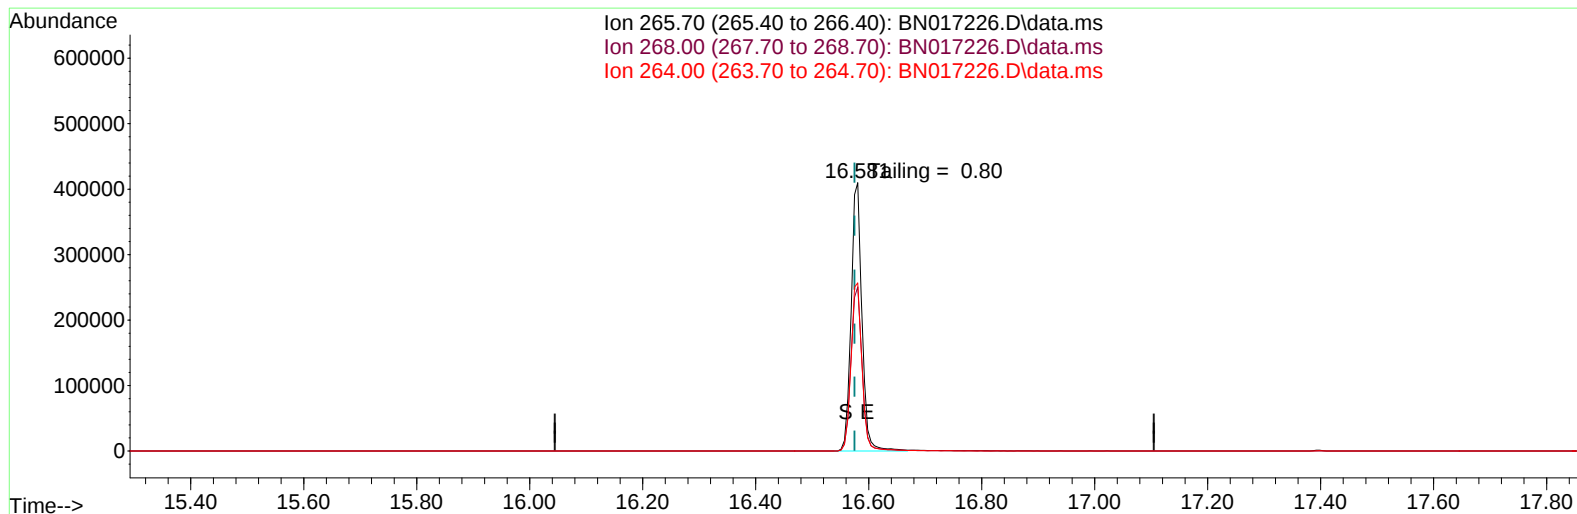

TIC: BN017226.D\data.ms

(70) Pentachlorophenol (C)

16.581min (+ 0.006) 23431.32 ng




response 549075

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.18
264.00	61.60	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110121\
Data File : BN017226.D
Acq On : 02 Nov 2021 00:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 02 05:25:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 01 19:02:51 2021
Response via : Initial Calibration

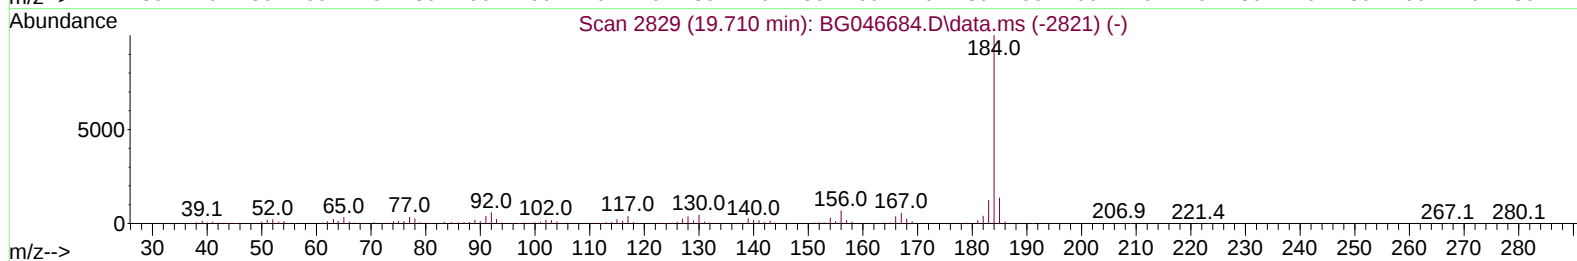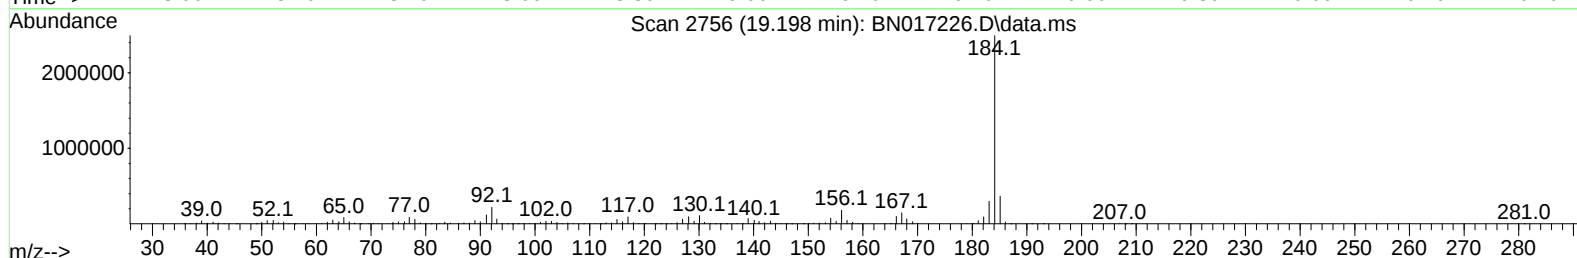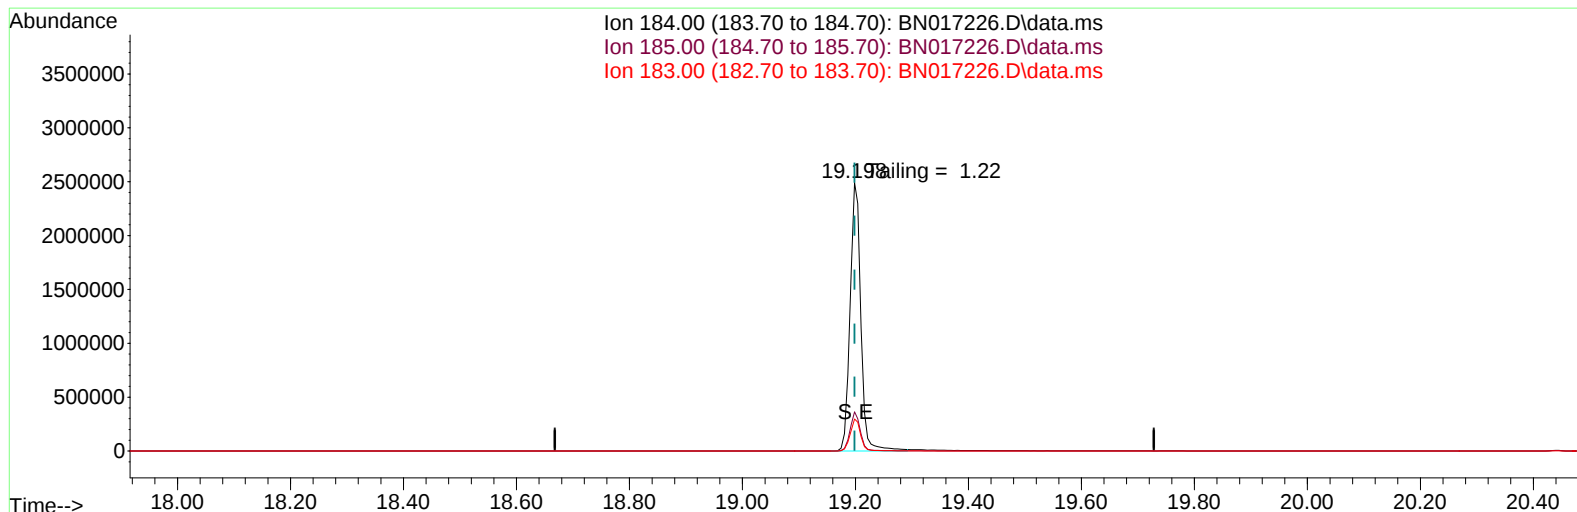

TIC: BN017226.D\data.ms

(77) Benzidine

19.198min (+ 0.000) 0.00 ng

response 3347172

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.63
183.00	13.20	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2021	BNA_N	<u>BN017226.D</u>
Compound Name	Response	Retention Time
DDT	1683029	20.439
DDD	16138	19.998
DDE	137	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16275	1699304	0.96

Instrument :
BNA_N
ClientSampleId :
DFTPP