
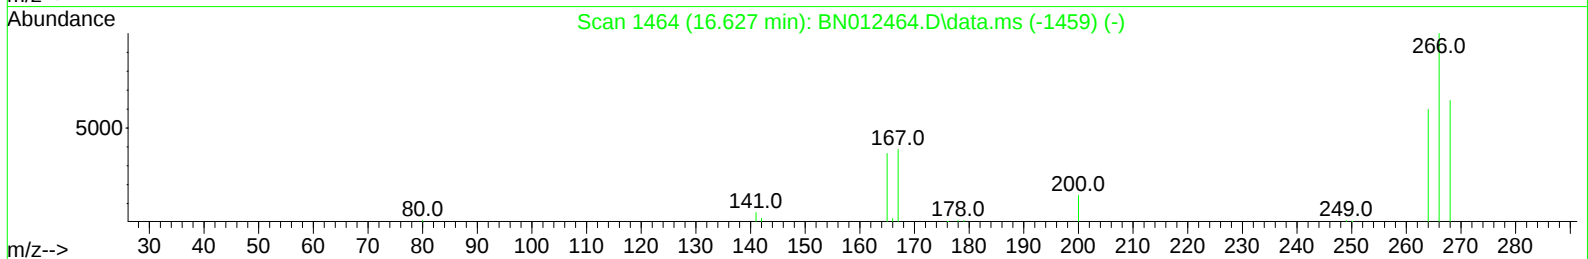
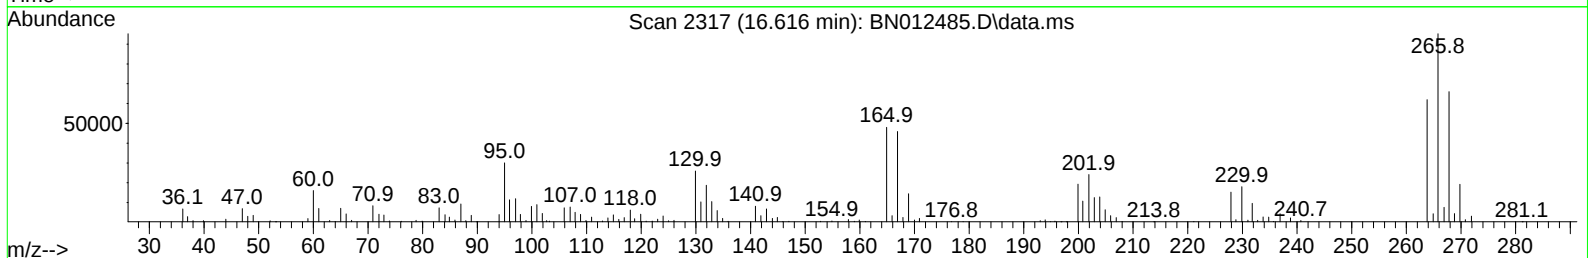


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110220\
 Data File : BN012485.D
 Acq On : 02 Nov 2020 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 01:20:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 30 14:49:10 2020
 Response via : Initial Calibration

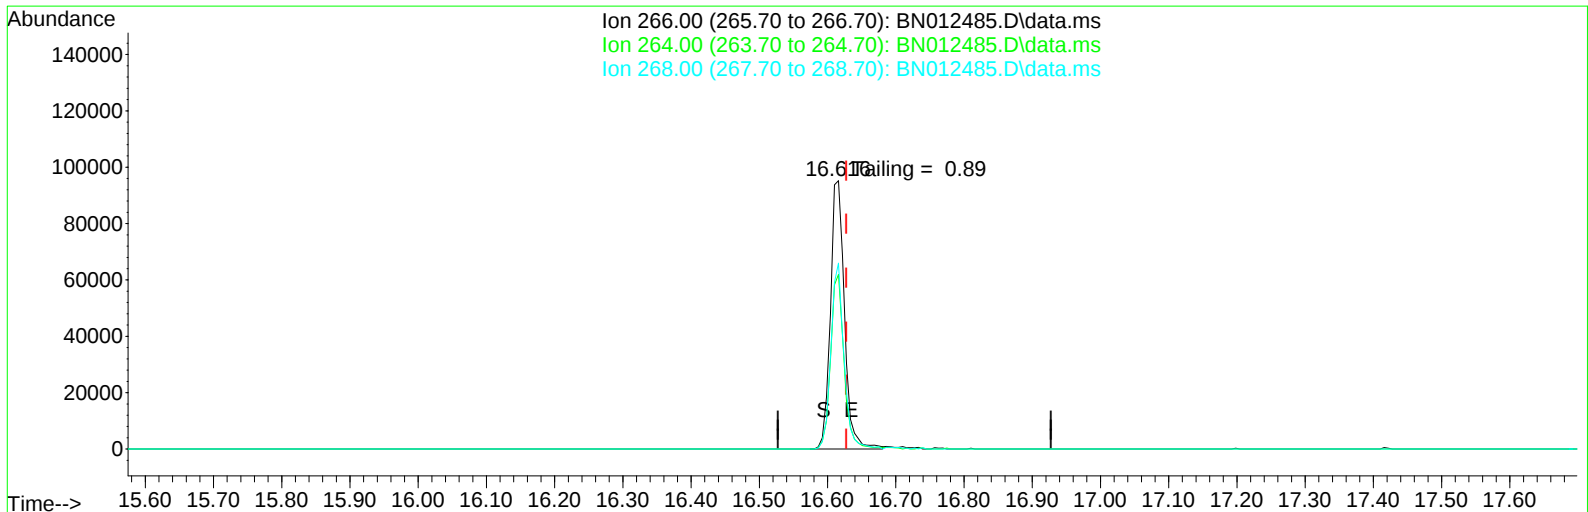

TIC: BN012485.D\data.ms

(24) Pentachlorophenol

16.616min (-0.011) 0.00 ng

response 137362

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.42
268.00	64.40	64.31
0.00	0.00	0.00