

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110220\
 Data File : BN012489.D
 Acq On : 02 Nov 2020 14:19
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Nov 02 14:52:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 02 08:41:36 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.562	152	657	0.40	ng	# 0.00
7) Naphthalene-d8	10.326	136	2777	0.40	ng	#-0.01
13) Acenaphthene-d10	14.205	164	1574	0.40	ng	-0.01
19) Phenanthrene-d10	16.956	188	3134	0.40	ng	#-0.01
29) Chrysene-d12	21.174	240	3101	0.40	ng	# 0.00
36) Perylene-d12	23.343	264	3660	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.178	112	808	0.35	ng	0.00
5) Phenol-d6	6.749	99	1009	0.36	ng	0.00
8) Nitrobenzene-d5	8.717	82	1138	0.36	ng	-0.01
11) 2-Methylnaphthalene-d10	11.931	152	1682	0.37	ng	0.00
14) 2,4,6-Tribromophenol	15.714	330	386	0.36	ng	0.00
15) 2-Fluorobiphenyl	12.822	172	2119	0.36	ng	-0.01
27) Fluoranthene-d10	19.003	212	3425	0.35	ng	0.00
31) Terphenyl-d14	19.613	244	2671	0.37	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.165	88	413	0.37	ng	# 85
3) n-Nitrosodimethylamine	3.479	42	1083	0.40	ng	# 68
6) bis(2-Chloroethyl)ether	7.006	93	622	0.34	ng	# 84
9) Naphthalene	10.377	128	2848	0.36	ng	98
10) Hexachlorobutadiene	10.668	225	598	0.37	ng	# 98
12) 2-Methylnaphthalene	12.007	142	1853	0.36	ng	# 86
16) Acenaphthylene	13.925	152	2819	0.36	ng	100
17) Acenaphthene	14.268	154	1816	0.36	ng	91
18) Fluorene	15.270	166	2233	0.36	ng	98
20) 4,6-Dinitro-2-methylph...	15.372	198	211	0.35	ng	# 1
21) 4-Bromophenyl-phenylether	16.165	248	693	0.36	ng	97
22) Hexachlorobenzene	16.274	284	886	0.37	ng	# 85
23) Atrazine	16.445	200	654	0.36	ng	95
24) Pentachlorophenol	16.627	266	375	0.35	ng	99
25) Phenanthrene	17.005	178	3364	0.36	ng	99
26) Anthracene	17.090	178	3005	0.35	ng	99
28) Fluoranthene	19.032	202	3840	0.35	ng	99
30) Pyrene	19.400	202	3923	0.37	ng	99
32) Benzo(a)anthracene	21.152	228	3410	0.35	ng	96
33) Chrysene	21.205	228	3871	0.37	ng	97
34) Bis(2-ethylhexyl)phtha...	21.099	149	2254	0.36	ng	93
35) Indeno(1,2,3-cd)pyrene	25.503	276	5717	0.37	ng	96
37) Benzo(b)fluoranthene	22.697	252	4080	0.35	ng	# 86
38) Benzo(k)fluoranthene	22.741	252	4496	0.36	ng	# 91
39) Benzo(a)pyrene	23.251	252	4145	0.37	ng	# 81
40) Dibenzo(a,h)anthracene	25.514	278	4702	0.37	ng	92
41) Benzo(g,h,i)perylene	26.157	276	4921	0.37	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110220\
Data File : BN012489.D
Acq On : 02 Nov 2020 14:19
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleID :
SSTDCCC0.4EC

Quant Time: Nov 02 14:52:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 02 08:41:36 2020
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.562 min Scan# 569
 Delta R.T. -0.008 min
 Lab File: BN012489.D
 Acq: 02 Nov 2020 14:19

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion: 152 Resp: 657




Ion	Ratio	Lower	Upper
152	100		
150	148.1	116.6	174.8
115	83.3	52.9	79.3




#2
 1,4-Dioxane
 Concen: 0.37 ng
 RT: 3.165 min Scan# 23
 Delta R.T. -0.000 min
 Lab File: BN012489.D
 Acq: 02 Nov 2020 14:19

Tgt Ion: 88 Resp: 413

Ion	Ratio	Lower	Upper
88	100		
58	79.2	59.4	89.2
43	60.3	32.3	48.5









#3
n-Nitrosodimethylamine
Concen: 0.40 ng
RT: 3.479 min Scan# 62
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 1083
Ion Ratio Lower Upper
42 100
74 51.8 64.4 96.6#
44 7.3 2.8 4.2#



#4
2-Fluorophenol
Concen: 0.35 ng
RT: 5.178 min Scan# 273
Delta R.T. -0.008 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion: 112 Resp: 808
Ion Ratio Lower Upper
112 100
64 72.5 49.5 74.3
63 57.1 32.0 48.0#









#5
Phenol-d6
Concen: 0.36 ng
RT: 6.749 min Scan# 468
Delta R.T. -0.008 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 1009
Ion Ratio Lower Upper
99 100
42 49.1 22.4 33.6#
71 63.8 37.8 56.6#



#6
bis(2-Chloroethyl)ether
Concen: 0.34 ng
RT: 7.006 min Scan# 500
Delta R.T. -0.008 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion: 93 Resp: 622
Ion Ratio Lower Upper
93 100
63 98.6 63.1 94.7#
95 33.3 26.1 39.1









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.326 min Scan# 821
Delta R.T. -0.013 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	2777
Ion	Ratio	Lower	Upper
136	100		
137	14.2	10.6	15.8
54	16.1	8.6	12.8#
68	7.7	5.7	8.5



#8
Nitrobenzene-d5
Concen: 0.36 ng
RT: 8.717 min Scan# 694
Delta R.T. -0.013 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:	82	Resp:	1138
Ion	Ratio	Lower	Upper
82	100		
128	38.8	30.6	46.0
54	76.6	48.3	72.5#









#9
Naphthalene
Concen: 0.36 ng
RT: 10.377 min Scan# 825
Delta R.T. -0.013 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:128 Resp: 2848




Ion	Ratio	Lower	Upper
128	100		
129	13.3	9.8	14.8
127	16.0	12.2	18.4




#10
Hexachlorobutadiene
Concen: 0.37 ng
RT: 10.668 min Scan# 848
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:225 Resp: 598

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	61.9	51.0	76.6









#11
2-Methylnaphthalene-d10
Concen: 0.37 ng
RT: 11.931 min Scan# 1008
Delta R.T. -0.009 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 1682
Ion Ratio Lower Upper
152 100
151 19.3 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.36 ng
RT: 12.007 min Scan# 1025
Delta R.T. -0.009 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:142 Resp: 1853
Ion Ratio Lower Upper
142 100
141 92.5 69.4 104.2
115 64.3 35.7 53.5#









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.205 min Scan# 1271
Delta R.T. -0.012 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	164	Resp:	1574
Ion	Ratio	Lower	Upper
164	100		
162	104.2	80.6	120.8
160	50.8	39.5	59.3



#14
2,4,6-Tribromophenol
Concen: 0.36 ng
RT: 15.714 min Scan# 1390
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:	330	Resp:	386
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	50.0	34.4	51.6









#15
2-Fluorobiphenyl
Concen: 0.36 ng
RT: 12.822 min Scan# 1162
Delta R.T. -0.013 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	172	Resp:	2119
Ion	Ratio	Lower	Upper
172	100		
171	39.4	28.2	42.4
170	27.9	20.0	30.0



#16
Acenaphthylene
Concen: 0.36 ng
RT: 13.925 min Scan# 1249
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:	152	Resp:	2819
Ion	Ratio	Lower	Upper
152	100		
151	19.8	15.8	23.8
153	13.4	10.6	16.0









#17
Acenaphthene
Concen: 0.36 ng
RT: 14.268 min Scan# 1276
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 1816
Ion Ratio Lower Upper
154 100
153 116.2 83.6 125.4
152 57.8 43.9 65.9



#18
Fluorene
Concen: 0.36 ng
RT: 15.270 min Scan# 1355
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:166 Resp: 2233
Ion Ratio Lower Upper
166 100
165 100.4 78.6 118.0
167 13.9 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.956 min Scan# 1491
Delta R.T. -0.012 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 3134
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.3 5.0 7.4#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.35 ng
RT: 15.372 min Scan# 1363
Delta R.T. -0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:198 Resp: 211
Ion Ratio Lower Upper
198 100
51 142.3 43.5 65.3#
105 81.1 27.2 40.8#







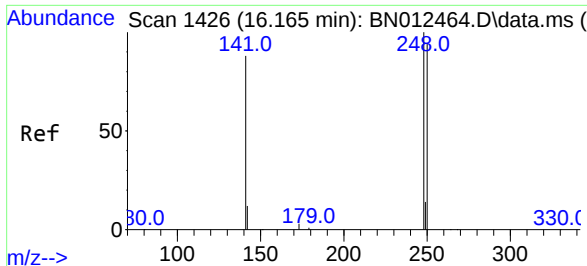

#21
4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.165 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	248	Resp:	693
Ion	Ratio	Lower	Upper
248	100		
250	99.8	77.3	115.9
141	74.2	57.8	86.8

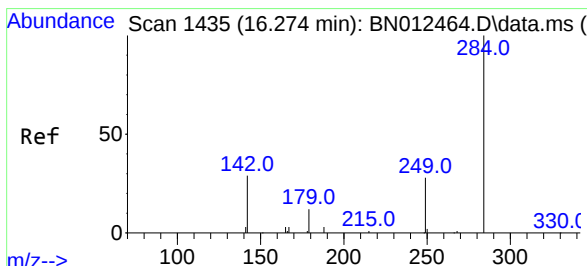

#22
Hexachlorobenzene
Concen: 0.37 ng
RT: 16.274 min Scan# 1435
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:	284	Resp:	886
Ion	Ratio	Lower	Upper
284	100		
142	55.5	32.0	48.0#
249	32.1	27.0	40.6









#23
Atrazine
Concen: 0.36 ng
RT: 16.445 min Scan# 1449
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	200	Resp:	654
Ion	Ratio	Lower	Upper
200	100		
173	28.8	22.8	34.2
215	52.7	38.1	57.1



#24
Pentachlorophenol
Concen: 0.35 ng
RT: 16.627 min Scan# 1464
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:	266	Resp:	375
Ion	Ratio	Lower	Upper
266	100		
264	64.5	50.9	76.3
268	63.2	51.5	77.3









#25
Phenanthrene
Concen: 0.36 ng
RT: 17.005 min Scan# 1495
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	178	Resp:	3364
Ion	Ratio	Lower	Upper
178	100		
176	19.6	14.8	22.2
179	15.5	12.4	18.6



#26
Anthracene
Concen: 0.35 ng
RT: 17.090 min Scan# 1502
Delta R.T. -0.012 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19





Tgt Ion:	178	Resp:	3005
Ion	Ratio	Lower	Upper
178	100		
176	18.8	14.8	22.2
179	15.0	12.5	18.7








#27
Fluoranthene-d10
Concen: 0.35 ng
RT: 19.003 min Scan# 1777
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19


Tgt Ion:	212	Resp:	3425
Ion Ratio	Lower	Upper	
212	100		
106	7.1	6.8	10.2
104	4.9	4.1	6.1



#28
Fluoranthene
Concen: 0.35 ng
RT: 19.032 min Scan# 1783
Delta R.T. -0.005 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:	202	Resp:	3840
Ion Ratio	Lower	Upper	
202	100		
101	6.3	5.8	8.6
203	17.1	13.7	20.5









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.174 min Scan# 2089
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 3101
Ion Ratio Lower Upper
240 100
120 9.5 5.3 7.9#
236 27.7 21.8 32.8



#30
Pyrene
Concen: 0.37 ng
RT: 19.400 min Scan# 1857
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:202 Resp: 3923
Ion Ratio Lower Upper
202 100
200 21.1 16.6 24.8
203 17.6 13.8 20.8









#31
Terphenyl-d14
Concen: 0.37 ng
RT: 19.613 min Scan# 1900
Delta R.T. -0.005 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:244 Resp: 2671
Ion Ratio Lower Upper
244 100
212 12.0 7.3 10.9#
122 13.0 7.3 10.9#



#32
Benzo(a)anthracene
Concen: 0.35 ng
RT: 21.152 min Scan# 2087
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:228 Resp: 3410
Ion Ratio Lower Upper
228 100
226 29.4 22.3 33.5
229 22.3 15.7 23.5









#33
Chrysene
Concen: 0.37 ng
RT: 21.205 min Scan# 2092
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	228	Resp:	3871
Ion	Ratio	Lower	Upper
228	100		
226	31.6	24.2	36.2
229	20.7	15.7	23.5



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.36 ng
RT: 21.099 min Scan# 2082
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:	149	Resp:	2254
Ion	Ratio	Lower	Upper
149	100		
167	24.6	23.2	34.8
279	5.0	3.9	5.9









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.37 ng
RT: 25.503 min Scan# 3110
Delta R.T. 0.003 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:276 Resp: 5717
Ion Ratio Lower Upper
276 100
138 13.3 13.3 19.9
277 24.6 20.2 30.4



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.343 min Scan# 2479
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:264 Resp: 3660
Ion Ratio Lower Upper
264 100
260 24.5 19.8 29.6
265 61.4 51.4 77.0









#37
Benzo(b)fluoranthene
Concen: 0.35 ng
RT: 22.697 min Scan# 2290
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 4080
Ion Ratio Lower Upper
252 100
253 30.9 20.1 30.1#
125 16.2 7.2 10.8#



#38
Benzo(k)fluoranthene
Concen: 0.36 ng
RT: 22.741 min Scan# 2303
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Tgt Ion:252 Resp: 4496
Ion Ratio Lower Upper
252 100
253 30.1 19.8 29.8#
125 11.0 7.1 10.7#





#39

Benzo(a)pyrene

Concen: 0.37 ng





RT: 23.251 min Scan# 2452

Delta R.T. 0.003 min

Lab File: BN012489.D

Acq: 02 Nov 2020 14:19

Tgt Ion:	252	Resp:	4145
Ion	Ratio	Lower	Upper
252	100		
253	35.6	21.3	31.9#
125	18.8	8.3	12.5#



#40

Dibenzo(a,h)anthracene

Concen: 0.37 ng




RT: 25.514 min Scan# 3113


Delta R.T. 0.000 min

Lab File: BN012489.D

Acq: 02 Nov 2020 14:19

Tgt Ion:	278	Resp:	4702
Ion	Ratio	Lower	Upper
278	100		
139	13.2	9.3	13.9
279	32.0	21.6	32.4



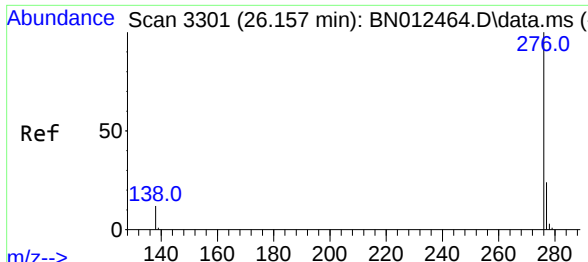

#41
Benzo(g,h,i)perylene
Concen: 0.37 ng
RT: 26.157 min Scan# 3301
Delta R.T. 0.000 min
Lab File: BN012489.D
Acq: 02 Nov 2020 14:19

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	276	Resp:	4921
Ion	Ratio	Lower	Upper
276	100		
277	27.2	19.8	29.8
138	15.5	11.7	17.5

