


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110220\
 Data File : BN012485.D
 Acq On : 02 Nov 2020 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN103020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 30 14:49:10 2020

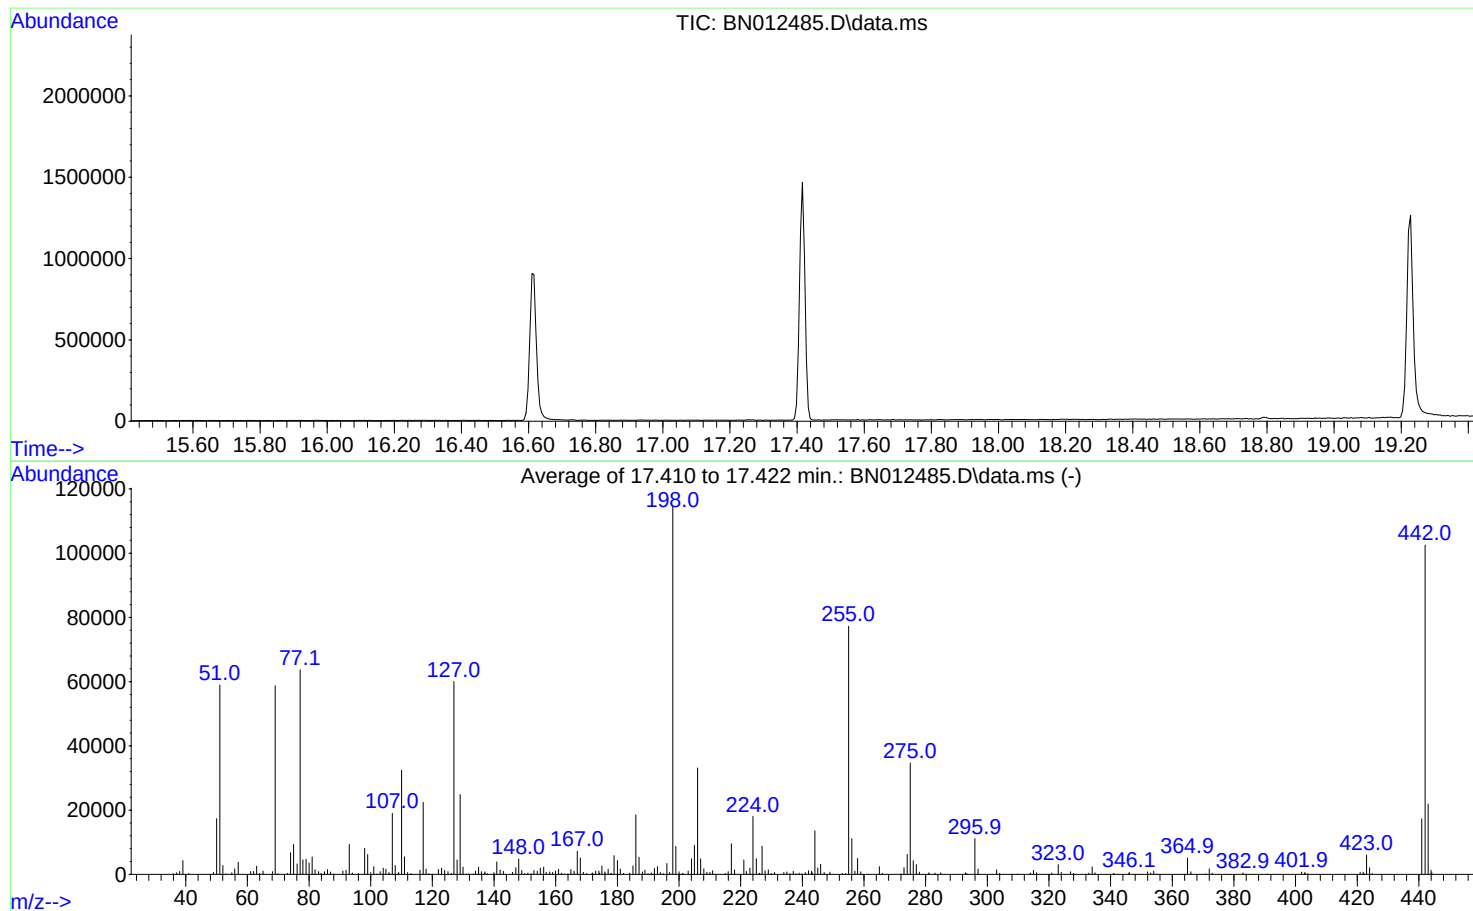

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	58963	PASS
68	69	0.00	2	1.5	857	PASS
69	198	0.00	100	51.3	58715	PASS
70	69	0.00	2	0.4	213	PASS
127	198	10	80	52.4	60045	PASS
197	198	0.00	2	0.5	547	PASS
198	198	100	100	100.0	114533	PASS
199	198	5	9	7.6	8691	PASS
275	198	10	60	30.3	34693	PASS
365	198	1	100	4.4	5072	PASS
441	198	0.01	100	15.1	17315	PASS
442	198	50	100	89.5	102520	PASS
443	442	15	24	21.4	21907	PASS