


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110221\  
Data File : BN017240.D  
Acq On : 02 Nov 2021 14:24  
Operator : CG/JU  
Sample : SSTD16041  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SSTD160241

Manual IntegrationsAPPROVED

Quant Time: Nov 02 15:39:30 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN110221.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Nov 02 15:36:06 2021  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2021  
Supervised By :mohammad ahmed 11/08/2021

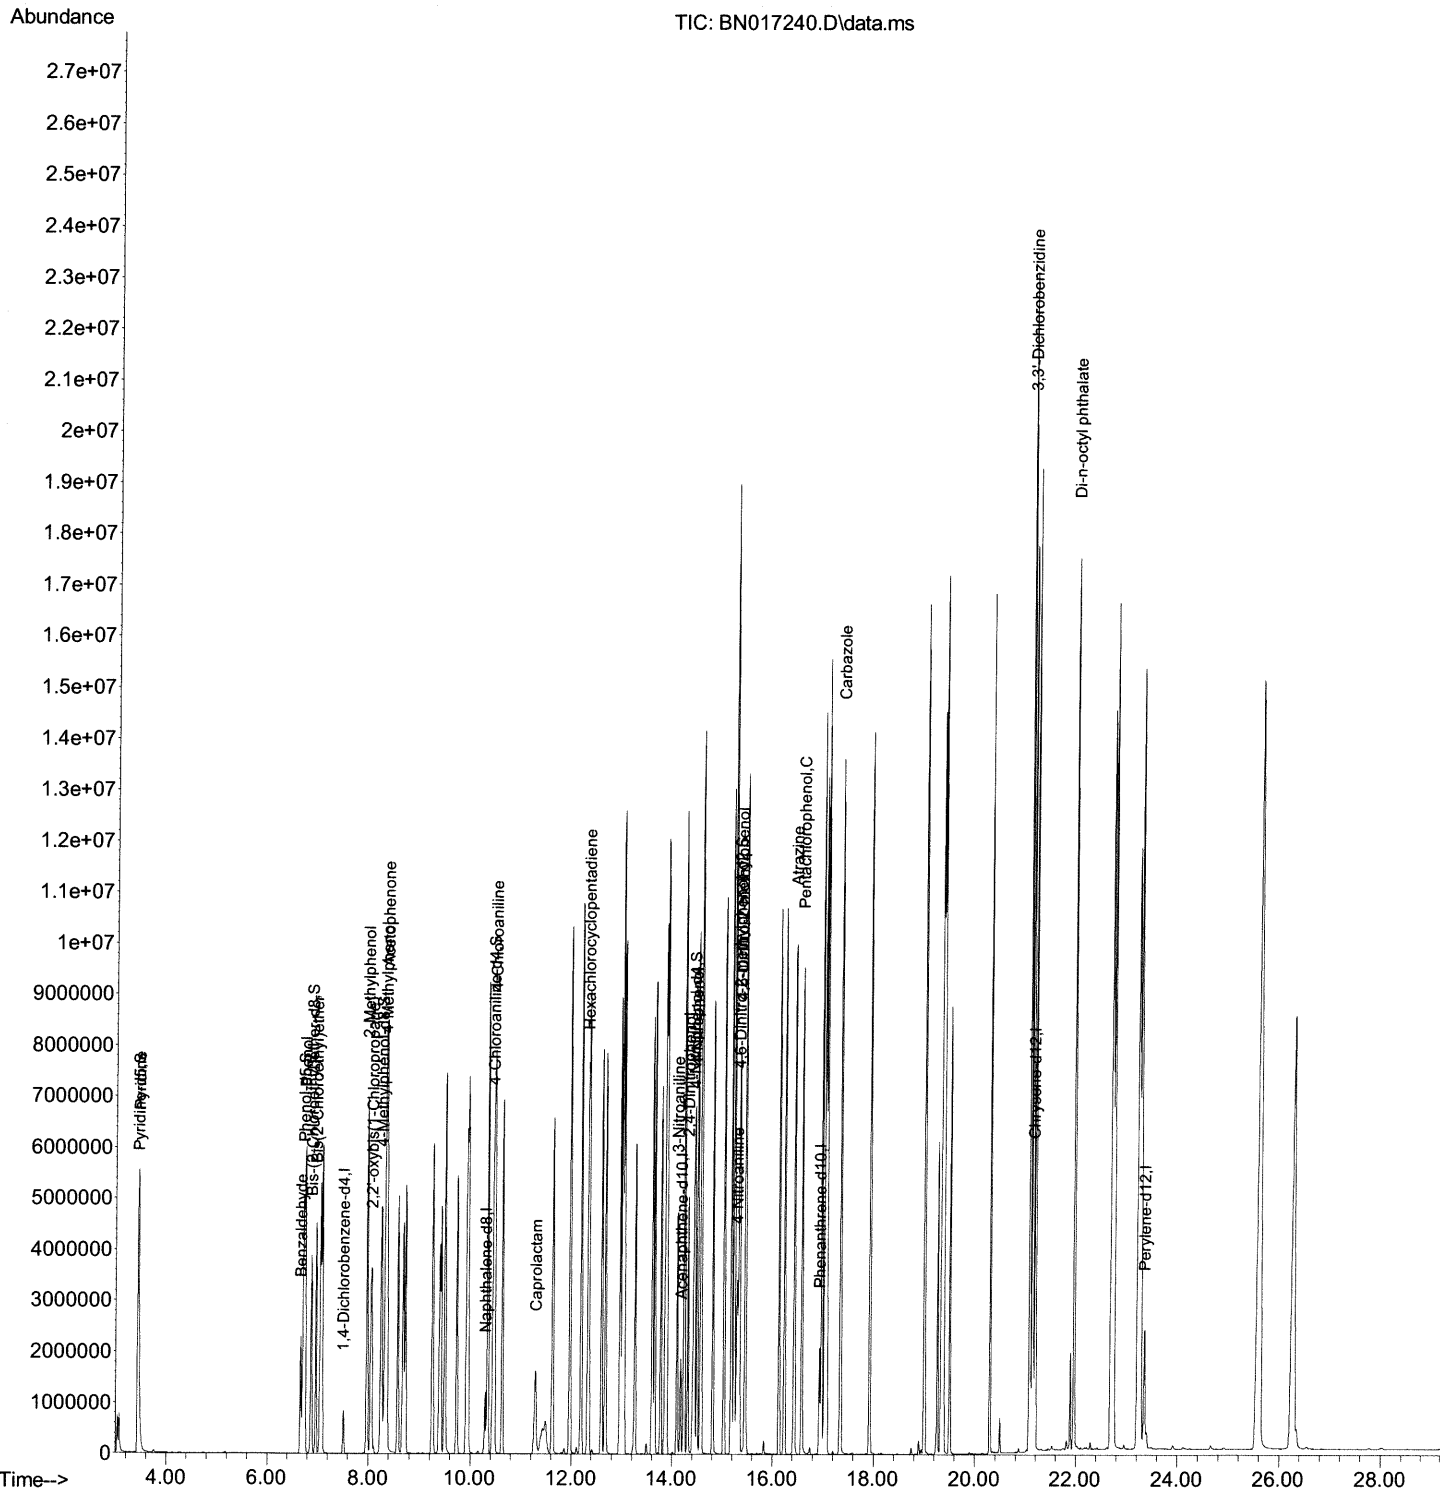

# Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110221\  
 Data File : BN017240.D  
 Acq On : 02 Nov 2021 14:24  
 Operator : CG/JU  
 Sample : SSTD16041  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTD160241

Manual IntegrationsAPPROVED

Quant Time: Nov 02 15:39:30 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN110221.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Nov 02 15:36:06 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2021  
 Supervised By :mohammad ahmed 11/08/2021

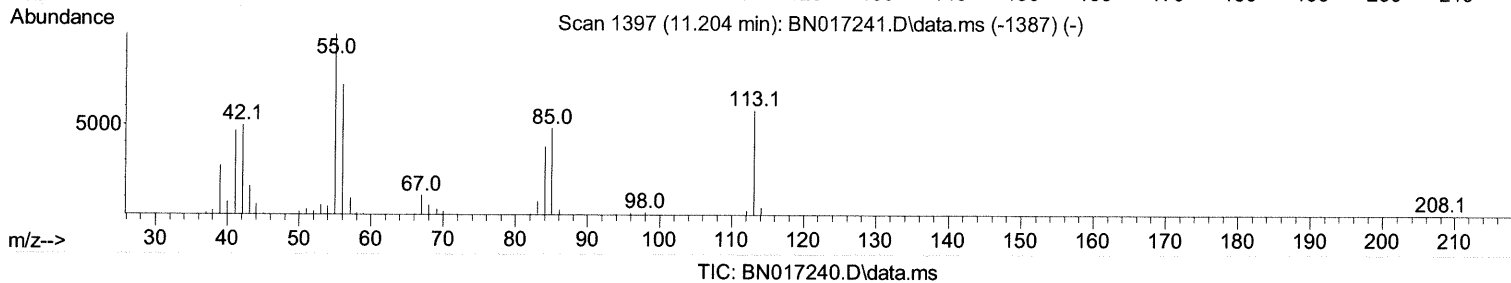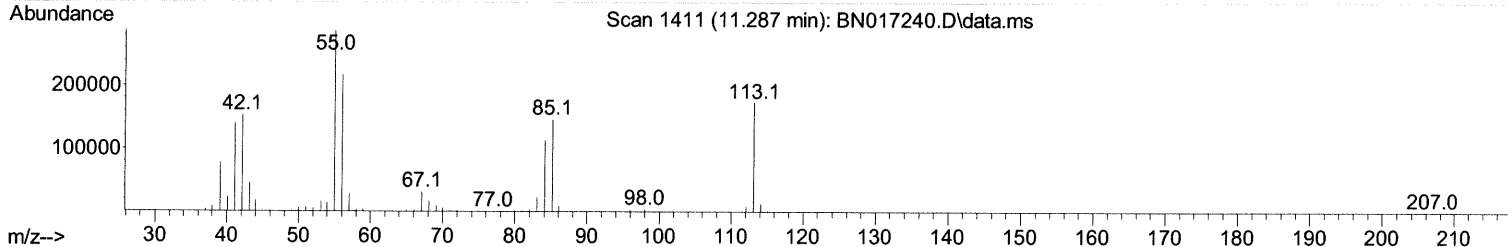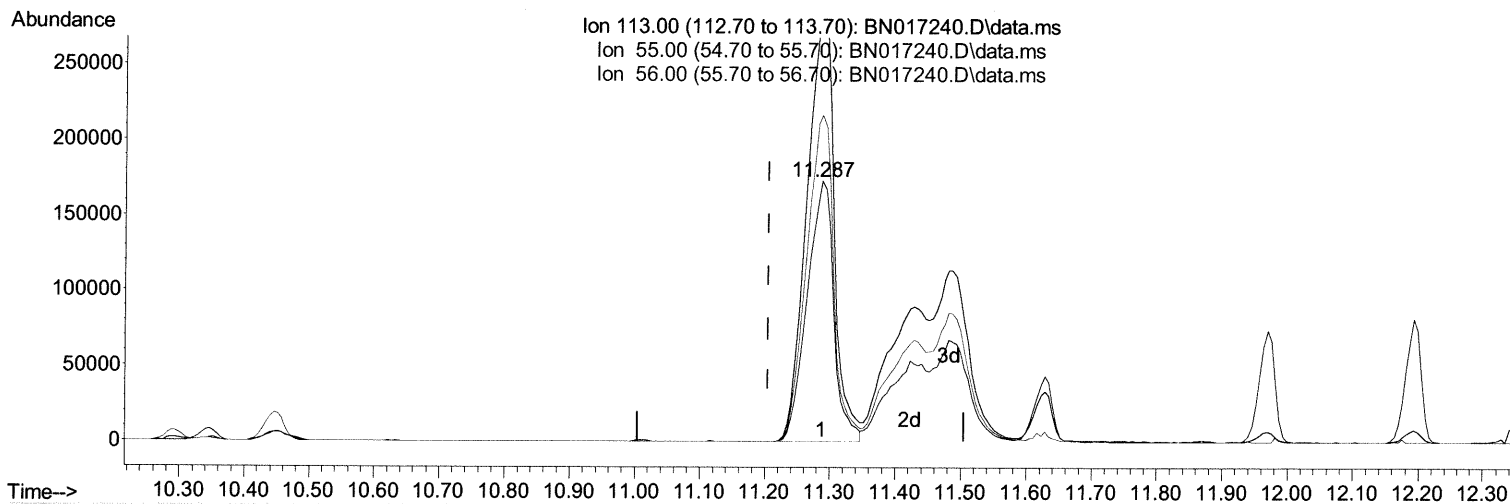

## (34) Caprolactam

11.287min (+ 0.082) 87.08 ng/ul

response 490353

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	172.30	166.00
56.00	123.70	125.31
0.00	0.00	0.00

# Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110221\  
 Data File : BN017240.D  
 Acq On : 02 Nov 2021 14:24  
 Operator : CG/JU  
 Sample : SSTD16041  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTD160241

Manual IntegrationsAPPROVED

Quant Time: Nov 02 15:39:30 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN110221.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Nov 02 15:36:06 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2021  
 Supervised By :mohammad ahmed 11/08/2021

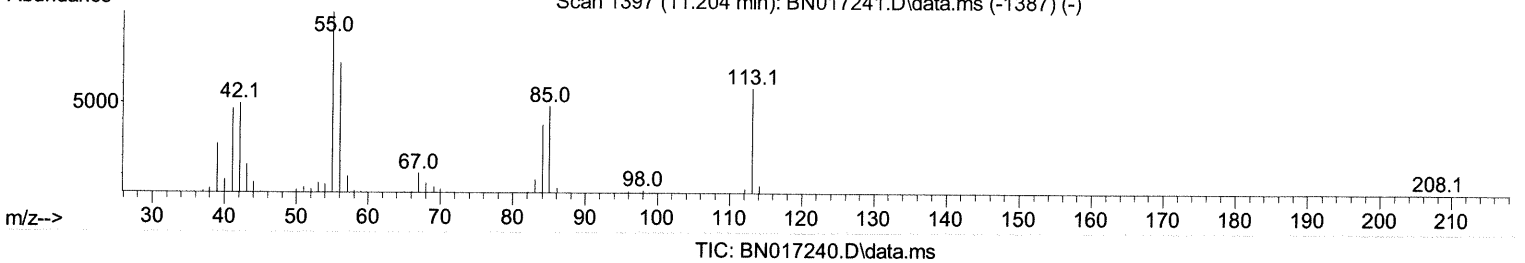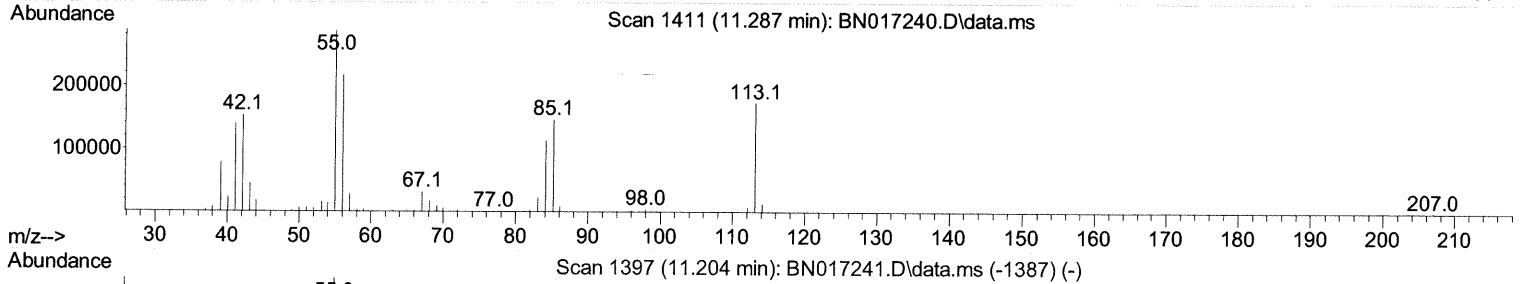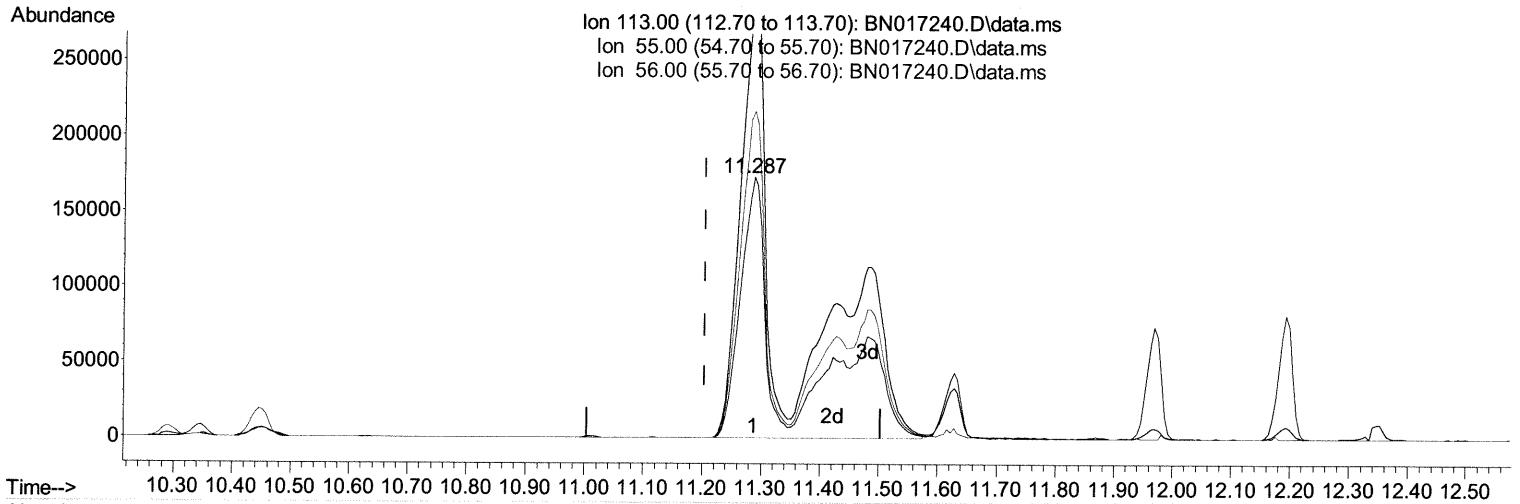

## (34) Caprolactam

11.287min (+ 0.082) 169.27 ng/ul m 11/04/2021

response 953181

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	172.30	166.00
56.00	123.70	125.31
0.00	0.00	0.00

# Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110221\  
 Data File : BN017240.D  
 Acq On : 02 Nov 2021 14:24  
 Operator : CG/JU  
 Sample : SSTD16041  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTD160241

Manual IntegrationsAPPROVED

Quant Time: Nov 02 15:39:30 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN110221.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Nov 02 15:36:06 2021  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2021  
 Supervised By :mohammad ahmed 11/08/2021

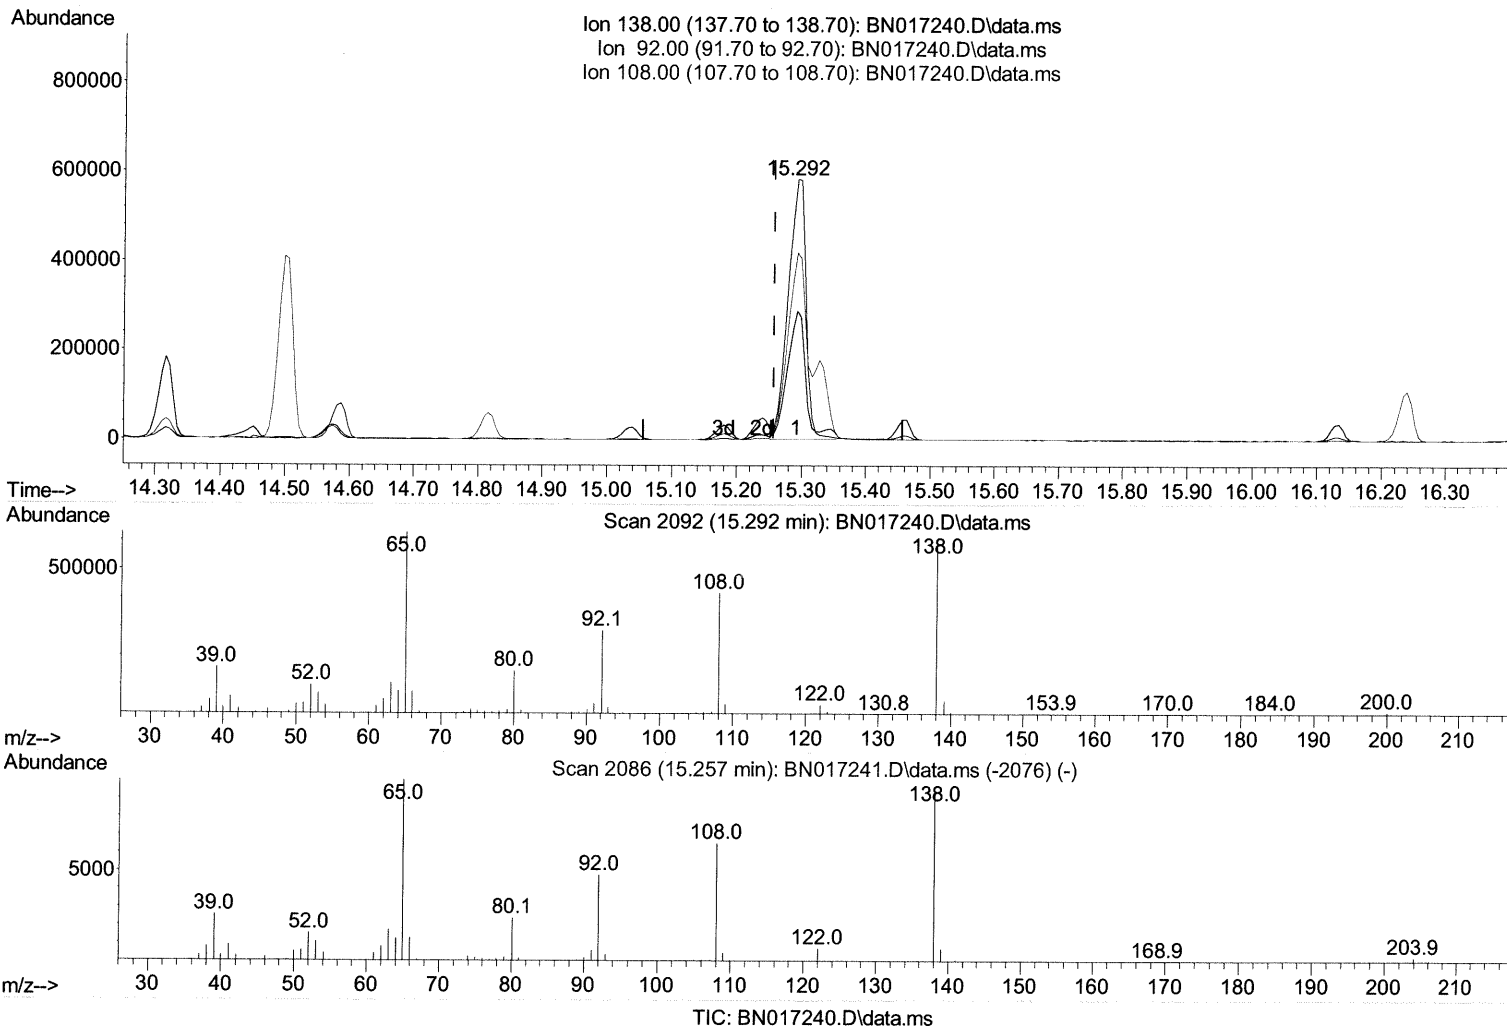

(63) 4-Nitroaniline

15.292min (+ 0.035) 104.07 ng/ul

response 1126677

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	50.40	49.41
108.00	68.90	71.75
0.00	0.00	0.00

## Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110221\  
Data File : BN017240.D  
Acq On : 02 Nov 2021 14:24  
Operator : CG/JU  
Sample : SSTD16041  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SSTD160241

Manual IntegrationsAPPROVED

Quant Time: Nov 02 15:39:30 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN110221.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Nov 02 15:36:06 2021  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/02/2021  
Supervised By :mohammad ahmed 11/08/2021

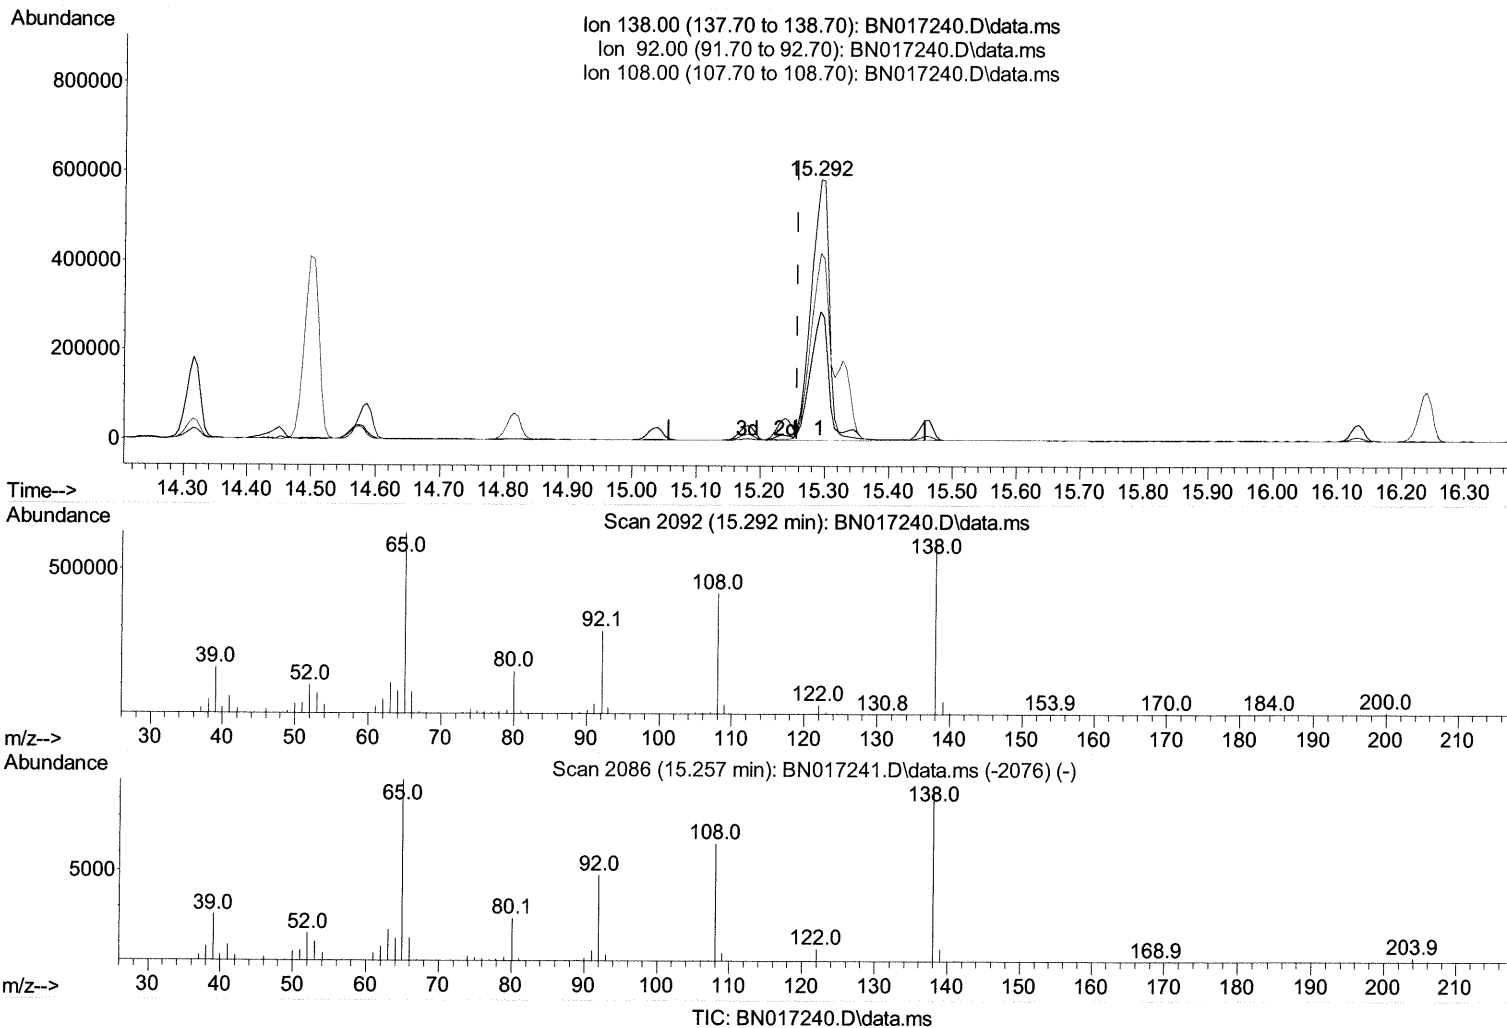

(63) 4-Nitroaniline

15.292min (+ 0.035) 111.70 ng/ul m 11/04/2021

response 1209292

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	50.40	49.41
108.00	68.90	71.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110221\  
 Data File : BN017240.D  
 Acq On : 02 Nov 2021 14:24  
 Operator : CG/JU  
 Sample : SSTD16041  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTD160241

## Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/02/2021  
 Supervised By :mohammad ahmed 11/08/2021

Quant Time: Nov 02 15:39:30 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN110221.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Nov 02 15:36:06 2021  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.510	152	219954	20.000 ng/ul	0.00
20) Naphthalene-d8	10.293	136	1003156	20.000 ng/ul	0.00
38) Acenaphthene-d10	14.175	164	641151	20.000 ng/ul	0.00
64) Phenanthrene-d10	16.933	188	1316701	20.000 ng/ul	0.01
79) Chrysene-d12	21.151	240	1206512	20.000 ng/ul	0.01
88) Perylene-d12	23.351	264	1448356	20.000 ng/ul	0.01
System Monitoring Compounds					
3) 1,4-Dioxane-d8	0.000	96	0d	0.000 ng/ul	
4) Pyridine-d5	3.428	84	2502800	153.883 ng/ul	0.00
7) Phenol-d5	6.716	99	3274488	160.210 ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.875	67	1823863	150.342 ng/ul	0.01
11) 2-Chlorophenol-d4	0.000	132	0d	0.000 ng/ul	
15) 4-Methylphenol-d8	8.252	113	2576945	154.449 ng/ul	0.02
21) Nitrobenzene-d5	0.000	128	0d	0.000 ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0d	0.000 ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000 ng/ul	
31) 4-Chloroaniline-d4	10.446	131	3623673	154.406 ng/ul	0.01
46) Dimethylphthalate-d6	0.000	166	0d	0.000 ng/ul	
49) Acenaphthylene-d8	0.000	160	0d	0.000 ng/ul	
54) 4-Nitrophenol-d4	14.434	143	1517431	160.223 ng/ul	0.04
60) Fluorene-d10	0.000	176	0d	0.000 ng/ul	
65) 4,6-Dinitro-2-methylph...	15.328	200	1403251	164.583 ng/ul	0.02
73) Anthracene-d10	0.000	188	0d	0.000 ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000 ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000 ng/ul	
Target Compounds					
5) Pyridine	3.446	79	2511915	152.612 ng/ul	98
6) Benzaldehyde	6.663	77	777827	63.871 ng/ul	100
8) Phenol	6.746	94	3195046	154.525 ng/ul	98
10) Bis(2-Chloroethyl)ether	6.969	93	2431711	149.674 ng/ul	97
13) 2-Methylphenol	7.975	108	2445177	155.438 ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.057	45	3495747	146.664 ng/ul	98
16) Acetophenone	8.352	105	3522673	142.459 ng/ul	98
18) 4-Methylphenol	8.328	108	2563643	147.514 ng/ul	98
32) 4-Chloroaniline	10.475	127	3513246	151.323 ng/ul	100
34) Caprolactam	11.287	113	953181m	169.273 ng/ul>	1164/1134
40) Hexachlorocyclopentadiene	12.322	237	1952936	164.431 ng/ul	95
51) 3-Nitroaniline	14.110	138	1365857	124.668 ng/ul	97
53) 2,4-Dinitrophenol	14.316	184	1136025	187.640 ng/ul	97
55) 4-Nitrophenol	14.451	109	1042598	156.002 ng/ul	93
63) 4-Nitroaniline	15.292	138	1209292m	111.705 ng/ul>	1164/1134
66) 4,6-Dinitro-2-methylph...	15.345	198	1361432	160.042 ng/ul#	98
70) Atrazine	16.439	200	2195958	149.327 ng/ul	98
71) Pentachlorophenol	16.586	266	1650723	168.400 ng/ul	96
77) Carbazole	17.351	167	9140686	140.924 ng/ul	98
84) 3,3'-Dichlorobenzidine	21.080	252	3599895	134.036 ng/ul#	93
89) Di-n-octyl phthalate	21.963	149	12619938	119.213 ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN110221\  
Data File : BN017240.D  
Acq On : 02 Nov 2021 14:24  
Operator : CG/JU  
Sample : SSTD16041  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SSTD160241

**Manual IntegrationsAPPROVED**

Reviewed By :Jagrut Upadhyay 11/02/2021  
Supervised By :mohammad ahmed 11/08/2021

Quant Time: Nov 02 15:39:30 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN110221.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Nov 02 15:36:06 2021  
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
(#) = qualifier out of range (m) = manual integration (+) = signals summed						