

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
 Data File : BN017258.D
 Acq On : 03 Nov 2021 02:25
 Operator : CG/JU
 Sample : M4400-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG349

Quant Time: Nov 03 02:55:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 02 15:59:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	178895	20.000	ng/u1	0.00
20) Naphthalene-d8	10.287	136	801164	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.169	164	532789	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.922	188	1143126	20.000	ng/u1	0.00
79) Chrysene-d12	21.133	240	1235381	20.000	ng/u1	0.00
88) Perylene-d12	23.327	264	1364825	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.034	96	22342	4.936	ng/uL	0.00
4) Pyridine-d5	3.434	84	48036	3.803	ng/u1	0.00
7) Phenol-d5	6.699	99	102150	6.186	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.857	67	237792	24.125	ng/u1	0.00
11) 2-Chlorophenol-d4	7.046	132	277543	21.151	ng/u1	0.00
15) 4-Methylphenol-d8	8.228	113	197049	14.474	ng/u1	0.00
21) Nitrobenzene-d5	8.663	128	155949	25.088	ng/u1	0.00
24) 2-Nitrophenol-d4	9.381	143	170749	24.627	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.916	165	340654	27.326	ng/u1	0.00
31) 4-Chloroaniline-d4	10.434	131	303743	16.258	ng/u1	0.00
46) Dimethylphthalate-d6	13.592	166	1300778	32.928	ng/u1	0.00
49) Acenaphthylene-d8	13.857	160	1504204	30.274	ng/u1	0.00
54) 4-Nitrophenol-d4	14.392	143	35694	4.604	ng/u1	0.00
60) Fluorene-d10	15.169	176	1105449	32.793	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.298	200	188145	25.730	ng/u1	0.00
73) Anthracene-d10	17.022	188	1809736	33.547	ng/u1	0.00
81) Pyrene-d10	19.327	212	2189227	32.748	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.192	264	2370302	32.146	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.074	149	81920	1.603	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017258.D
Acq On : 03 Nov 2021 02:25
Operator : CG/JU
Sample : M4400-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG349

Quant Time: Nov 03 02:55:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 02 15:59:34 2021
Response via : Initial Calibration

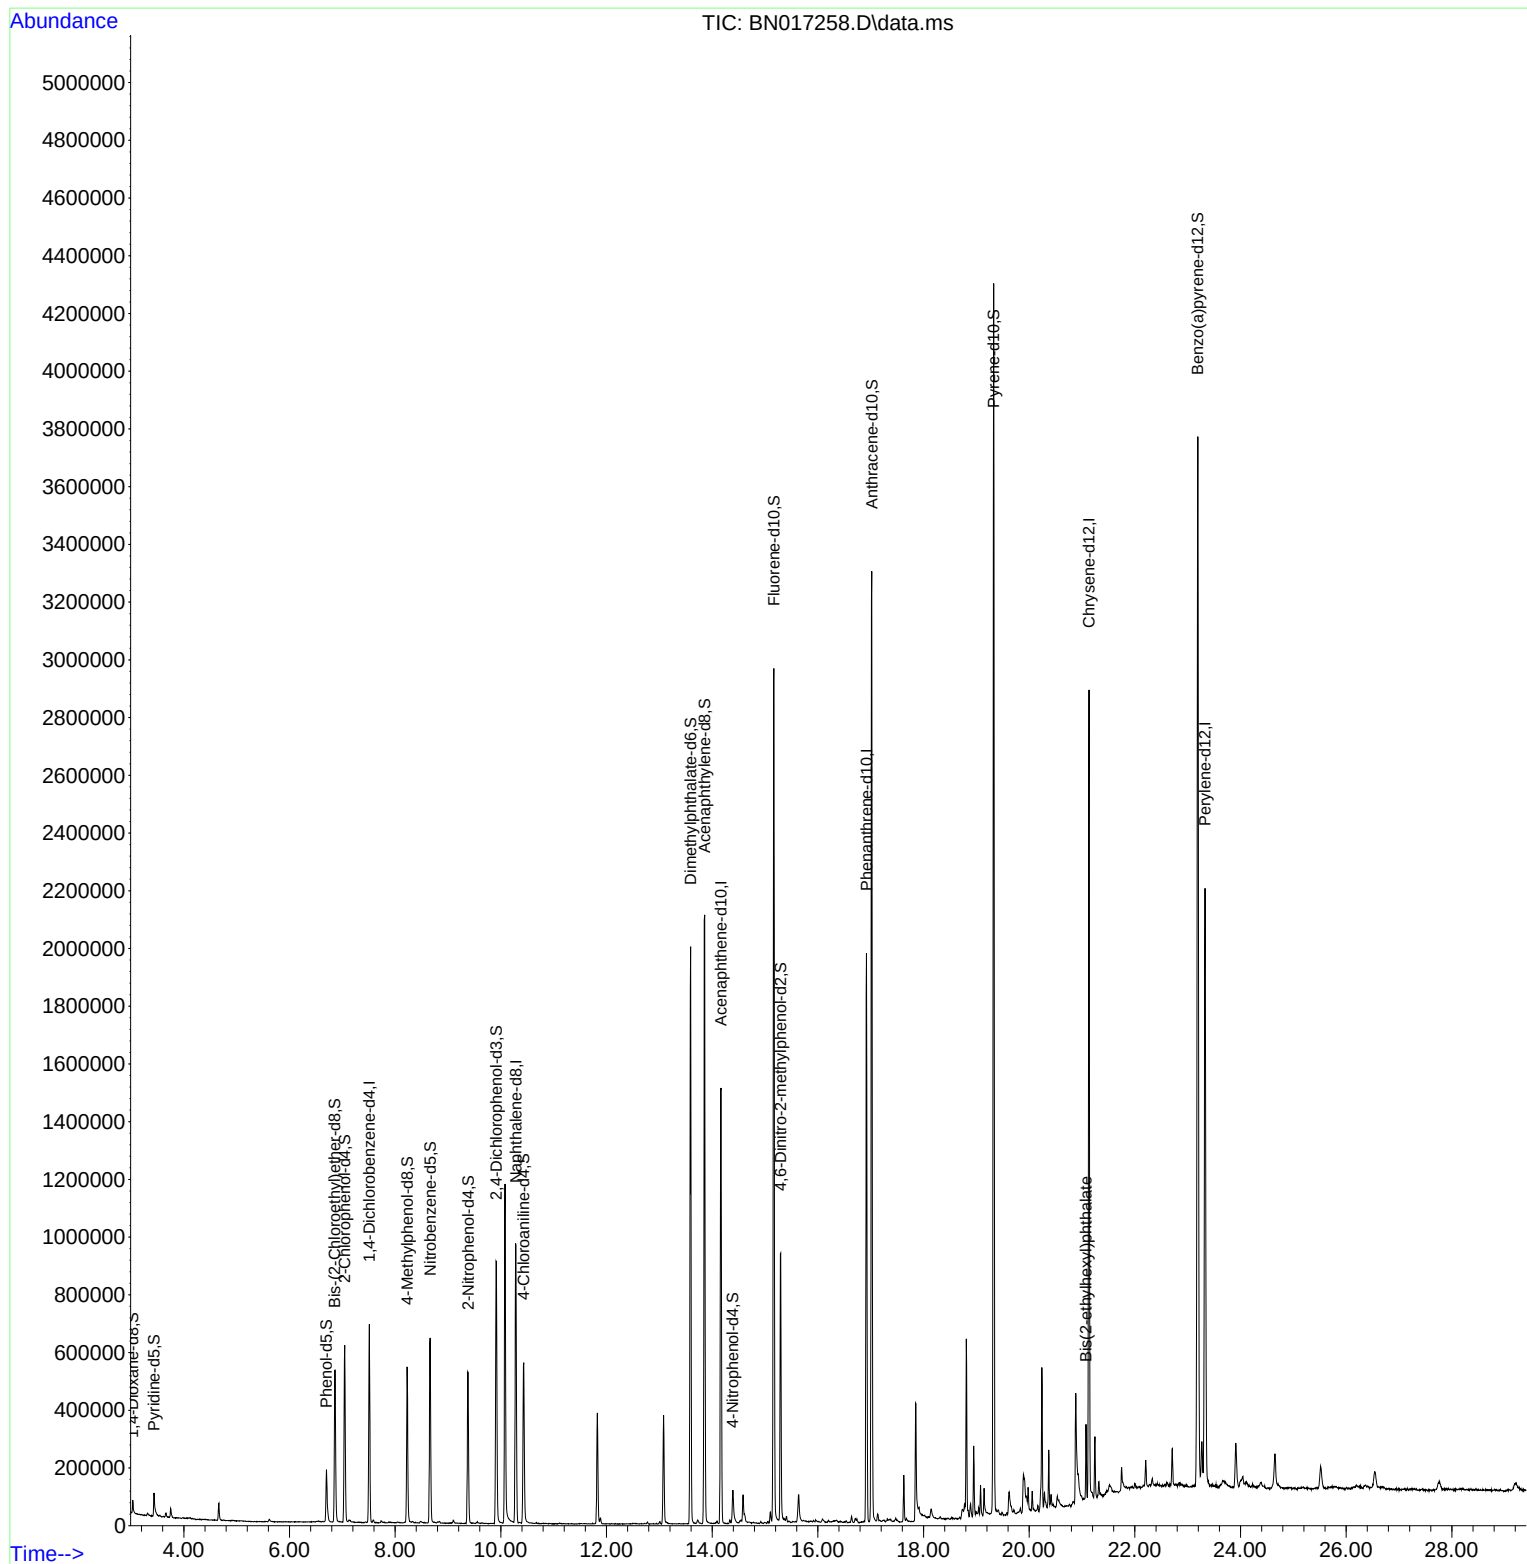

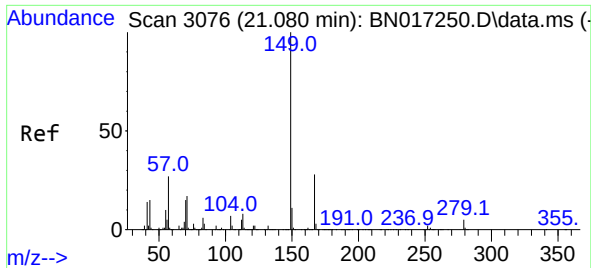

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.603 ng/ul
 RT: 21.074 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BN017258.D
 Acq: 03 Nov 2021 02:25

Instrument :
 BNA_N
 ClientSampleId :
 BG349

Tgt Ion:149 Resp: 81920
 Ion Ratio Lower Upper
 149 100
 167 26.9 21.6 32.4
 279 4.2 3.2 4.8

