

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
 Data File : BN017243.D
 Acq On : 02 Nov 2021 16:47
 Operator : CG/JU
 Sample : PB140385BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK385

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	4	8	17	rVB	50543	78746	1.18%	0.116%
2	3.423	71	74	95	rBV	617911	1082609	16.27%	1.592%
3	3.752	127	130	138	rVB	13885	21102	0.32%	0.031%
4	6.693	624	630	642	rBV	801034	1260472	18.94%	1.854%
5	6.858	652	658	672	rVB	681819	1047006	15.73%	1.540%
6	7.040	683	689	701	rBV	865260	1314860	19.76%	1.934%
7	7.511	762	769	779	rBV	947181	1477210	22.20%	2.173%
8	8.222	884	890	906	rBV	1017419	1644291	24.71%	2.418%
9	8.658	957	964	981	rBV	821329	1310076	19.69%	1.927%
10	9.375	1079	1086	1099	rBV	700484	1095161	16.46%	1.611%
11	9.910	1170	1177	1192	rBV	1032111	1664952	25.02%	2.449%
12	10.281	1233	1240	1253	rBV	1599903	2541726	38.20%	3.738%
13	10.428	1258	1265	1281	rBV	1091788	1842096	27.68%	2.709%
14	11.887	1506	1513	1521	rBV3	15960	27433	0.41%	0.040%
15	13.593	1796	1803	1816	rBV	2133325	2861075	43.00%	4.208%
16	13.851	1841	1847	1856	rBV	2303518	3434709	51.62%	5.052%
17	14.163	1894	1900	1910	rBV	2509726	3707378	55.72%	5.453%
18	14.387	1932	1938	1961	rBV	736023	1235283	18.56%	1.817%
19	15.169	2064	2071	2082	rBV	3036649	4356878	65.48%	6.408%
20	15.298	2086	2093	2106	rVV	998881	1332326	20.02%	1.960%
21	15.404	2108	2111	2116	rVB	18545	23386	0.35%	0.034%
22	16.710	2328	2333	2341	rVB2	11936	17461	0.26%	0.026%
23	16.922	2363	2369	2379	rBV	3272337	4534033	68.14%	6.668%
24	17.022	2379	2386	2403	rVB	3543956	4913923	73.85%	7.227%
25	17.857	2521	2528	2534	rBV4	3635	8540	0.13%	0.013%
26	18.892	2697	2704	2708	rBV	36098	51153	0.77%	0.075%
27	18.963	2711	2716	2724	rVV	37541	53226	0.80%	0.078%
28	19.328	2769	2778	2791	rBV	4267604	5816793	87.42%	8.555%
29	20.357	2949	2953	2955	rBV2	9592	12305	0.18%	0.018%
30	20.880	3040	3042	3046	rBV5	6691	9106	0.14%	0.013%
31	21.133	3080	3085	3097	rBV	4131554	5239379	78.74%	7.706%
32	21.322	3115	3117	3121	rBV5	12219	13557	0.20%	0.020%
33	21.751	3187	3190	3195	rBV2	21773	28324	0.43%	0.042%
34	22.210	3265	3268	3272	rBV2	57192	69001	1.04%	0.101%
35	22.710	3349	3353	3358	rVB	98026	138920	2.09%	0.204%
36	23.198	3428	3436	3444	rBV2	3603706	6654099	100.00%	9.786%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017243.D
Acq On : 02 Nov 2021 16:47
Operator : CG/JU
Sample : PB140385BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK385

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Title : SVOA CALIBRATION

37	23.274	3444	3449	3452	rVV	171116	301872	4.54%	0.444%
38	23.333	3452	3459	3475	rVB2	2988279	5540310	83.26%	8.148%
39	23.916	3552	3558	3565	rVB2	164206	304731	4.58%	0.448%
40	24.657	3678	3684	3696	rVB3	159497	355263	5.34%	0.522%
41	25.527	3826	3832	3841	rVB	123563	303098	4.56%	0.446%
42	26.551	4000	4006	4018	rVB3	93875	269207	4.05%	0.396%


Sum of corrected areas: 67993076

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017243.D
Acq On : 02 Nov 2021 16:47
Operator : CG/JU
Sample : PB140385BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK385

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

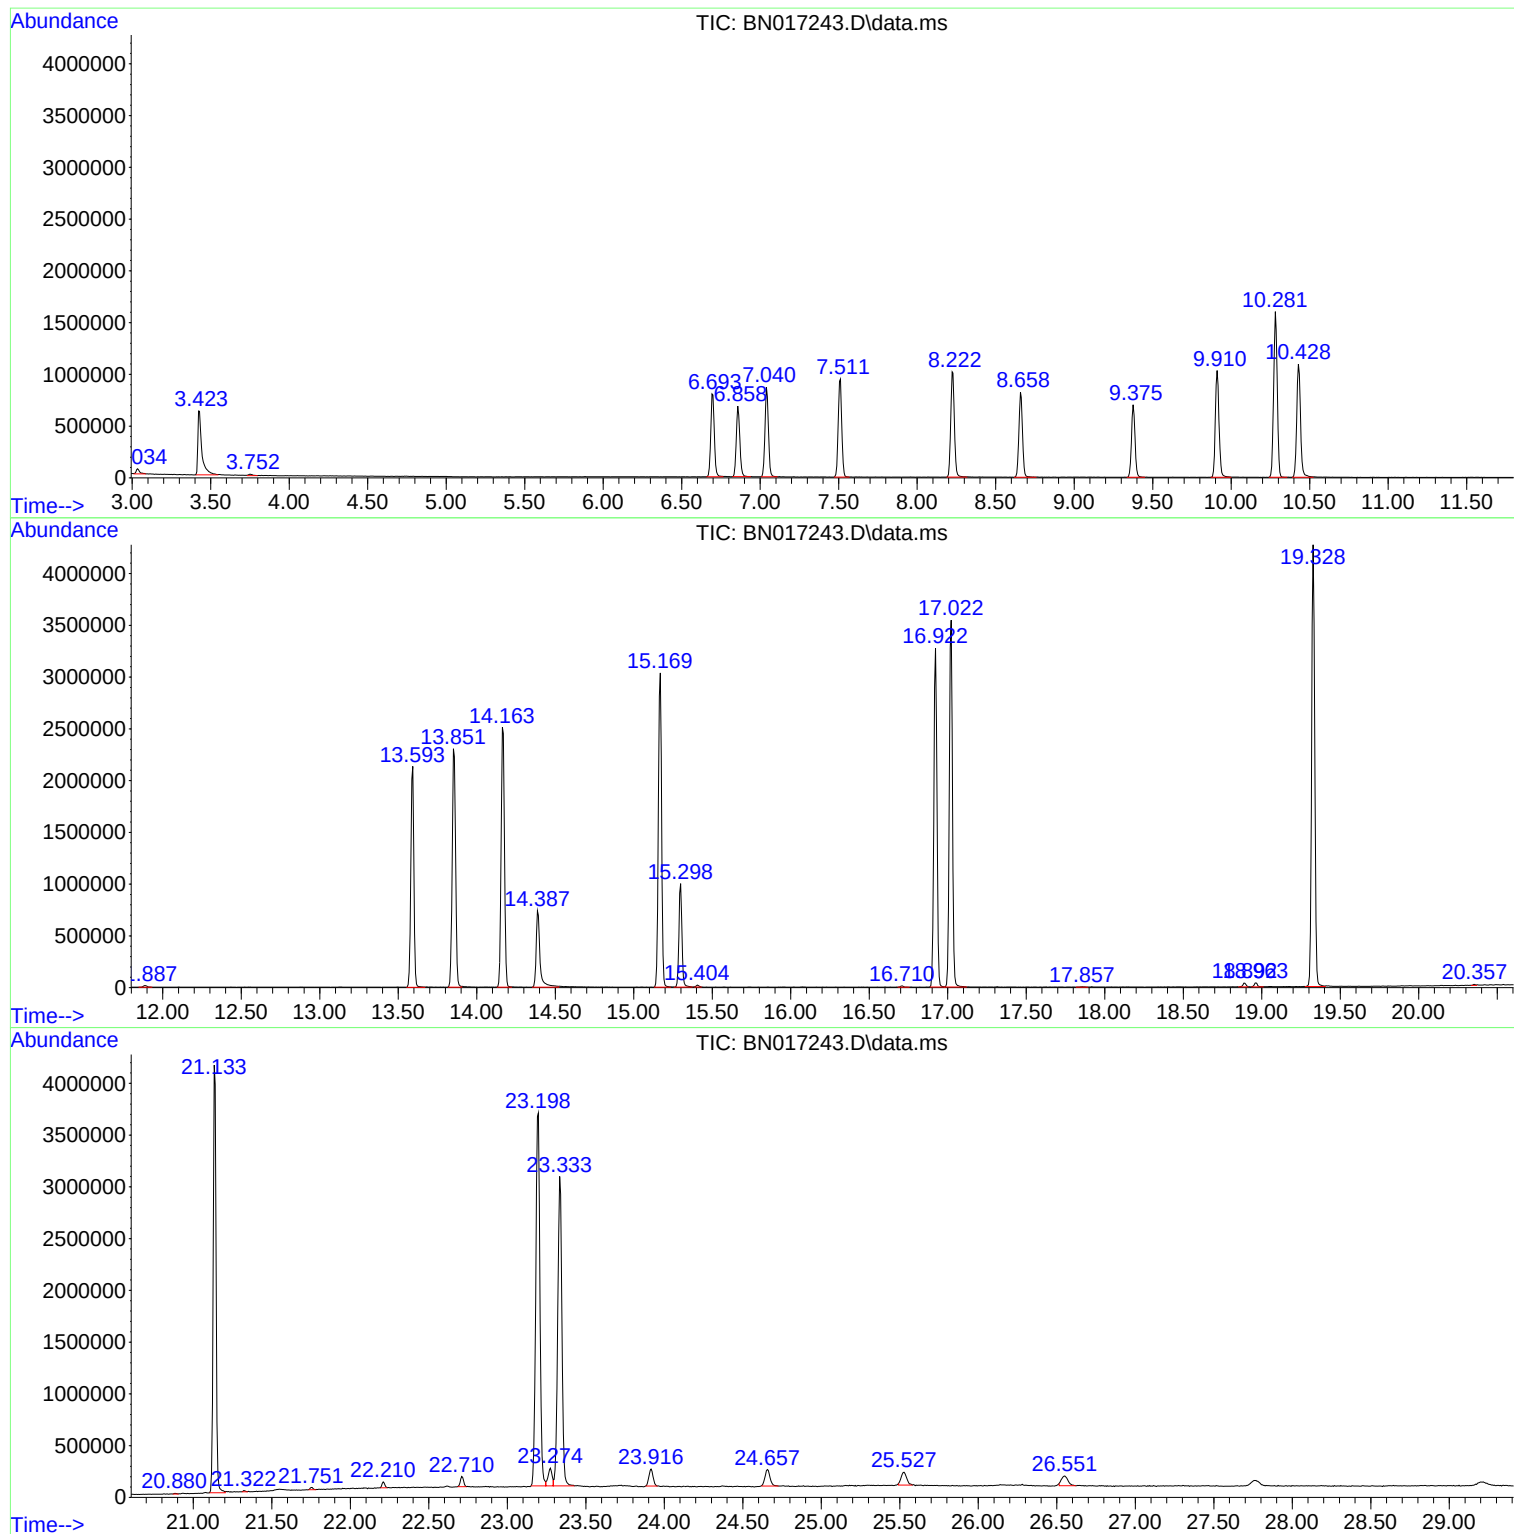

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017243.D
Acq On : 02 Nov 2021 16:47
Operator : CG/JU
Sample : PB140385BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK385

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017243.D
Acq On : 02 Nov 2021 16:47
Operator : CG/JU
Sample : PB140385BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK385

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc