

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
 Data File : BN017251.D
 Acq On : 02 Nov 2021 22:13
 Operator : CG/JU
 Sample : PB140353BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	5	8	18	rVB	54595	78296	1.17%	0.117%
2	3.428	71	75	101	rVB	694626	1135155	16.91%	1.698%
3	3.752	127	130	137	rVB	27050	37909	0.56%	0.057%
4	6.699	625	631	643	rBV	852743	1296503	19.32%	1.940%
5	6.863	653	659	669	rBV	688084	1084892	16.16%	1.623%
6	7.046	683	690	700	rBV	869344	1349942	20.11%	2.020%
7	7.511	762	769	782	rBV	912726	1391161	20.73%	2.081%
8	8.228	883	891	907	rBV	1087743	1692811	25.22%	2.533%
9	8.663	958	965	978	rBV	851590	1316892	19.62%	1.970%
10	9.381	1080	1087	1098	rBV	689919	1110247	16.54%	1.661%
11	9.916	1171	1178	1191	rBV	1017723	1708827	25.46%	2.557%
12	10.287	1233	1241	1249	rBV	1388417	2319429	34.56%	3.470%
13	10.434	1258	1266	1283	rBV	1081084	1879630	28.01%	2.812%
14	11.887	1508	1513	1520	rBV2	17156	30168	0.45%	0.045%
15	13.593	1796	1803	1817	rBV	2099712	2811316	41.89%	4.206%
16	13.857	1841	1848	1862	rBV	2373897	3452943	51.45%	5.166%
17	14.169	1894	1901	1913	rBV	2317712	3342010	49.79%	5.000%
18	14.393	1932	1939	1958	rBV	694527	1203382	17.93%	1.800%
19	15.169	2064	2071	2084	rBV	2998167	4322675	64.40%	6.468%
20	15.298	2087	2093	2107	rVV	1001523	1322642	19.71%	1.979%
21	15.410	2107	2112	2116	rVB	18018	26292	0.39%	0.039%
22	16.710	2328	2333	2339	rBV2	10141	17308	0.26%	0.026%
23	16.922	2362	2369	2379	rBV	2979649	4074919	60.71%	6.097%
24	17.022	2379	2386	2402	rVV	3482692	4856713	72.36%	7.267%
25	18.892	2697	2704	2709	rBV2	37222	53040	0.79%	0.079%
26	18.963	2711	2716	2720	rBV	37432	49323	0.73%	0.074%
27	19.328	2769	2778	2790	rBV	4318101	5864028	87.37%	8.774%
28	20.351	2949	2952	2954	rBV4	10398	11965	0.18%	0.018%
29	21.133	3079	3085	3099	rBV	4009052	4979137	74.19%	7.450%
30	21.316	3114	3116	3120	rBV3	11183	15624	0.23%	0.023%
31	21.751	3187	3190	3196	rVB2	28771	32150	0.48%	0.048%
32	22.210	3264	3268	3273	rVB	60853	79225	1.18%	0.119%
33	22.710	3349	3353	3358	rVB2	103173	139090	2.07%	0.208%
34	23.192	3427	3435	3444	rBV	3725568	6711734	100.00%	10.042%
35	23.269	3444	3448	3452	rVV	187494	317375	4.73%	0.475%
36	23.333	3452	3459	3475	rVB2	2955476	5537069	82.50%	8.285%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017251.D
Acq On : 02 Nov 2021 22:13
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK353

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Title : SVOA CALIBRATION

37	23.910	3552	3557	3566	rVB	168309	312105	4.65%	0.467%
38	24.651	3677	3683	3695	rVB2	159873	344852	5.14%	0.516%
39	25.521	3825	3831	3841	rVB2	110349	276480	4.12%	0.414%
40	26.545	3999	4005	4019	rVB3	88676	250856	3.74%	0.375%




Sum of corrected areas: 66836115

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017251.D
Acq On : 02 Nov 2021 22:13
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

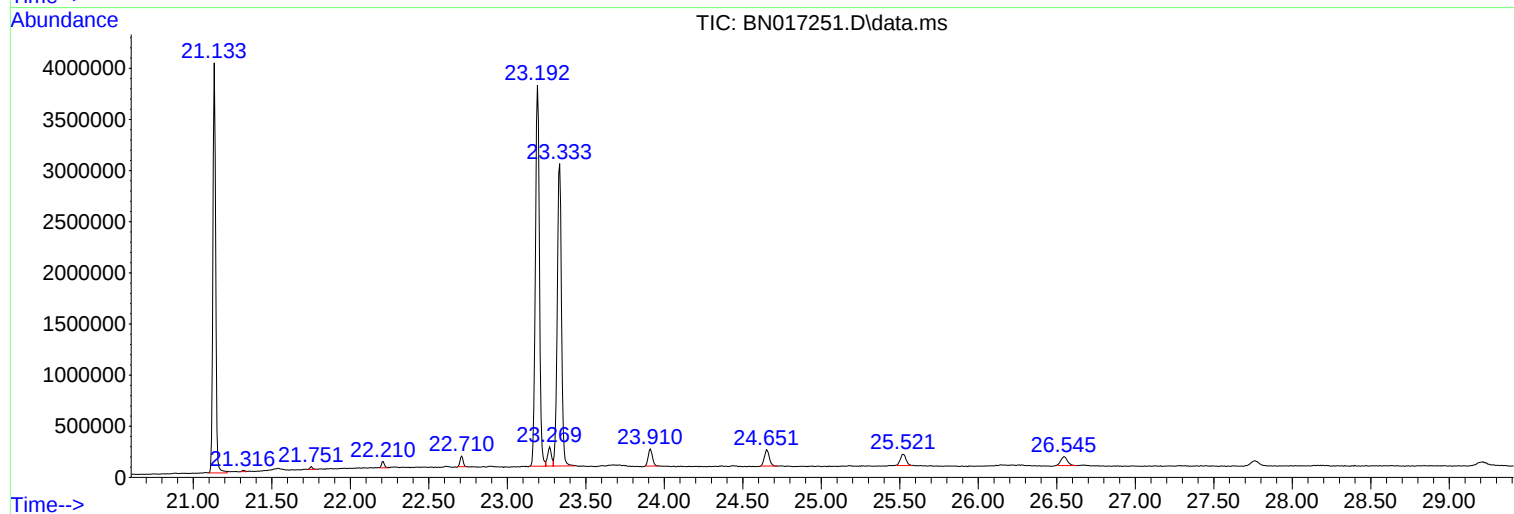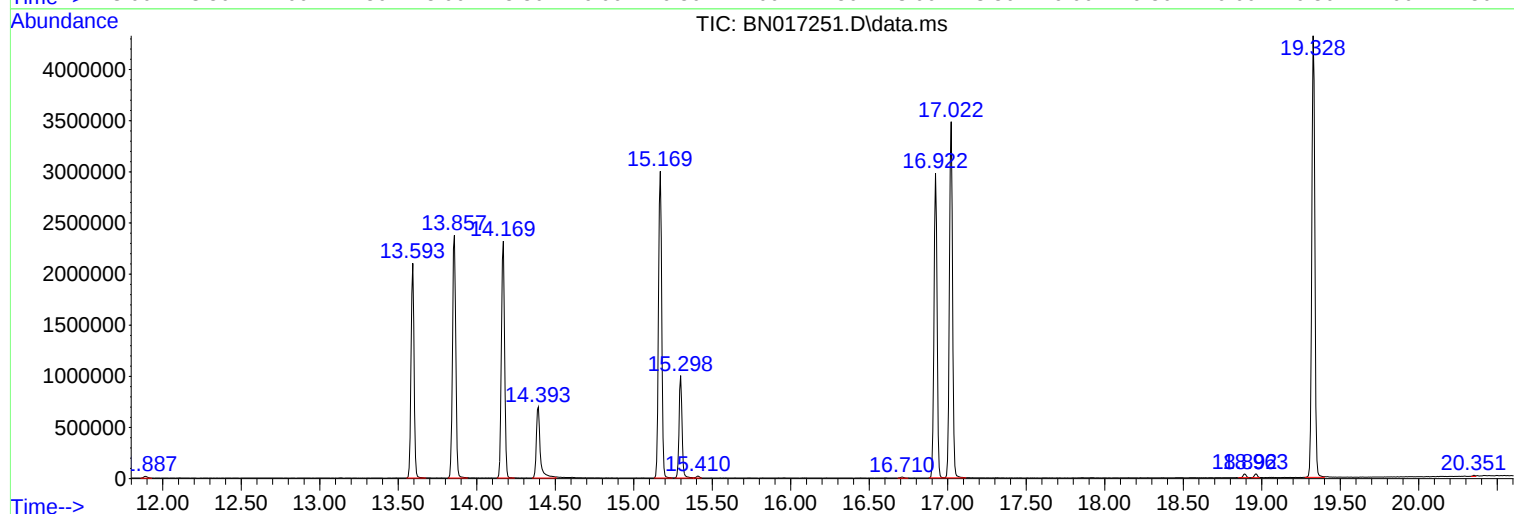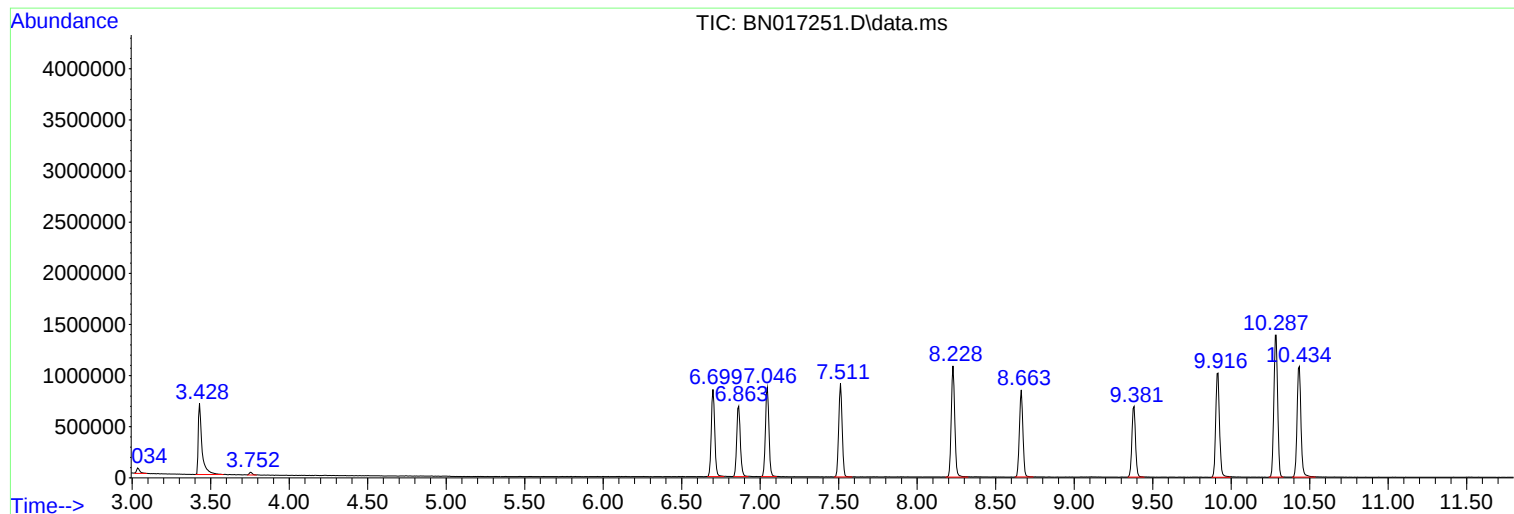

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017251.D
Acq On : 02 Nov 2021 22:13
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017251.D
Acq On : 02 Nov 2021 22:13
Operator : CG/JU
Sample : PB140353BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK353

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------