

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
 Data File : BN017257.D
 Acq On : 03 Nov 2021 01:49
 Operator : CG/JU
 Sample : M4400-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG335

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
 Title : SVOA CALIBRATION

Signal : TIC: BN017257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	5	8	17	rVB	47836	67701	0.94%	0.092%
2	3.434	73	76	90	rBV	174355	294070	4.10%	0.399%
3	3.663	111	115	121	rVB2	20115	32151	0.45%	0.044%
4	3.757	127	131	135	rVB2	17418	23296	0.33%	0.032%
5	5.616	444	447	454	rVB3	6908	11070	0.15%	0.015%
6	6.699	623	631	640	rBV	172657	290863	4.06%	0.395%
7	6.857	652	658	672	rBV	640801	1034436	14.43%	1.404%
8	7.046	683	690	701	rBV	601875	945763	13.20%	1.283%
9	7.510	762	769	777	rBV	1210237	1824554	25.46%	2.476%
10	7.587	778	782	789	rVB3	10344	17929	0.25%	0.024%
11	8.228	885	891	902	rBV	511878	788010	10.99%	1.069%
12	8.663	958	965	973	rBV	798787	1278399	17.84%	1.735%
13	8.840	986	995	1000	rVB7	4019	10590	0.15%	0.014%
14	9.104	1034	1040	1049	rVB2	15613	27787	0.39%	0.038%
15	9.375	1080	1086	1099	rBV	567205	920011	12.84%	1.248%
16	9.910	1169	1177	1193	rBV	855027	1446913	20.19%	1.963%
17	10.081	1200	1206	1214	rBV	41404	71306	0.99%	0.097%
18	10.287	1233	1241	1249	rBV	1844847	3068002	42.80%	4.163%
19	10.428	1258	1265	1278	rBV	889353	1555311	21.70%	2.110%
20	11.886	1508	1513	1521	rBV	18325	31325	0.44%	0.043%
21	12.775	1660	1664	1669	rVB4	5944	8610	0.12%	0.012%
22	13.010	1700	1704	1709	rBV	10802	15786	0.22%	0.021%
23	13.081	1711	1716	1721	rBV3	5845	10354	0.14%	0.014%
24	13.592	1796	1803	1816	rBV	2211660	3028152	42.25%	4.109%
25	13.857	1841	1848	1860	rBV	2340692	3508507	48.95%	4.760%
26	14.092	1882	1888	1894	rBV4	9332	12814	0.18%	0.017%
27	14.169	1894	1901	1912	rBV	3036066	4420332	61.67%	5.998%
28	14.392	1934	1939	1957	rVV	99984	217799	3.04%	0.296%
29	14.551	1959	1966	1971	rVV7	9009	21194	0.30%	0.029%
30	14.610	1971	1976	1981	rVB5	12690	19457	0.27%	0.026%
31	14.698	1988	1991	1999	rVB8	4959	9084	0.13%	0.012%
32	14.992	2036	2041	2043	rBV3	5242	7253	0.10%	0.010%
33	15.051	2048	2051	2057	rVB4	9536	13442	0.19%	0.018%
34	15.169	2064	2071	2085	rBV	3308673	4707662	65.68%	6.388%
35	15.298	2085	2093	2101	rBV	969876	1307589	18.24%	1.774%
36	15.404	2108	2111	2116	rVB	20393	28001	0.39%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
 Data File : BN017257.D
 Acq On : 03 Nov 2021 01:49
 Operator : CG/JU
 Sample : M4400-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG335

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
 Title : SVOA CALIBRATION

37	15.622	2141	2148	2151	rVB4	8768	12737	0.18%	0.017%
38	15.922	2195	2199	2202	rVV3	8723	11845	0.17%	0.016%
39	15.963	2202	2206	2210	rVB6	5731	10555	0.15%	0.014%
40	16.080	2219	2226	2230	rBV5	8801	17455	0.24%	0.024%

41	16.433	2282	2286	2289	rBV3	5707	8619	0.12%	0.012%
42	16.498	2293	2297	2301	rBV6	4998	9580	0.13%	0.013%
43	16.710	2327	2333	2336	rBV3	22241	36819	0.51%	0.050%
44	16.739	2336	2338	2342	rVB4	8911	9397	0.13%	0.013%
45	16.827	2347	2353	2355	rBV6	7639	10794	0.15%	0.015%

46	16.922	2362	2369	2378	rBV	3915171	5390866	75.21%	7.315%
47	17.021	2378	2386	2400	rVV	3952977	5479595	76.45%	7.435%
48	17.133	2401	2405	2411	rVB7	10852	17475	0.24%	0.024%
49	17.316	2429	2436	2440	rBV9	10756	22031	0.31%	0.030%
50	17.469	2456	2462	2465	rBV3	12543	21516	0.30%	0.029%

51	17.510	2465	2469	2474	rVB6	6700	11676	0.16%	0.016%
52	17.627	2484	2489	2494	rVV	32207	43320	0.60%	0.059%
53	17.686	2495	2499	2505	rVB5	9233	15690	0.22%	0.021%
54	17.851	2522	2527	2535	rBV	129597	196900	2.75%	0.267%
55	17.916	2536	2538	2546	rVB	12637	21614	0.30%	0.029%

56	18.151	2572	2578	2582	rVB7	13063	25996	0.36%	0.035%
57	18.563	2644	2648	2650	rVB5	6687	7664	0.11%	0.010%
58	18.621	2650	2658	2659	rBV6	4816	11058	0.15%	0.015%
59	18.810	2687	2690	2694	rVB2	20015	22347	0.31%	0.030%
60	18.892	2699	2704	2711	rVB	51503	80096	1.12%	0.109%

61	18.957	2711	2715	2720	rBV2	63680	92763	1.29%	0.126%
62	19.051	2728	2731	2734	rBV5	9066	11239	0.16%	0.015%
63	19.145	2743	2747	2752	rBV2	47780	66478	0.93%	0.090%
64	19.327	2769	2778	2790	rBV	5016506	6662084	92.95%	9.039%
65	19.415	2790	2793	2798	rVB6	14766	22375	0.31%	0.030%

66	19.574	2818	2820	2825	rVB4	8840	9599	0.13%	0.013%
67	19.915	2875	2878	2881	rBV3	12463	12165	0.17%	0.017%
68	20.351	2949	2952	2957	rBV4	32047	37567	0.52%	0.051%
69	20.415	2960	2963	2966	rVB	28902	30292	0.42%	0.041%
70	20.880	3037	3042	3056	rBV	208268	518097	7.23%	0.703%

71	21.074	3073	3075	3079	rVB2	27716	26311	0.37%	0.036%
72	21.133	3079	3085	3098	rBV	5111320	6404074	89.35%	8.689%
73	21.321	3113	3117	3122	rBV	63769	74236	1.04%	0.101%
74	21.751	3186	3190	3196	rBV	83110	119071	1.66%	0.162%
75	22.204	3263	3267	3273	rVB	140724	189083	2.64%	0.257%

76	22.709	3348	3353	3358	rBV	230338	326133	4.55%	0.443%
----	--------	------	------	------	-----	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
 Data File : BN017257.D
 Acq On : 03 Nov 2021 01:49
 Operator : CG/JU
 Sample : M4400-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG335

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
 Title : SVOA CALIBRATION

77	23.192	3427	3435	3443	rBV2	4019837	7167484	100.00%	9.725%
78	23.268	3443	3448	3452	rVV	317094	548608	7.65%	0.744%
79	23.333	3452	3459	3476	rVB2	3732019	6804076	94.93%	9.232%
80	23.909	3551	3557	3567	rBV	298904	565643	7.89%	0.767%
81	24.651	3677	3683	3698	rVB2	250982	594471	8.29%	0.807%
82	25.521	3824	3831	3843	rVB2	173242	461780	6.44%	0.627%
83	26.545	3998	4005	4017	rVB3	129193	386279	5.39%	0.524%


Sum of corrected areas: 73701076

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017257.D
Acq On : 03 Nov 2021 01:49
Operator : CG/JU
Sample : M4400-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

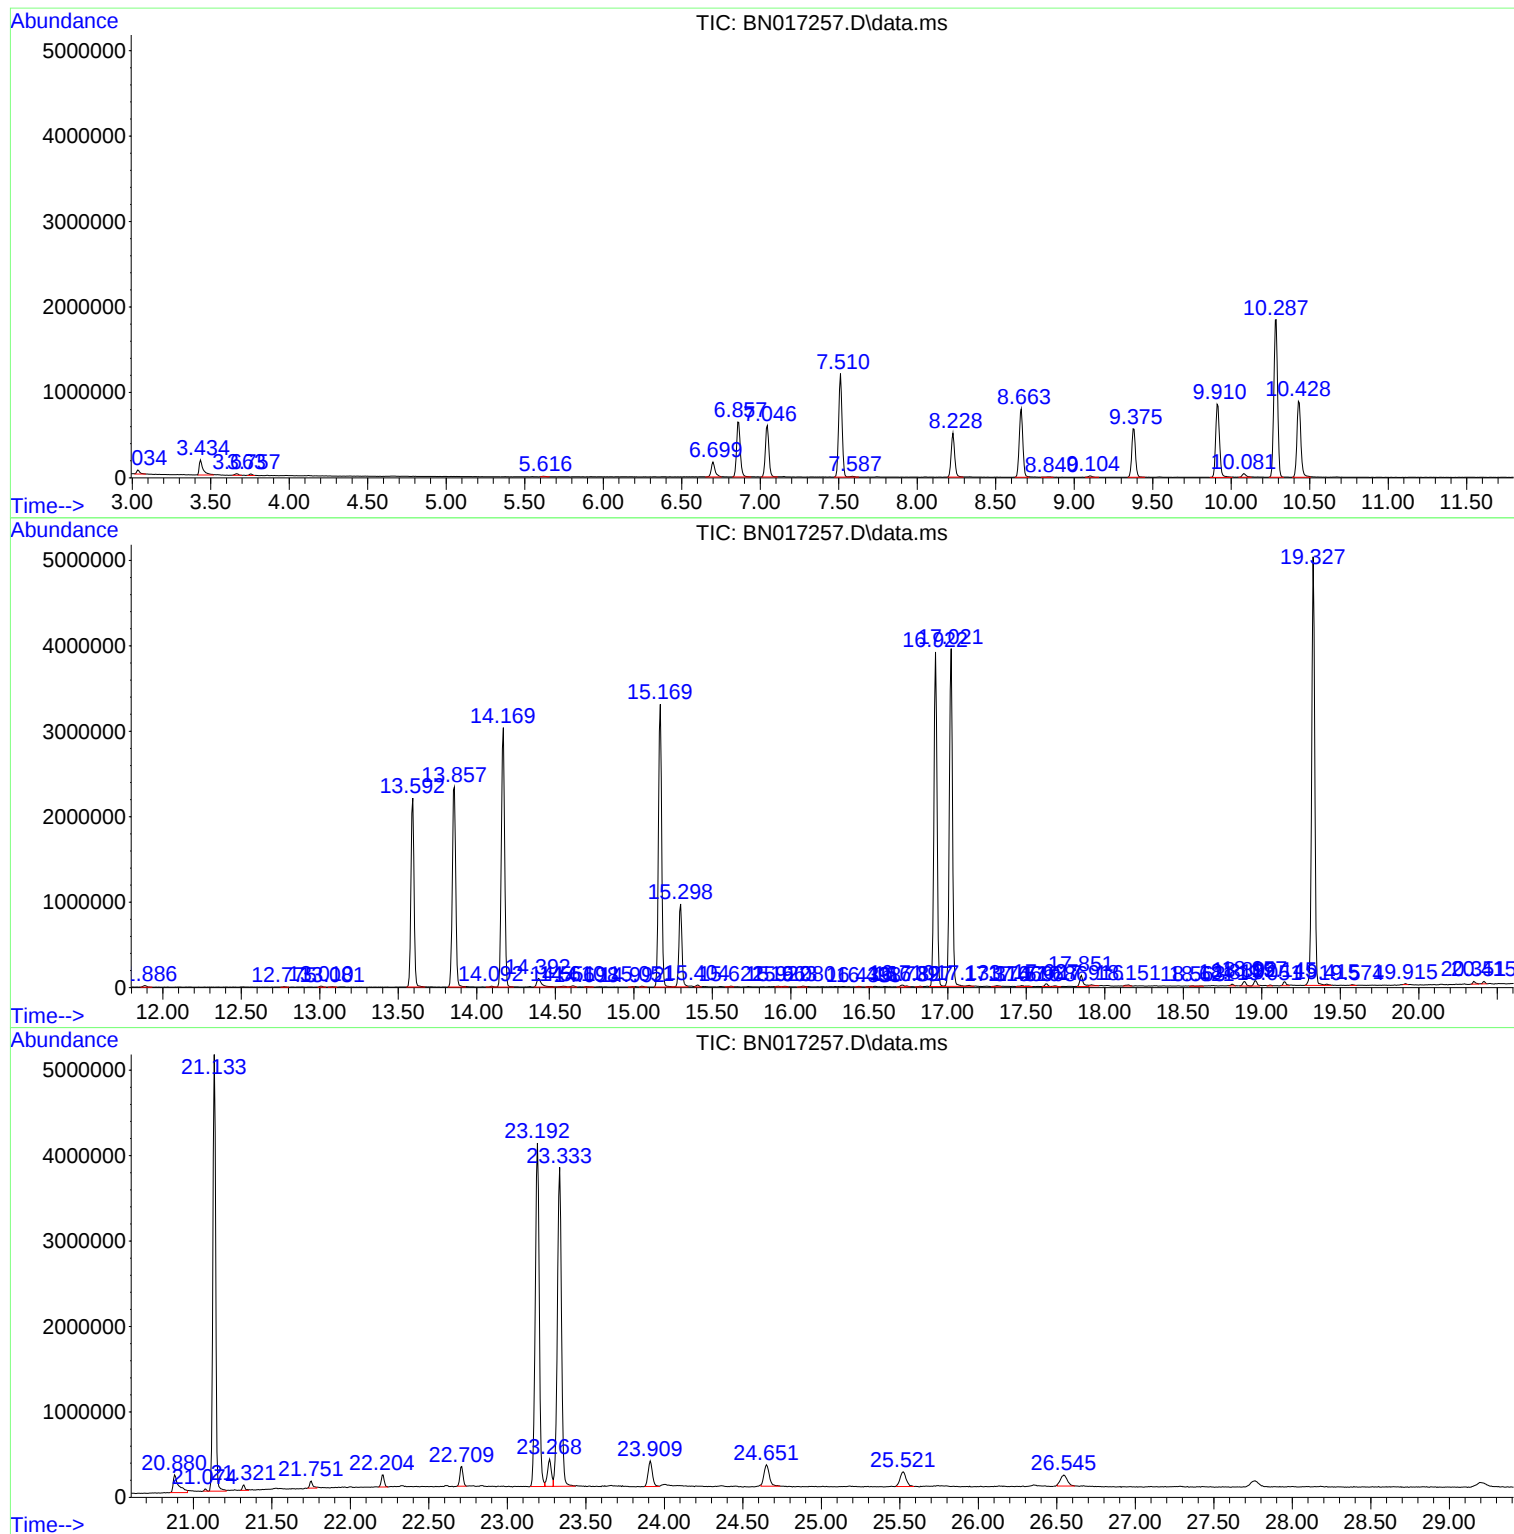

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017257.D
Acq On : 03 Nov 2021 01:49
Operator : CG/JU
Sample : M4400-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110221\
Data File : BN017257.D
Acq On : 03 Nov 2021 01:49
Operator : CG/JU
Sample : M4400-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG335

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN110221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc