
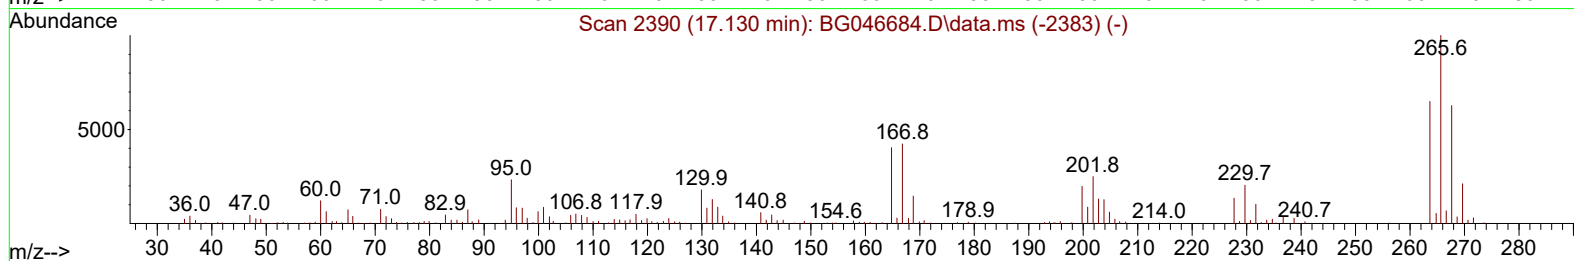
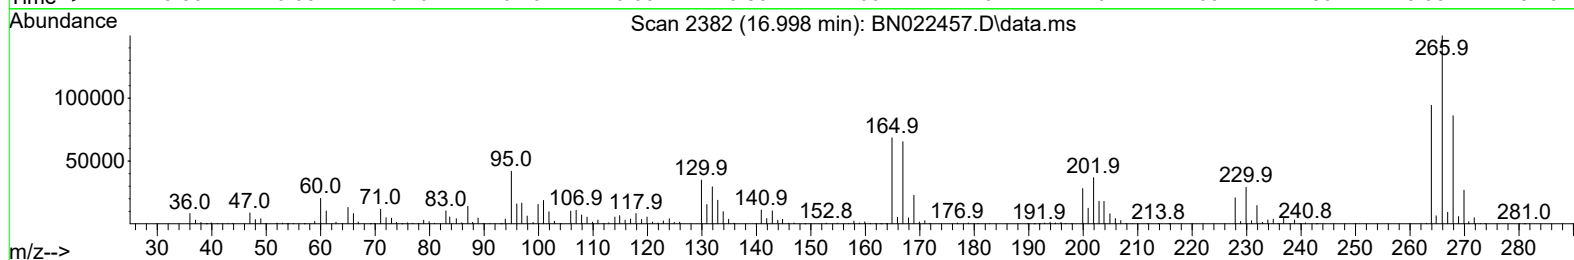


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110222\
Data File : BN022457.D
Acq On : 02 Nov 2022 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 08:42:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 03 08:42:49 2022
Response via : Initial Calibration

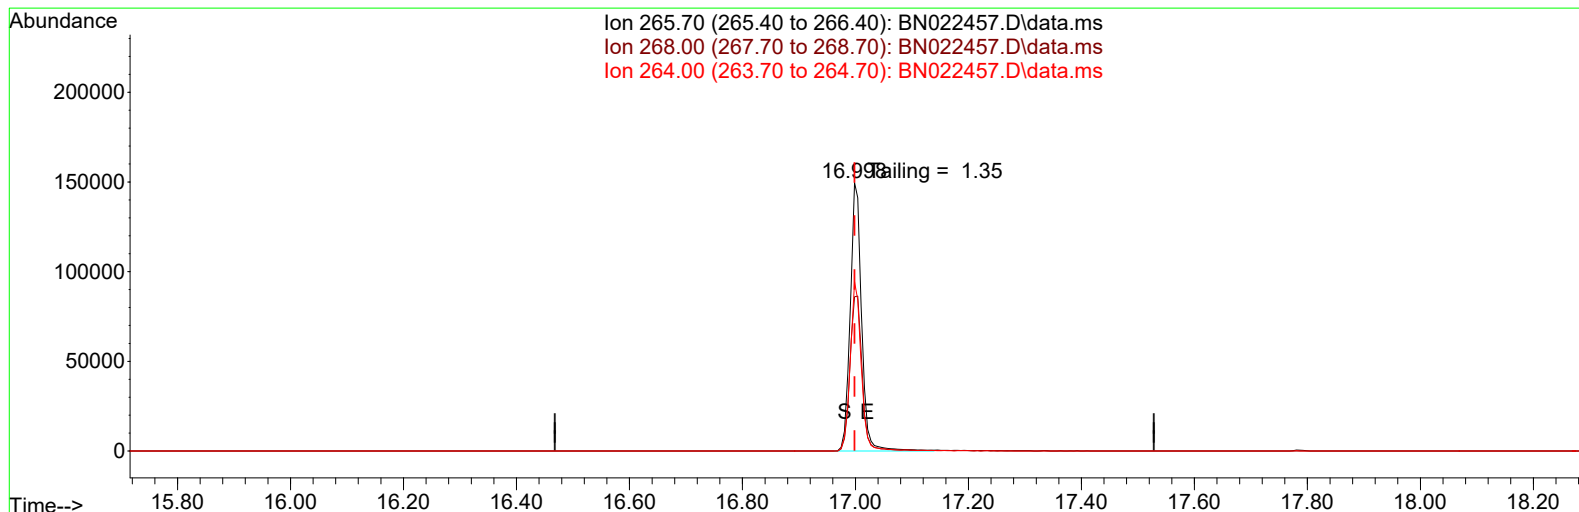

TIC: BN022457.D\data.ms

(70) Pentachlorophenol (C)




16.998min (0.000) 22466.38 ng

response 210691

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.48
264.00	61.60	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110222\
Data File : BN022457.D
Acq On : 02 Nov 2022 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 08:42:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 03 08:42:49 2022
Response via : Initial Calibration

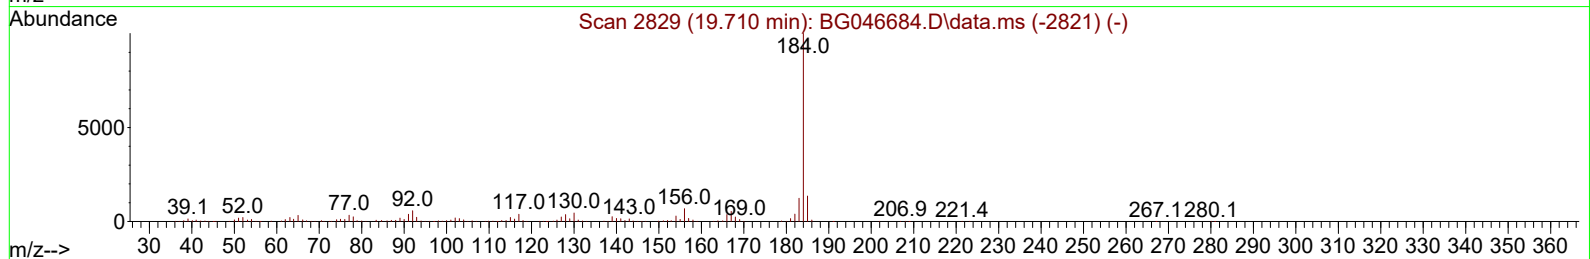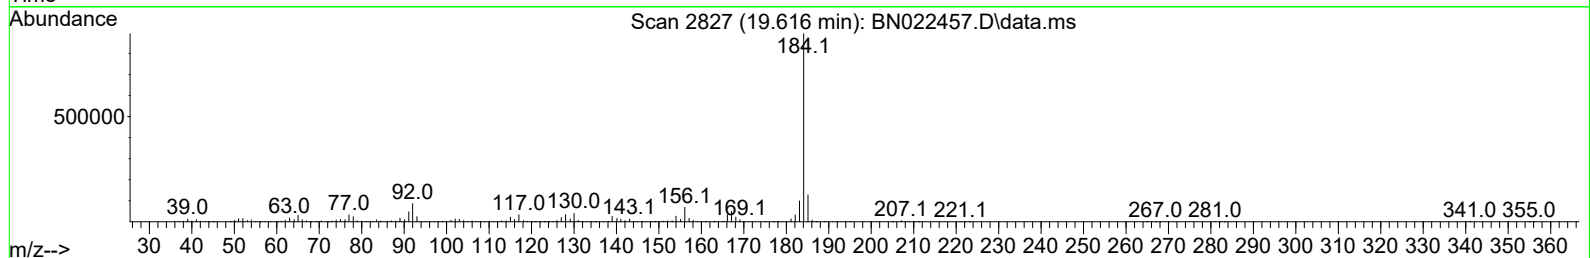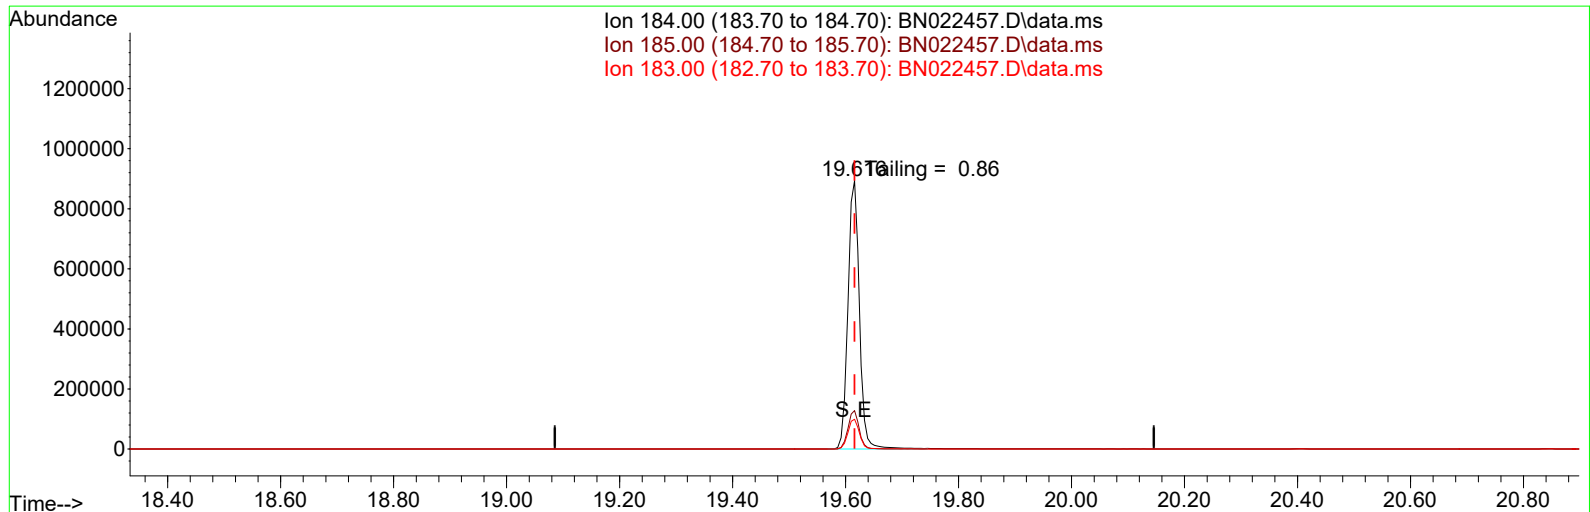

TIC: BN022457.D\data.ms

(77) Benzidine**19.616min (0.000) 42138.77 ng****response 1261274**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	11.10
0.00	0.00	0.00