


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110222\
 Data File : BN022457.D
 Acq On : 02 Nov 2022 09:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 02 05:31:40 2022

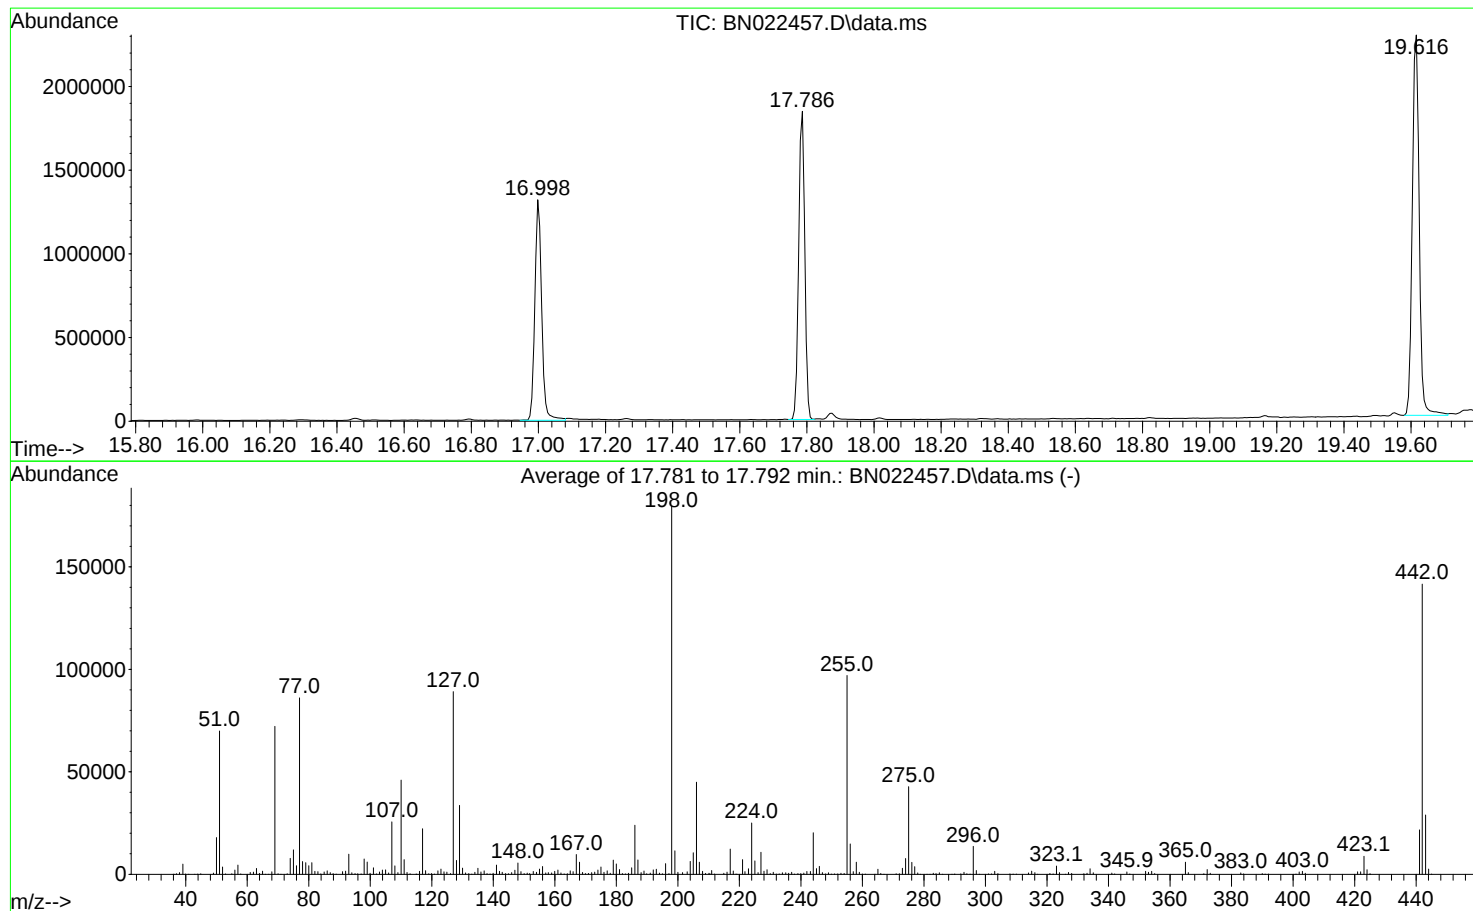




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	69955	PASS
68	69	0.00	2	1.7	1249	PASS
69	198	0.00	100	40.2	72204	PASS
70	69	0.00	2	0.4	318	PASS
127	198	10	80	49.7	89165	PASS
197	198	0.00	2	0.2	339	PASS
198	198	100	100	100.0	179499	PASS
199	198	5	9	6.4	11421	PASS
275	198	10	60	23.8	42781	PASS
365	198	1	100	3.3	5902	PASS
441	198	0.01	100	12.1	21691	PASS
442	442	50	100	100.0	141584	PASS
443	442	15	24	20.5	28968	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110222\
Data File : BN022457.D
Acq On : 02 Nov 2022 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 03 08:42:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 03 08:42:49 2022
Response via : Initial Calibration

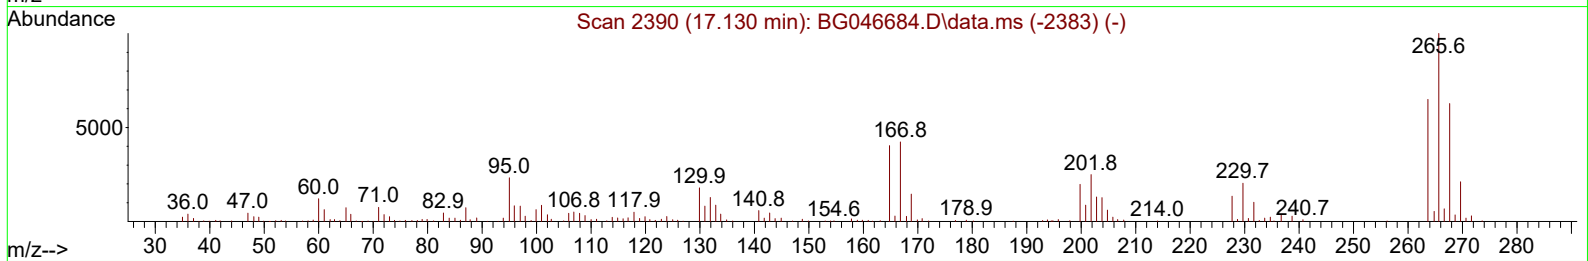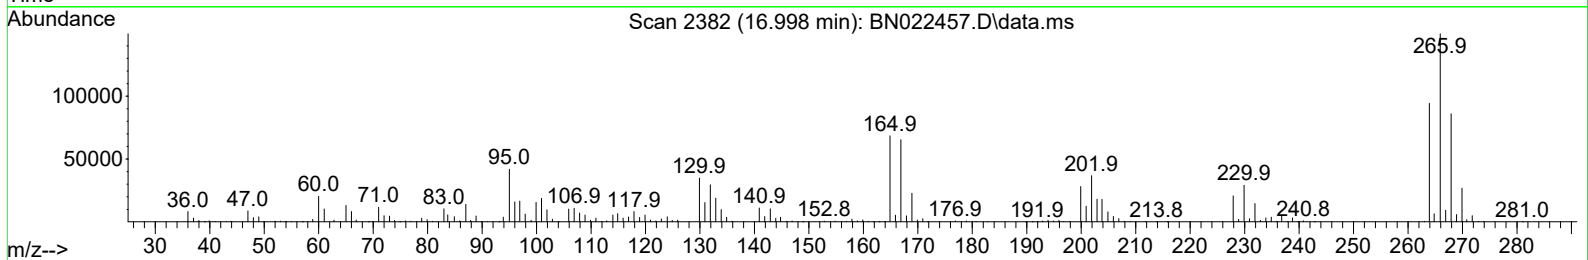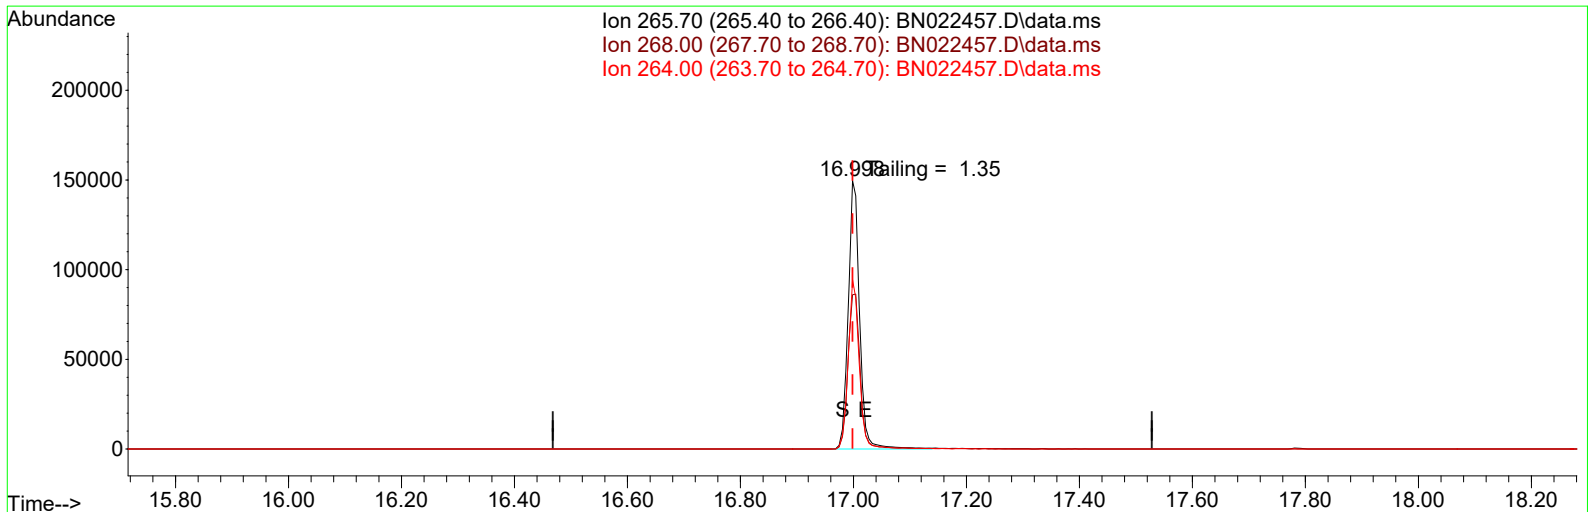

TIC: BN022457.D\data.ms

(70) Pentachlorophenol (C)

16.998min (0.000) 22466.38 ng




response 210691

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.48
264.00	61.60	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110222\
Data File : BN022457.D
Acq On : 02 Nov 2022 09:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 03 08:42:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 03 08:42:49 2022
Response via : Initial Calibration

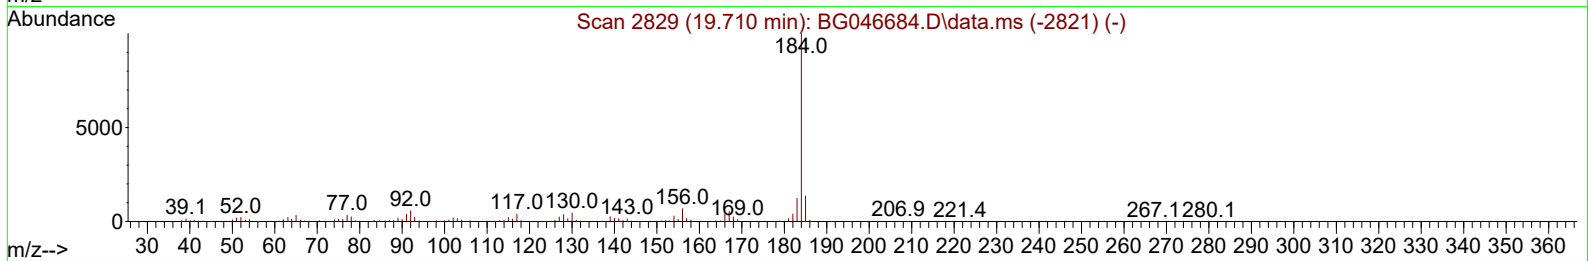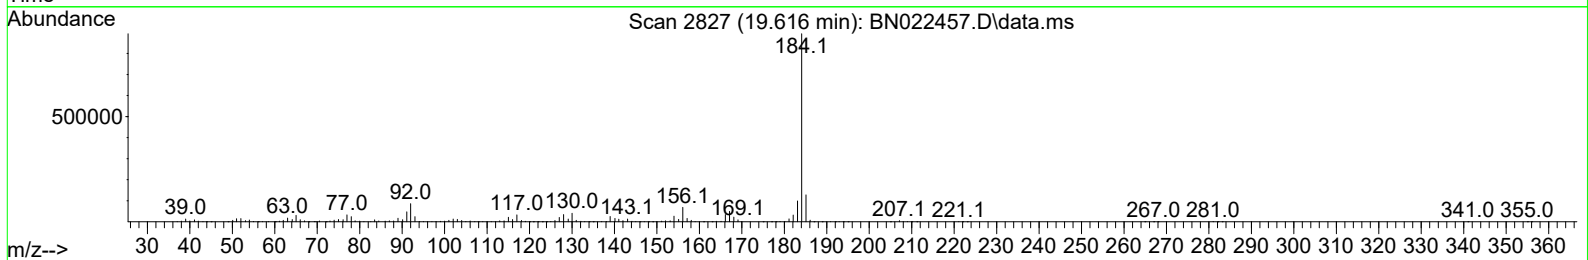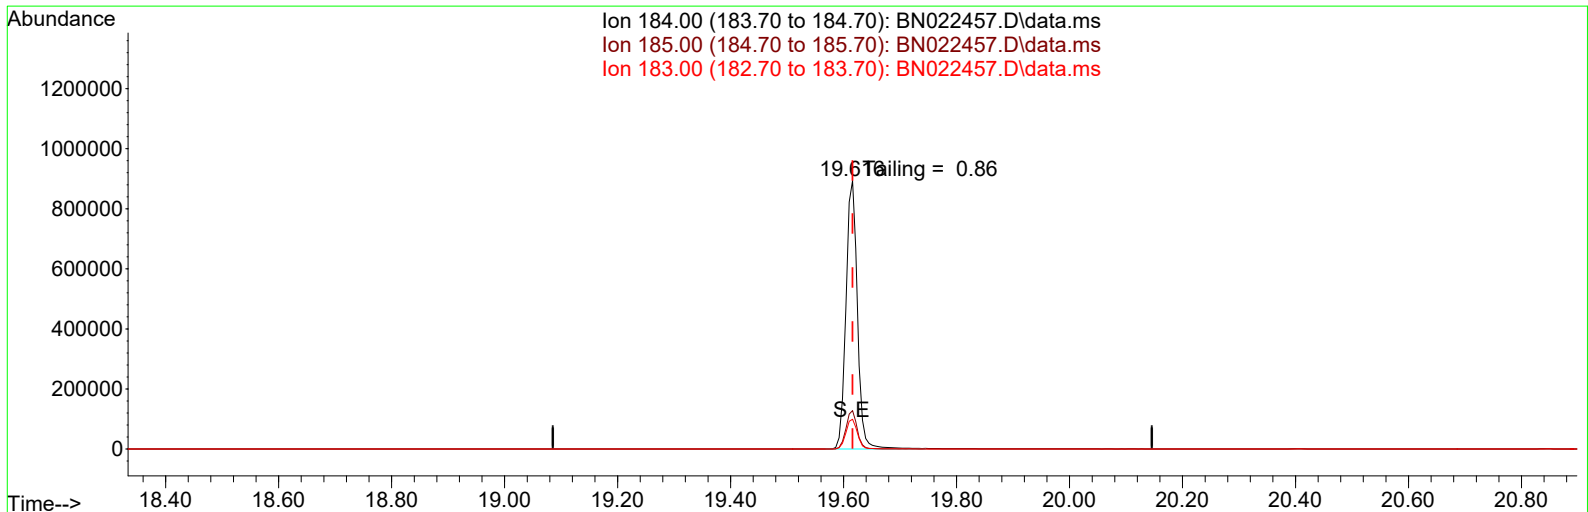

TIC: BN022457.D\data.ms

(77) Benzidine

19.616min (0.000) 42138.77 ng

response 1261274

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.31
183.00	13.20	11.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2022	BNA_N	<u>BN022457.D</u>
Compound Name	Response	Retention Time
DDT	163865	20.845
DDD	290152	20.404
DDE	442	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
290594	454459	63.94

Instrument :
BNA_N
ClientSampleId :
DFTPP