

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017283.D
 Acq On : 03 Nov 2021 20:09
 Operator : CG/JU
 Sample : PB140308BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK308

Quant Time: Nov 08 01:06:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4645	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	19000	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	12058	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	25468	0.400	ng/ul	0.00
17) Chrysene-d12	21.140	240	20930	0.400	ng/ul	0.00
23) Perylene-d12	23.332	264	25762	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	28627	5.543	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.894	152	9662	0.348	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	23852	0.435	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.169	166	3133	0.064	ng/ul#	14
20) Pyrene	19.328	202	3105	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.195	252	7364	0.085	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017283.D
Acq On : 03 Nov 2021 20:09
Operator : CG/JU
Sample : PB140308BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK308

Quant Time: Nov 08 01:06:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




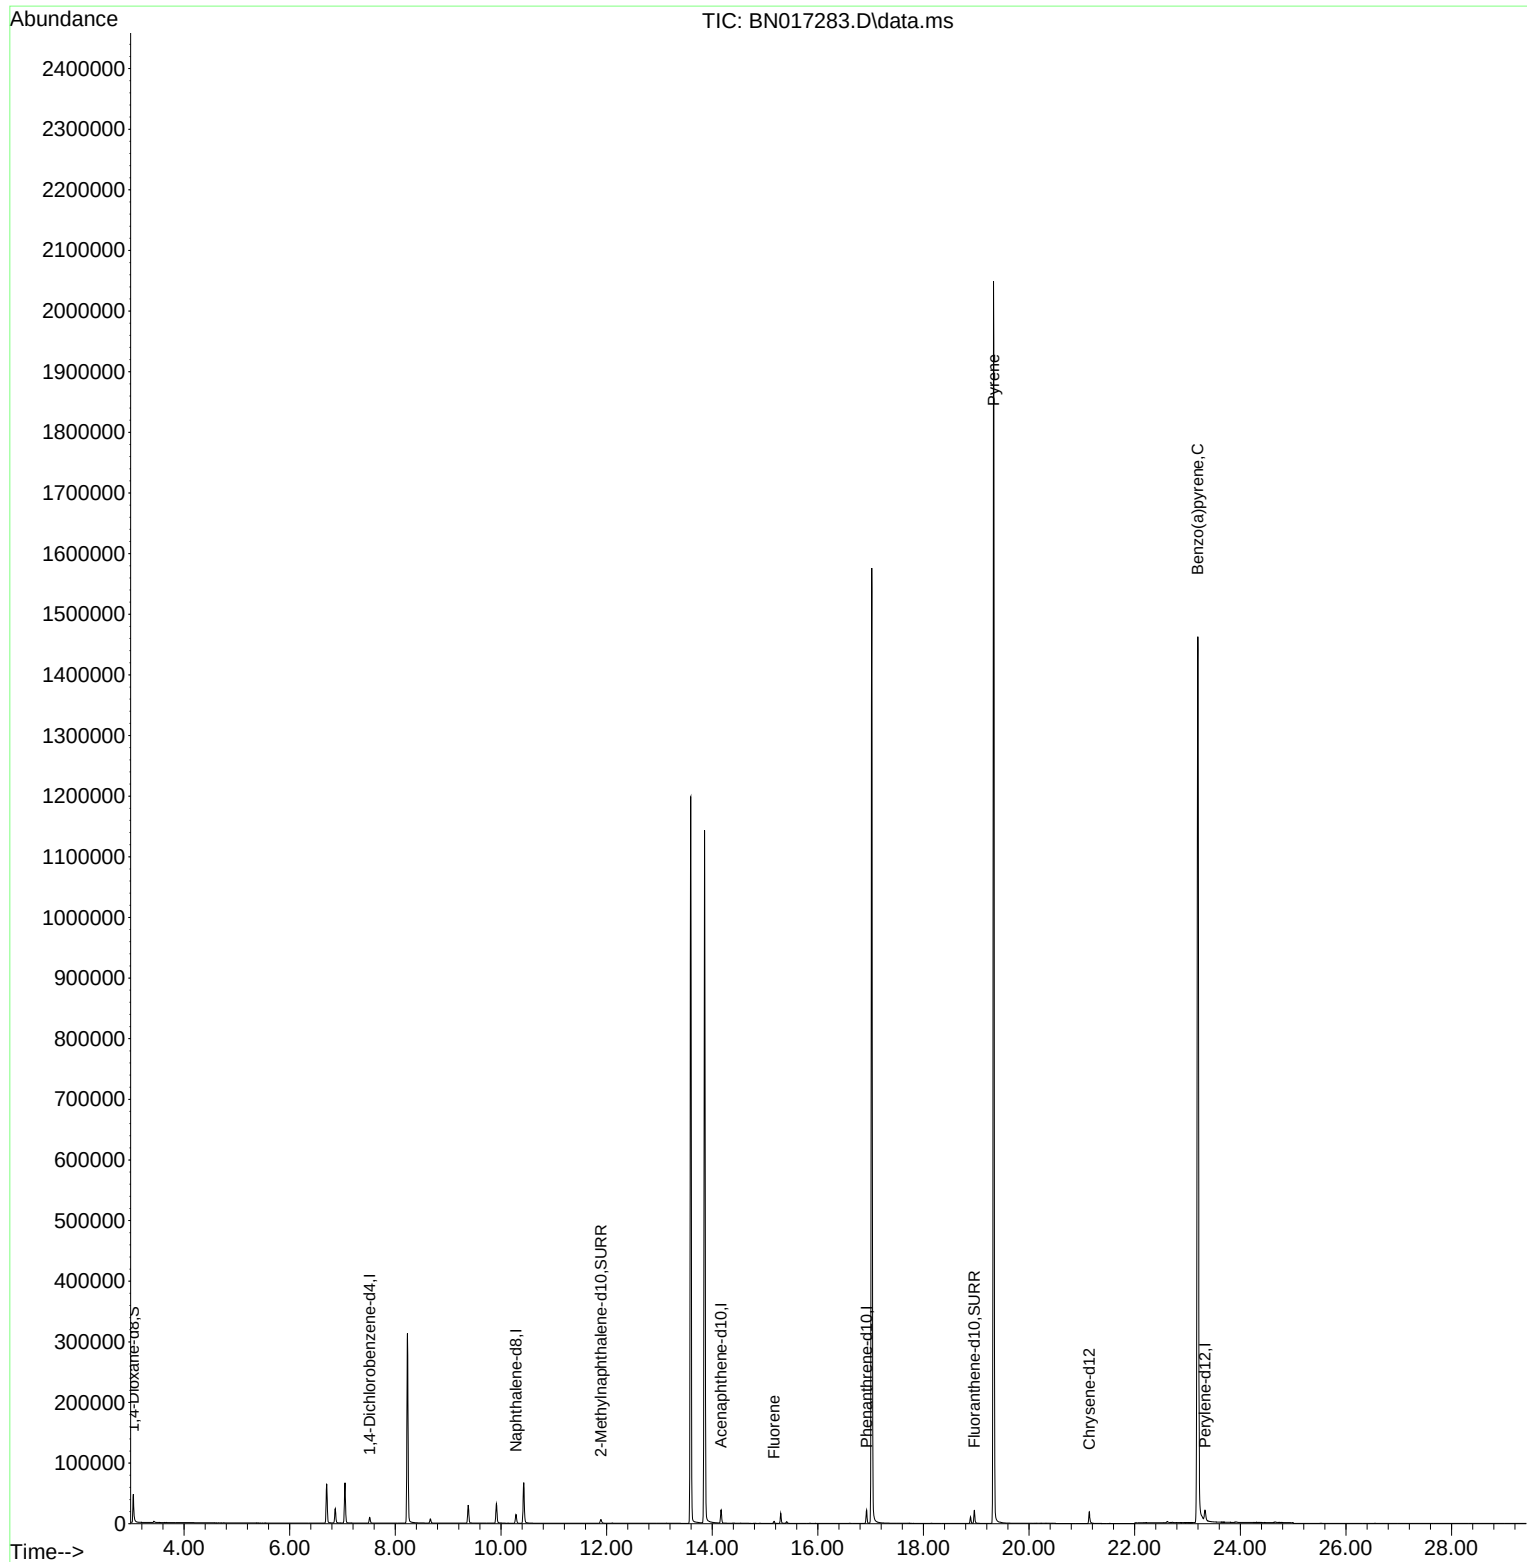


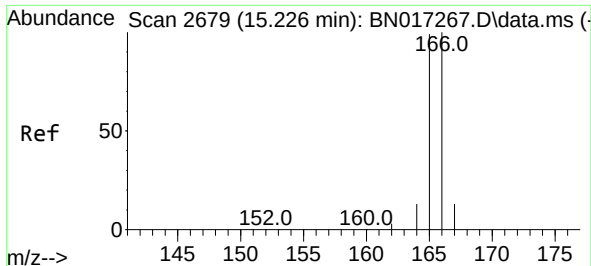

#12
Fluorene
Concen: 0.064 ng/ul
RT: 15.169 min Scan# 2667
Delta R.T. -0.057 min
Lab File: BN017283.D
Acq: 03 Nov 2021 20:09




Instrument :
BNA_N
ClientSampleId :
SBLK308


Tgt Ion:166 Resp: 3133
Ion Ratio Lower Upper
166 100
165 7.3 77.7 116.5#
167 32.9 11.1 16.7#

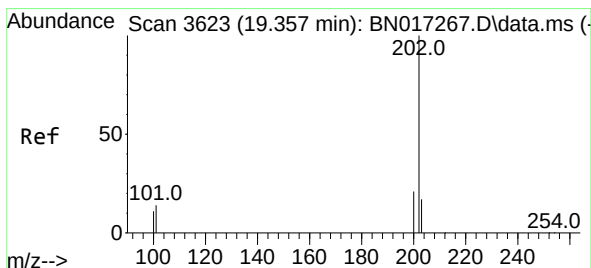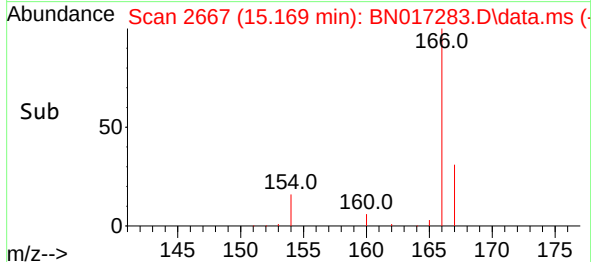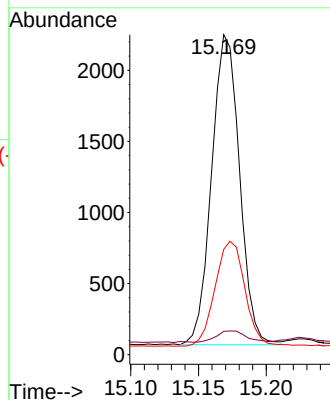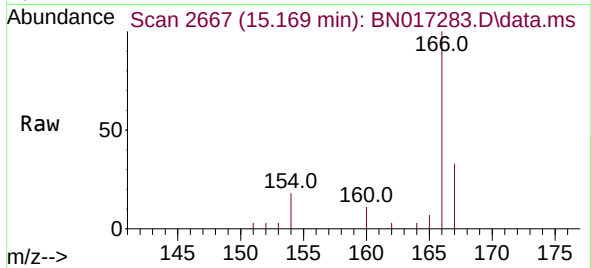

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.328 min Scan# 3617
Delta R.T. -0.029 min
Lab File: BN017283.D
Acq: 03 Nov 2021 20:09

Tgt Ion:202 Resp: 3105
Ion Ratio Lower Upper
202 100
101 151.4 10.3 15.5#
100 1137.7 8.2 12.2#

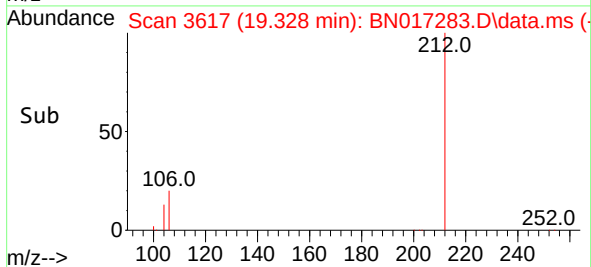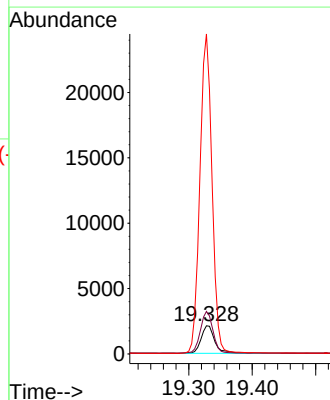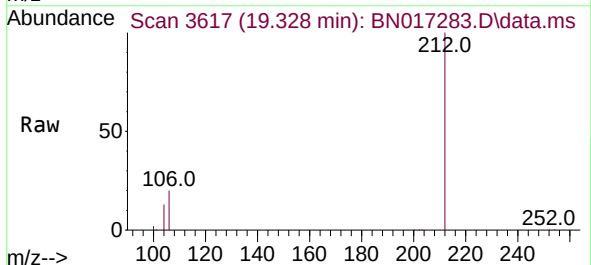

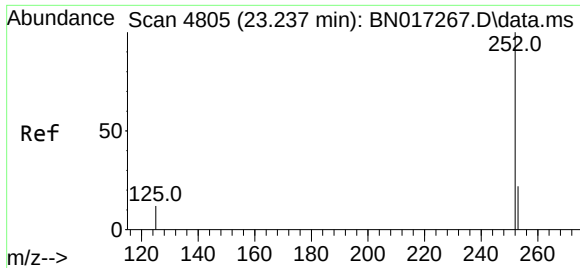

#26

Benzo(a)pyrene

Concen: 0.085 ng/ul

RT: 23.195 min Scan# 41

Delta R.T. -0.042 min

Lab File: BN017283.D


Acq: 03 Nov 2021 20:09

Instrument :

BNA_N

ClientSampleId :

SBLK308

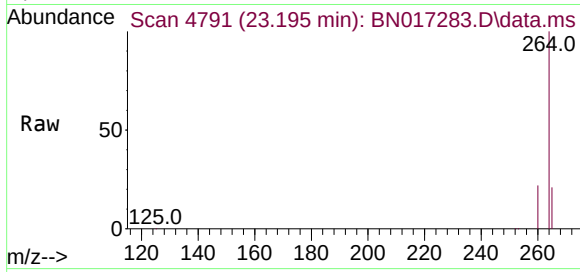

Tgt Ion:252 Resp: 7364

Ion Ratio Lower Upper

252 100

253 38.9 19.3 28.9#

125 24.8 10.8 16.2#

