

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017284.D
 Acq On : 03 Nov 2021 20:45
 Operator : CG/JU
 Sample : PB140309BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK309

Quant Time: Nov 08 01:06:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	19499	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	12772	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	27574	0.400	ng/ul	0.00
17) Chrysene-d12	21.140	240	22265	0.400	ng/ul	0.00
23) Perylene-d12	23.332	264	27354	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	29158	5.515	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.894	152	9937	0.349	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	25670	0.440	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.169	166	3276	0.063	ng/ul#	14
20) Pyrene	19.332	202	3260	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.195	252	7790	0.085	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017284.D
Acq On : 03 Nov 2021 20:45
Operator : CG/JU
Sample : PB140309BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK309

Quant Time: Nov 08 01:06:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




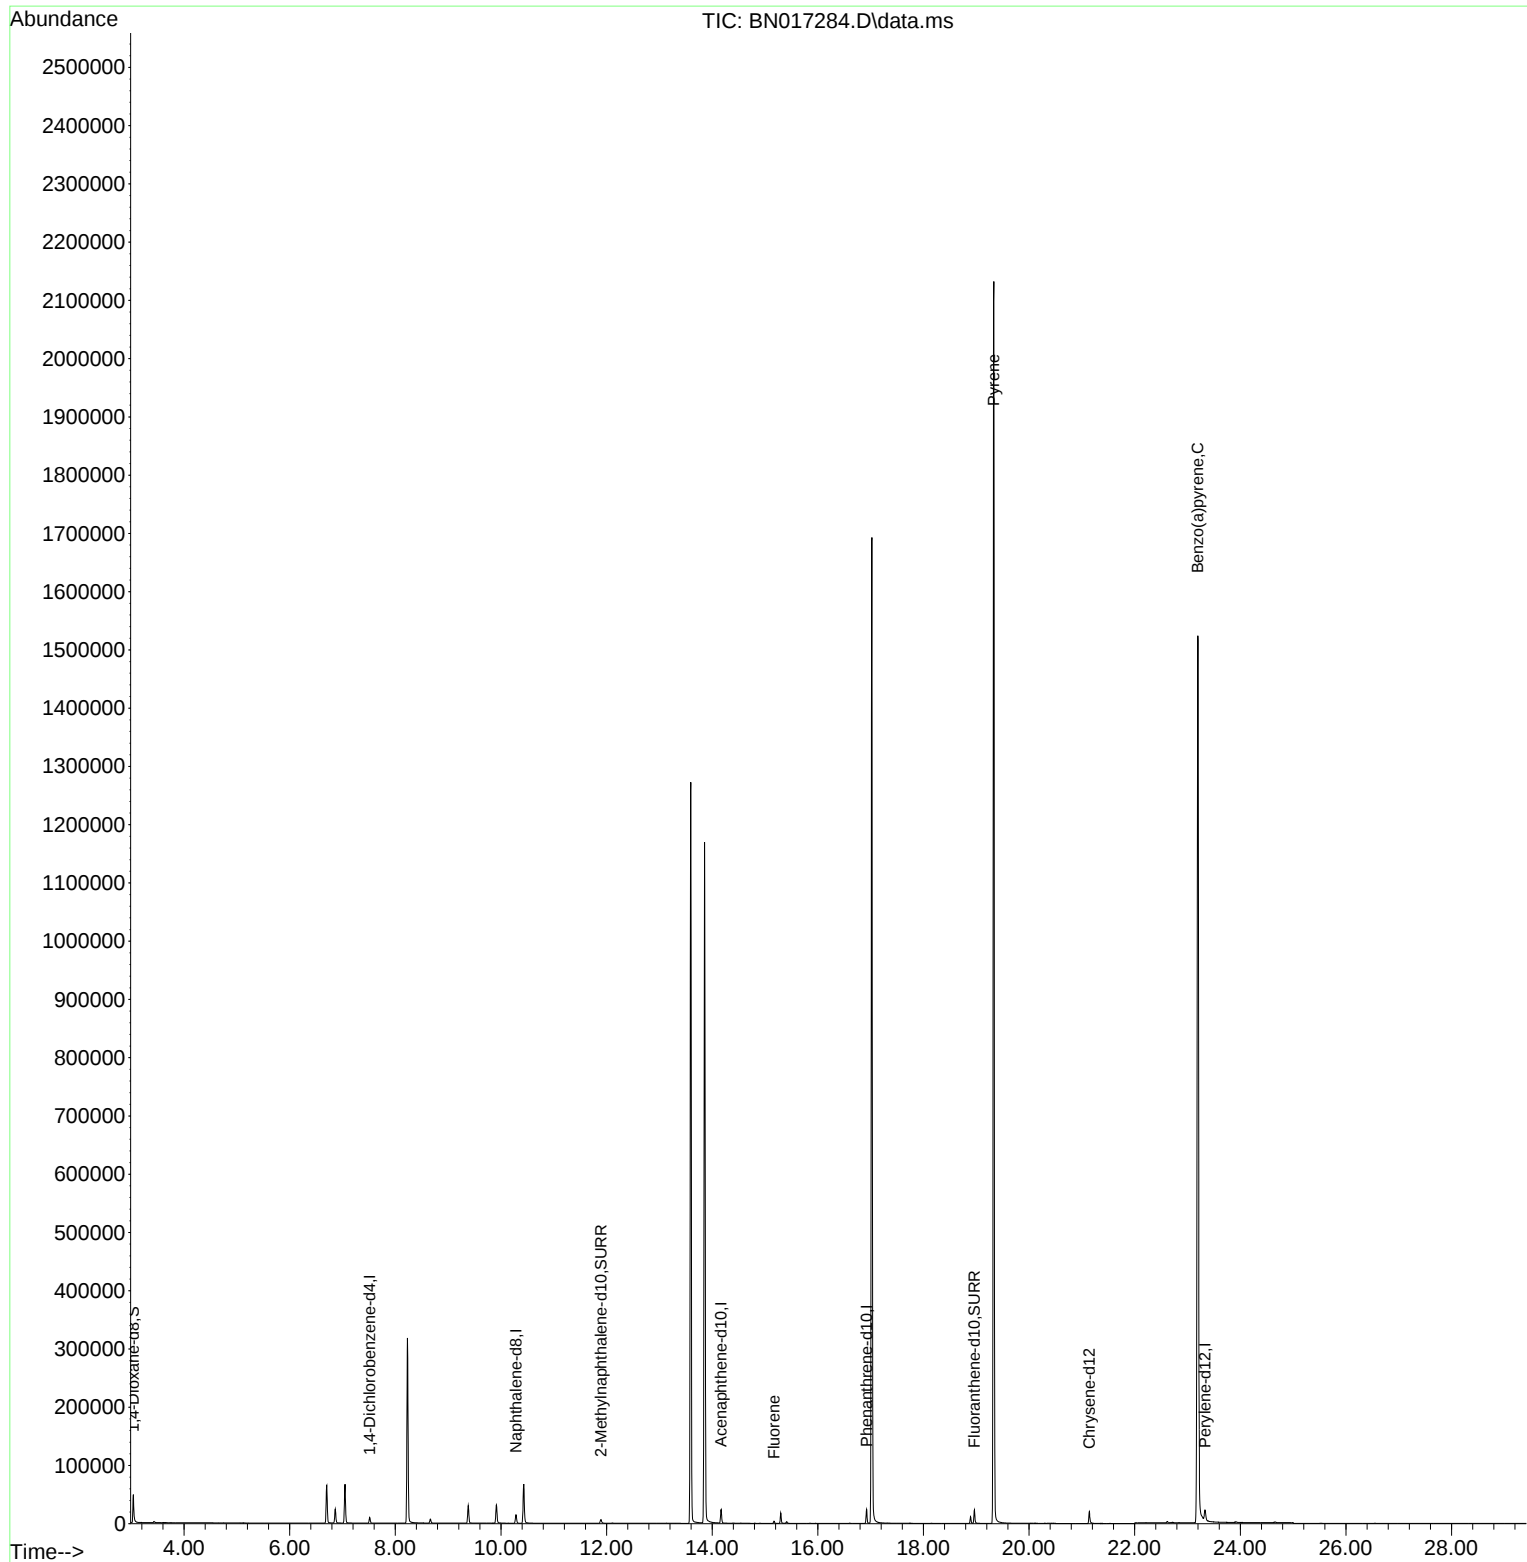


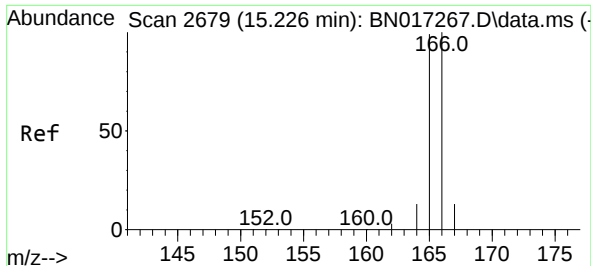

#12
Fluorene
Concen: 0.063 ng/ul
RT: 15.169 min Scan# 2667
Delta R.T. -0.057 min
Lab File: BN017284.D
Acq: 03 Nov 2021 20:45




Instrument :
BNA_N
ClientSampleId :
SBLK309


Tgt Ion:166 Resp: 3276
Ion Ratio Lower Upper
166 100
165 6.3 77.7 116.5#
167 32.4 11.1 16.7#

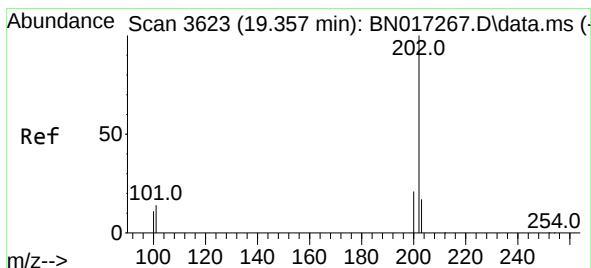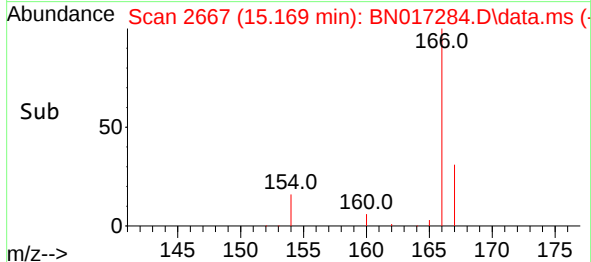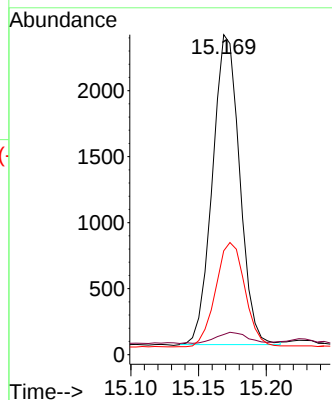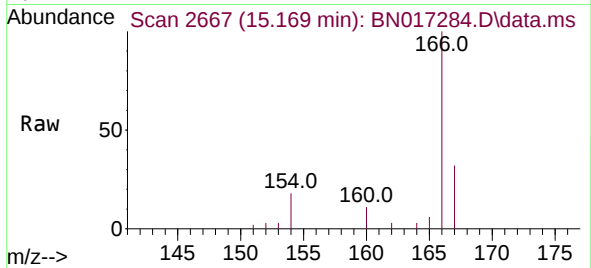

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.332 min Scan# 3618
Delta R.T. -0.024 min
Lab File: BN017284.D
Acq: 03 Nov 2021 20:45

Tgt Ion:202 Resp: 3260
Ion Ratio Lower Upper
202 100
101 141.9 10.3 15.5#
100 1004.9 8.2 12.2#

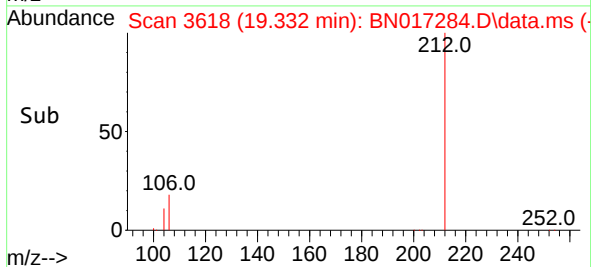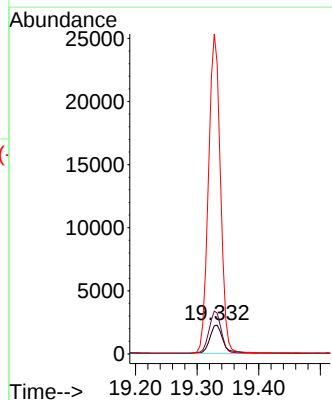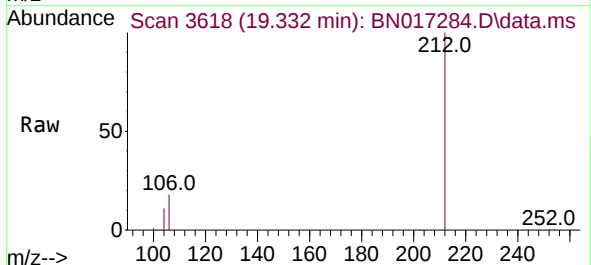

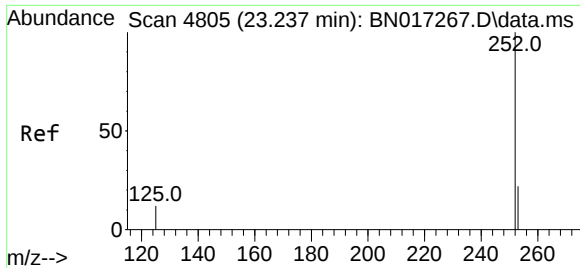

#26

Benzo(a)pyrene

Concen: 0.085 ng/ul

RT: 23.195 min Scan# 41

Delta R.T. -0.042 min

Lab File: BN017284.D


Acq: 03 Nov 2021 20:45

Instrument :

BNA_N

ClientSampleId :

SBLK309

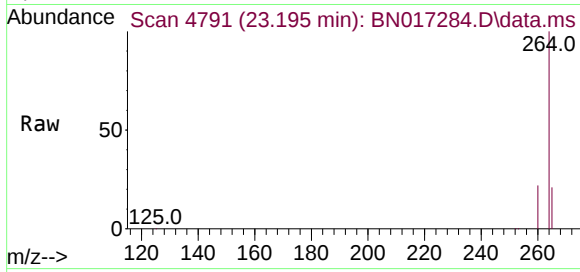

Tgt Ion:252 Resp: 7790

Ion Ratio Lower Upper

252 100

253 38.7 19.3 28.9#

125 24.7 10.8 16.2#

