

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017289.D
 Acq On : 03 Nov 2021 23:46
 Operator : CG/JU
 Sample : M4364-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG328

Quant Time: Nov 08 01:07:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.515	152	4857	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	20104	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	12888	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.923	188	27057	0.400	ng/ul	0.00
17) Chrysene-d12	21.136	240	23462	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	26808	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	26681	4.941	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	12594	0.429	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	34117	0.555	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.329	202	4334	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.193	252	9488	0.106	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017289.D
Acq On : 03 Nov 2021 23:46
Operator : CG/JU
Sample : M4364-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG328

Quant Time: Nov 08 01:07:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




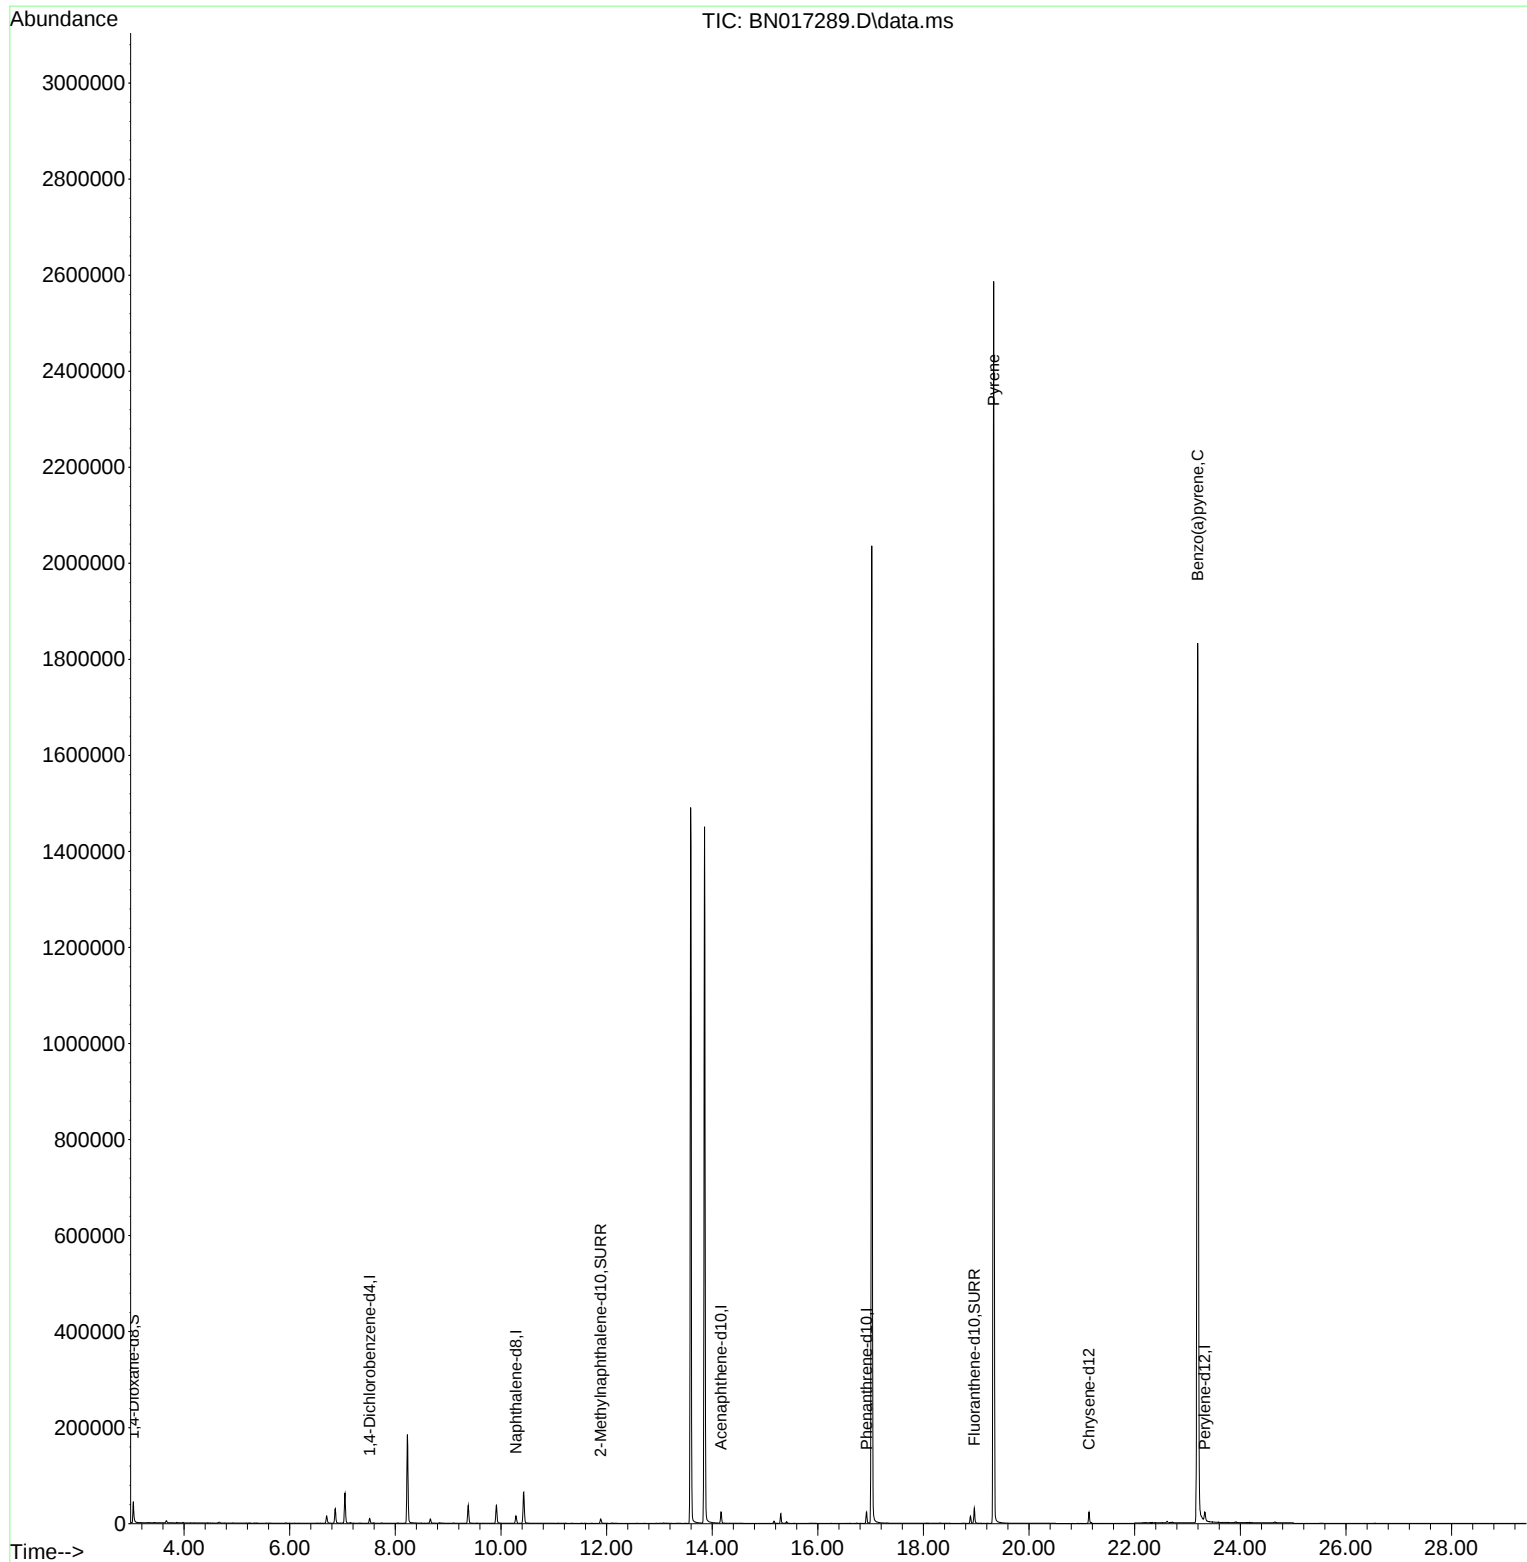


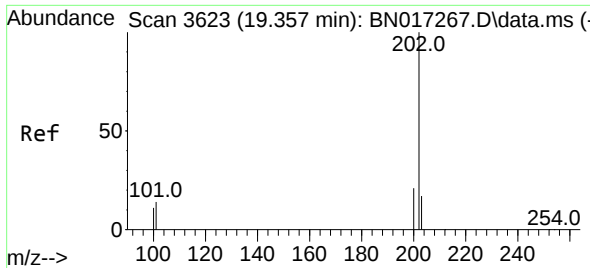

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.329 min Scan# 30
Delta R.T. -0.028 min
Lab File: BN017289.D
Acq: 03 Nov 2021 23:46

Instrument :
BNA_N
ClientSampleId :
BG328

Tgt Ion:202 Resp: 4334
Ion Ratio Lower Upper
202 100
101 150.8 10.3 15.5#
100 1114.1 8.2 12.2#

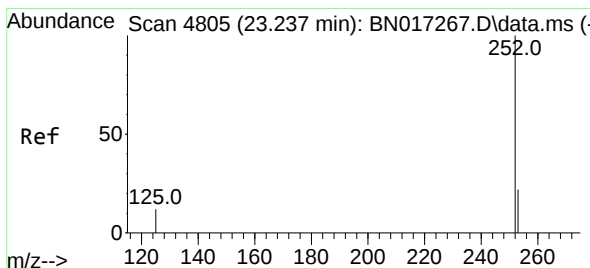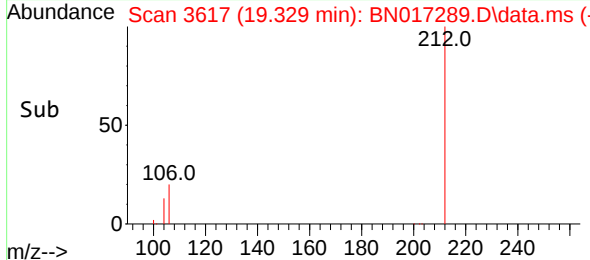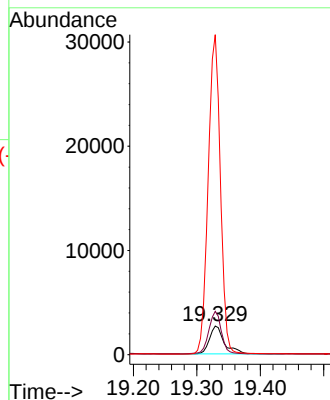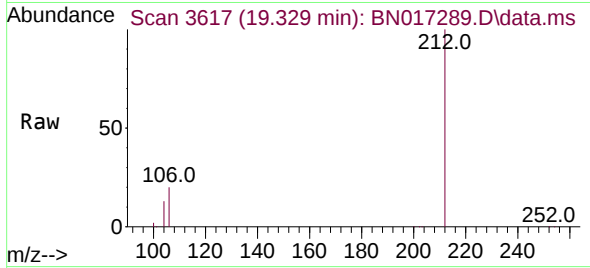

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.193 min Scan# 4790
Delta R.T. -0.044 min
Lab File: BN017289.D
Acq: 03 Nov 2021 23:46

Tgt Ion:252 Resp: 9488
Ion Ratio Lower Upper
252 100
253 37.1 19.3 28.9#
125 24.3 10.8 16.2#

