

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017294.D
 Acq On : 04 Nov 2021 02:46
 Operator : CG/JU
 Sample : M4374-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG328

Quant Time: Nov 08 01:07:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4062	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	16651	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	10557	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	22472	0.400	ng/ul	0.00
17) Chrysene-d12	21.135	240	20637	0.400	ng/ul	0.00
23) Perylene-d12	23.326	264	24135	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	19454	4.308	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	10240	0.421	ng/ul	0.00
18) Fluoranthene-d10	18.961	212	28533	0.527	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.328	202	3735	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.192	252	8462	0.105	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017294.D
Acq On : 04 Nov 2021 02:46
Operator : CG/JU
Sample : M4374-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG328

Quant Time: Nov 08 01:07:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




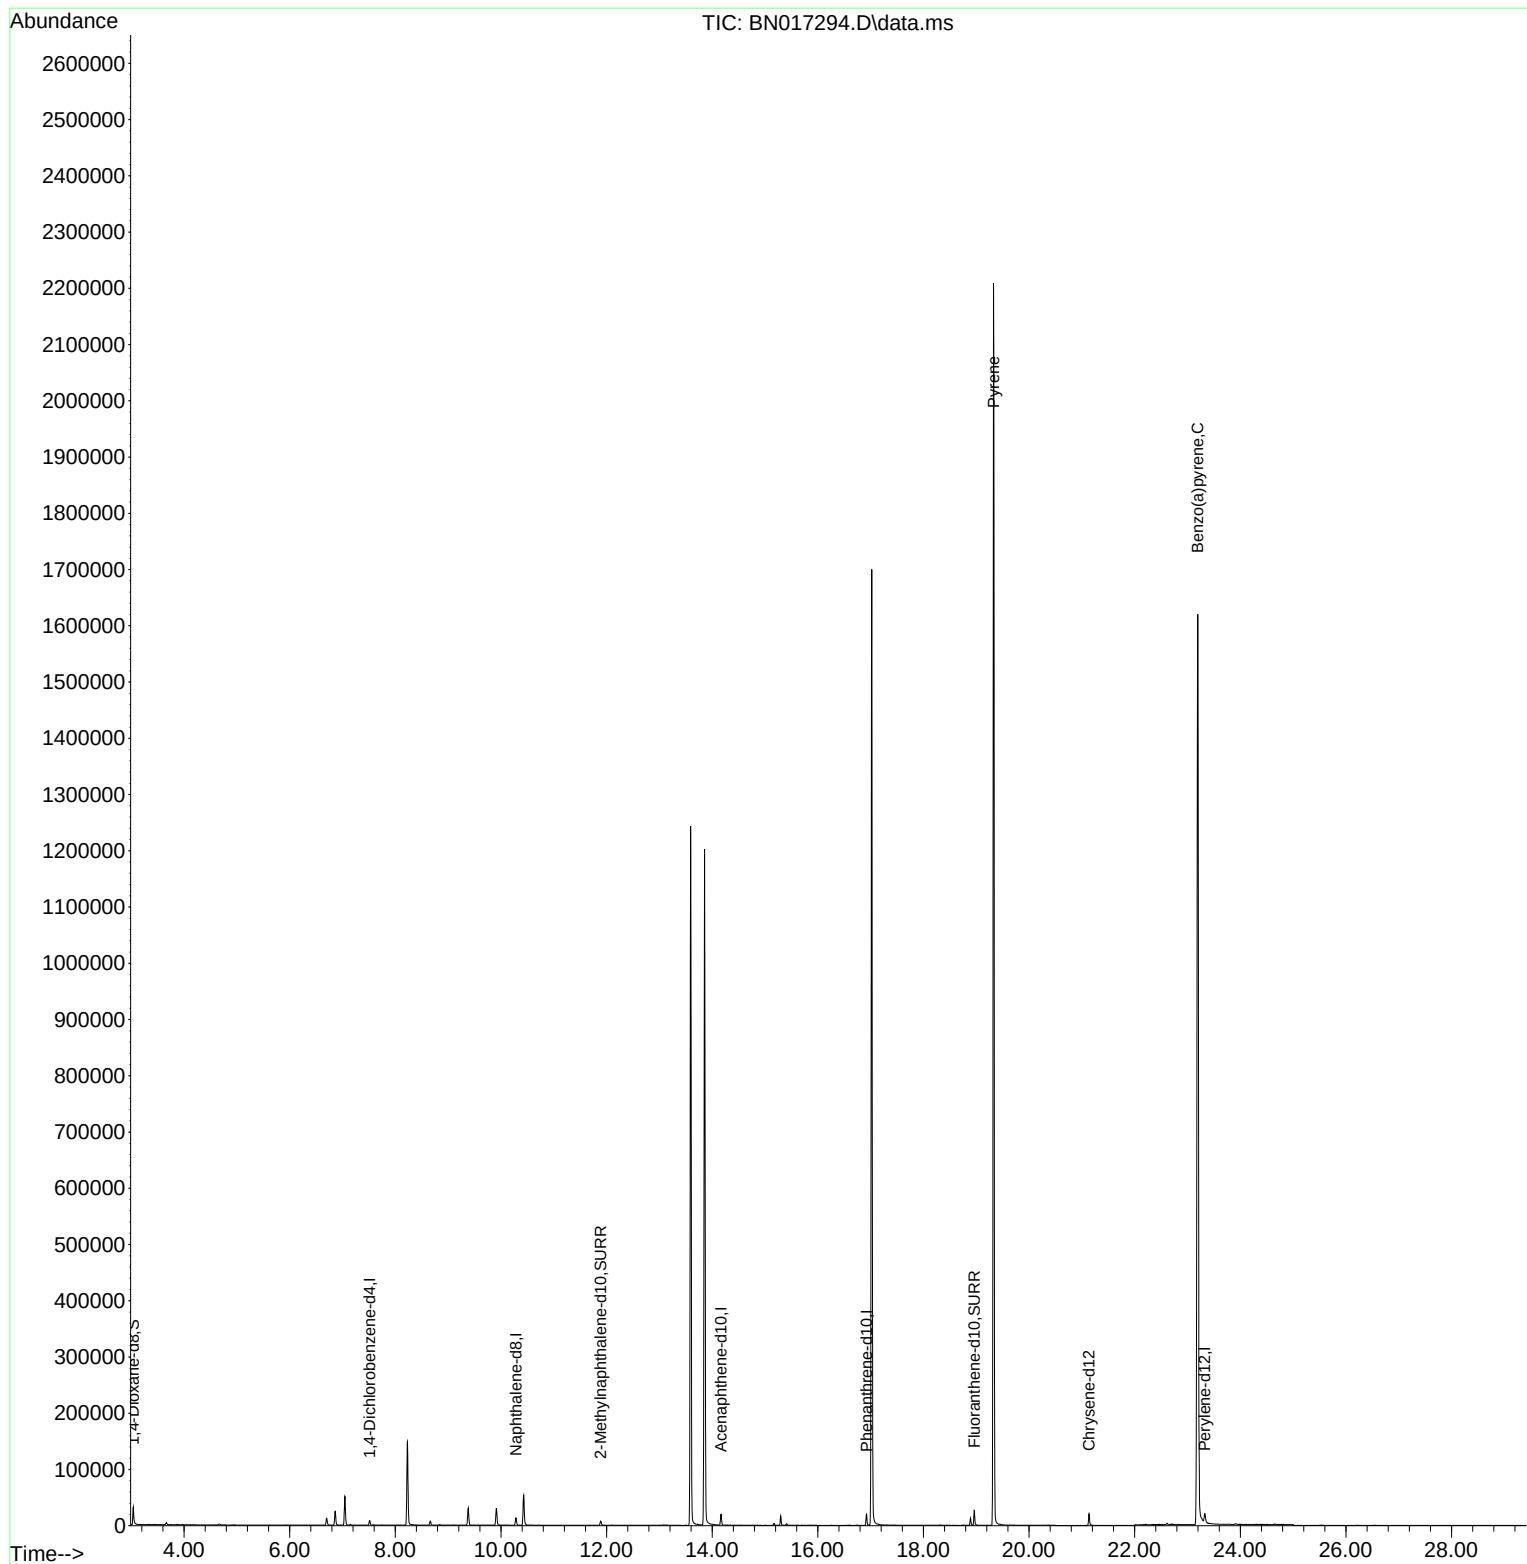


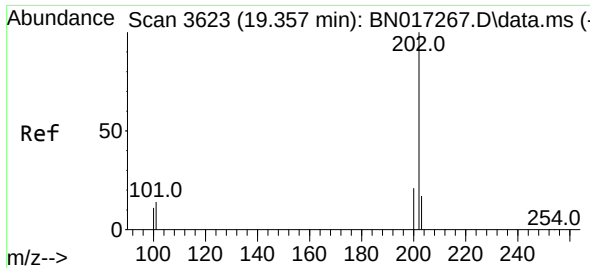

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.328 min Scan# 3617
Delta R.T. -0.029 min
Lab File: BN017294.D
Acq: 04 Nov 2021 02:46

Instrument :
BNA_N
ClientSampleId :
BG328

Tgt Ion:202 Resp: 3735
Ion Ratio Lower Upper
202 100
101 149.0 10.3 15.5#
100 1105.3 8.2 12.2#

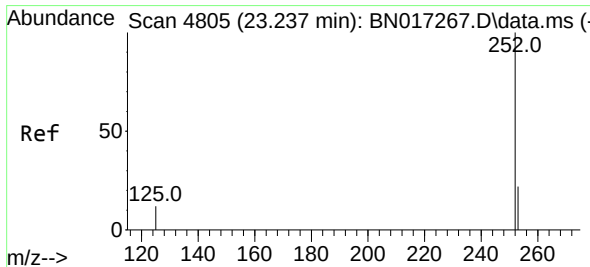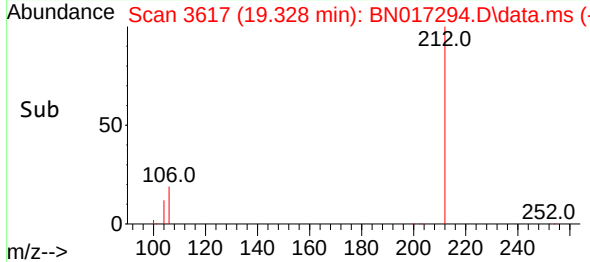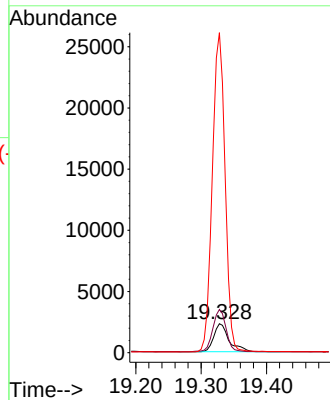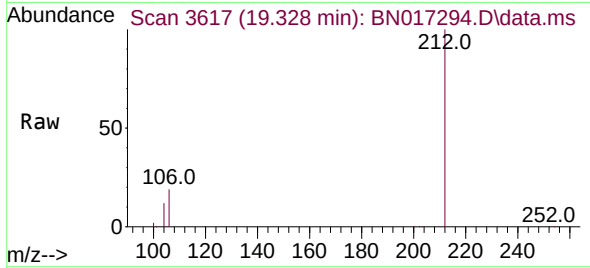

#26
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.192 min Scan# 4790
Delta R.T. -0.045 min
Lab File: BN017294.D
Acq: 04 Nov 2021 02:46

Tgt Ion:252 Resp: 8462
Ion Ratio Lower Upper
252 100
253 38.0 19.3 28.9#
125 25.3 10.8 16.2#

