

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017296.D
 Acq On : 04 Nov 2021 03:58
 Operator : CG/JU
 Sample : M4374-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG336

Quant Time: Nov 08 01:07:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.515	152	4860	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	19829	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	12414	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.924	188	26799	0.400	ng/ul	0.00
17) Chrysene-d12	21.133	240	24355	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	27220	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	23207	4.295	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	10271	0.355	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	32489	0.509	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.329	202	4084	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.191	252	8845	0.097	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017296.D
Acq On : 04 Nov 2021 03:58
Operator : CG/JU
Sample : M4374-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG336

Quant Time: Nov 08 01:07:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration

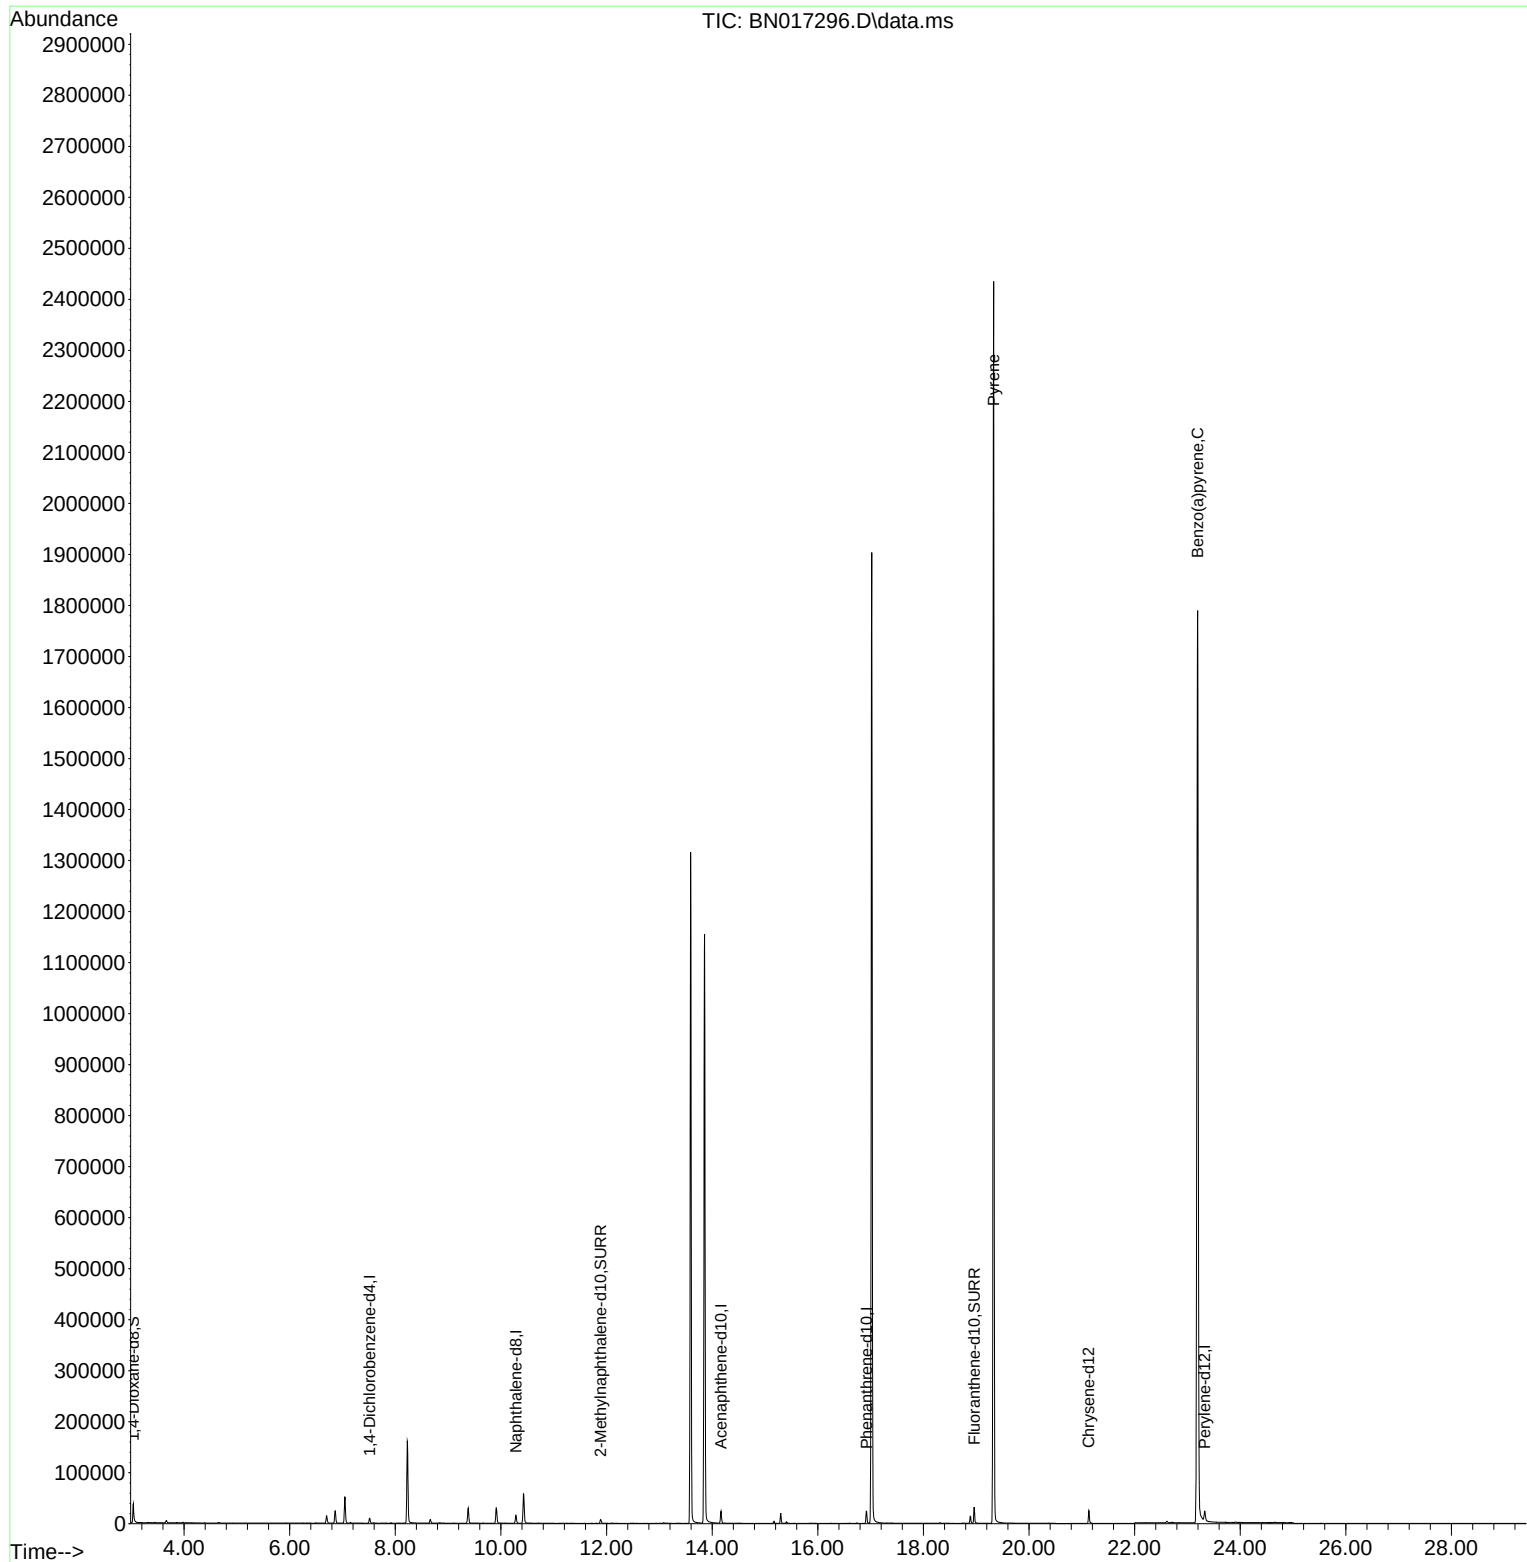

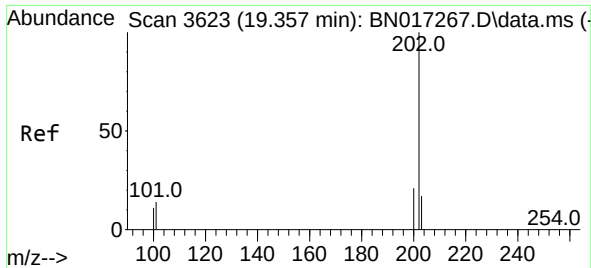

#20

Pyrene

Concen: 0.046 ng/ul

RT: 19.329 min Scan# 3

Delta R.T. -0.028 min

Lab File: BN017296.D

Acq: 04 Nov 2021 03:58

Instrument :





BNA_N

ClientSampleId :

BG336

Tgt Ion:202 Resp: 4084

Ion	Ratio	Lower	Upper
202	100		
101	143.8	10.3	15.5#
100	1045.6	8.2	12.2#

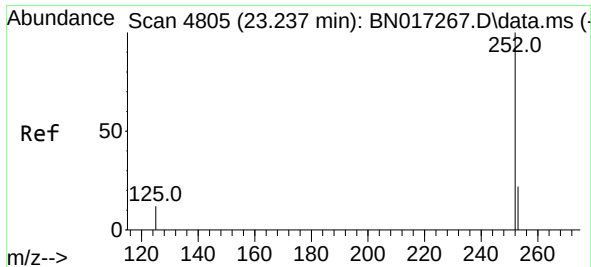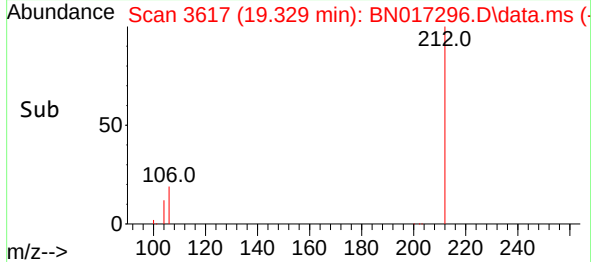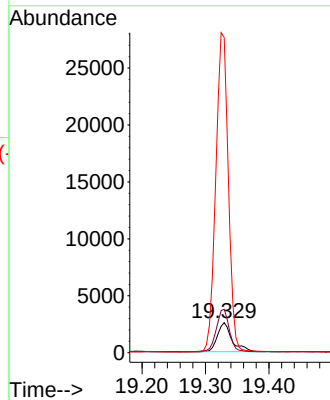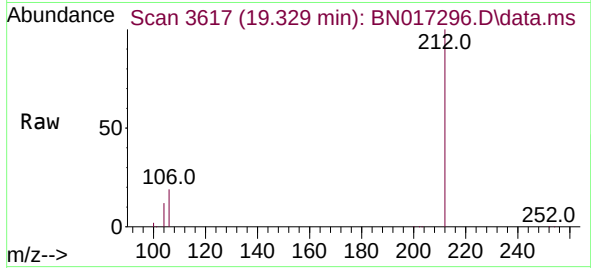

#26

Benzo(a)pyrene

Concen: 0.097 ng/ul

RT: 23.191 min Scan# 4789

Delta R.T. -0.046 min

Lab File: BN017296.D

Acq: 04 Nov 2021 03:58

Tgt Ion:252 Resp: 8845

Ion	Ratio	Lower	Upper
252	100		
253	37.2	19.3	28.9#
125	25.2	10.8	16.2#

