

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017298.D
 Acq On : 04 Nov 2021 05:46
 Operator : CG/JU
 Sample : PB140424BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK424

Quant Time: Nov 08 01:07:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	5114	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	19861	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	12391	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.924	188	26700	0.400	ng/ul	0.00
17) Chrysene-d12	21.136	240	21834	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	26125	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	29730	5.229	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	9145	0.315	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	23633	0.413	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.170	166	2962	0.059	ng/ul#	14
20) Pyrene	19.329	202	3022	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.190	252	7243	0.083	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017298.D
Acq On : 04 Nov 2021 05:46
Operator : CG/JU
Sample : PB140424BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK424

Quant Time: Nov 08 01:07:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




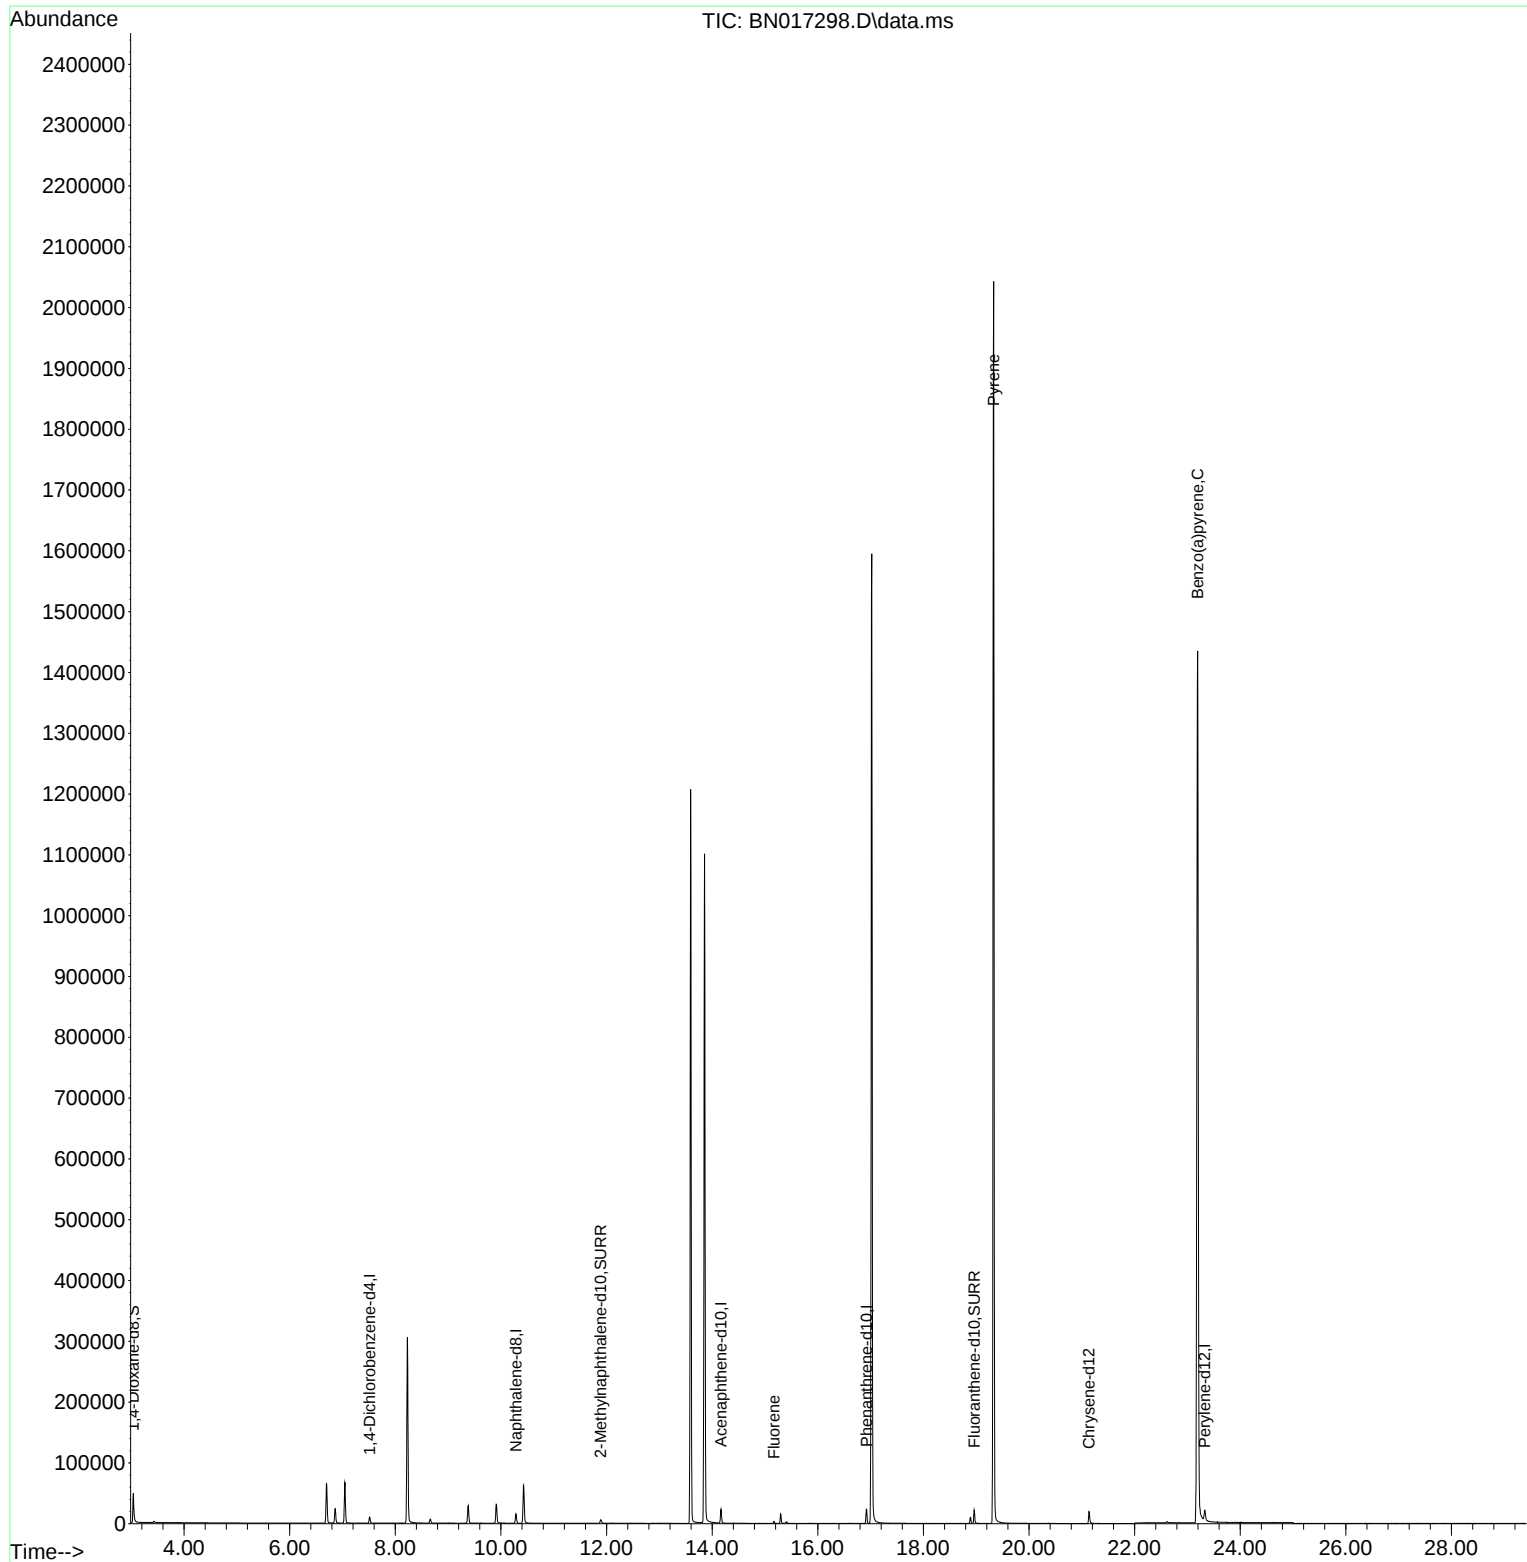


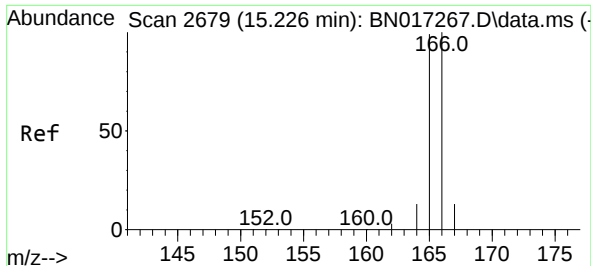

#12
Fluorene
Concen: 0.059 ng/ul
RT: 15.170 min Scan# 2667
Delta R.T. -0.056 min
Lab File: BN017298.D
Acq: 04 Nov 2021 05:46




Instrument :
BNA_N
ClientSampleId :
SBLK424


Tgt Ion:166 Resp: 2962
Ion Ratio Lower Upper
166 100
165 7.1 77.7 116.5#
167 34.2 11.1 16.7#

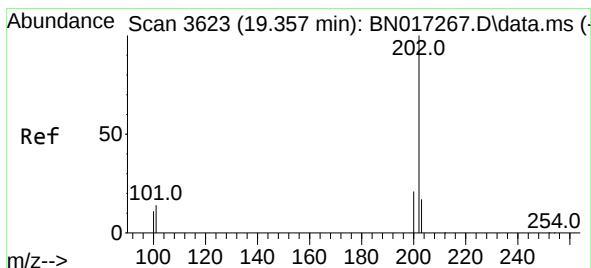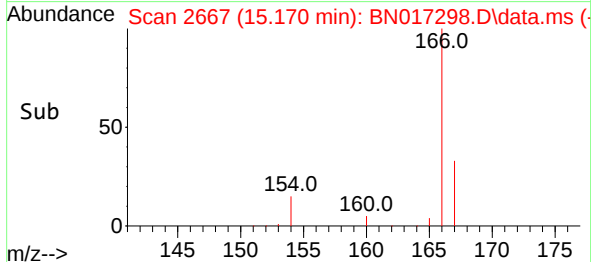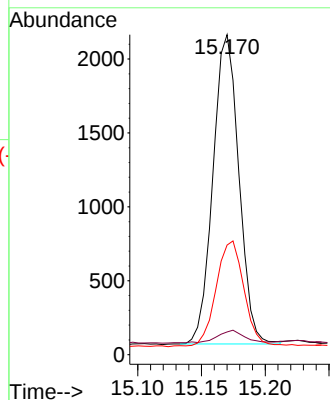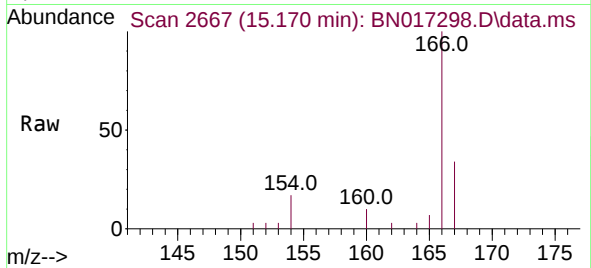

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.329 min Scan# 3617
Delta R.T. -0.028 min
Lab File: BN017298.D
Acq: 04 Nov 2021 05:46

Tgt Ion:202 Resp: 3022
Ion Ratio Lower Upper
202 100
101 145.0 10.3 15.5#
100 1033.9 8.2 12.2#

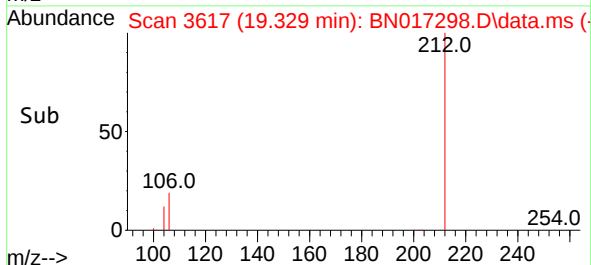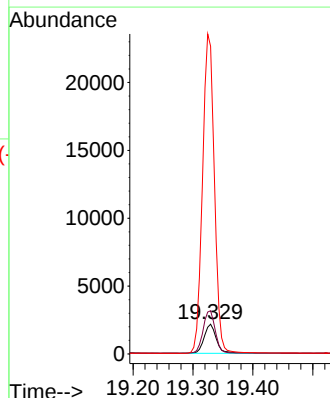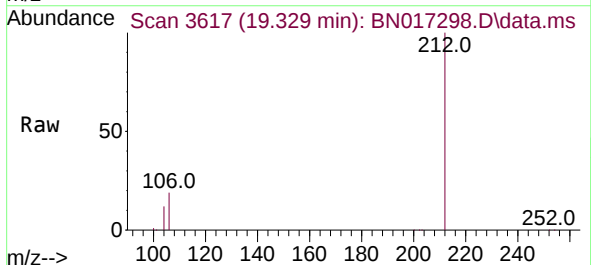

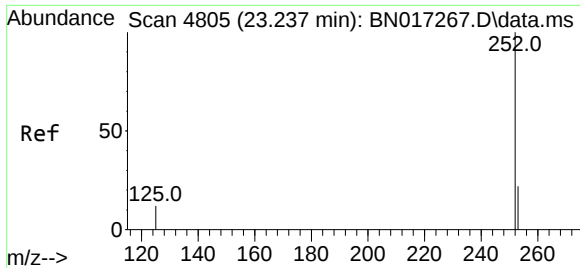

#26

Benzo(a)pyrene

Concen: 0.083 ng/ul

RT: 23.190 min Scan# 41

Delta R.T. -0.046 min

Lab File: BN017298.D


Acq: 04 Nov 2021 05:46

Instrument :

BNA_N

ClientSampleId :

SBLK424

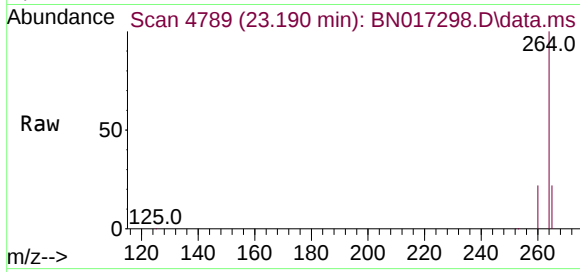

Tgt Ion:252 Resp: 7243

Ion Ratio Lower Upper

252 100

253 37.7 19.3 28.9#

125 24.9 10.8 16.2#

