

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017299.D
 Acq On : 04 Nov 2021 06:22
 Operator : CG/JU
 Sample : PB140425BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK425

Quant Time: Nov 08 01:08:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.515	152	5474	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	21931	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	13652	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.919	188	28624	0.400	ng/ul	0.00
17) Chrysene-d12	21.136	240	22077	0.400	ng/ul	0.00
23) Perylene-d12	23.331	264	26411	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	31341	5.150	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	10500	0.328	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	25237	0.436	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.170	166	3271	0.059	ng/ul#	13
20) Pyrene	19.329	202	3123	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.191	252	7386	0.084	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017299.D
Acq On : 04 Nov 2021 06:22
Operator : CG/JU
Sample : PB140425BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK425

Quant Time: Nov 08 01:08:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




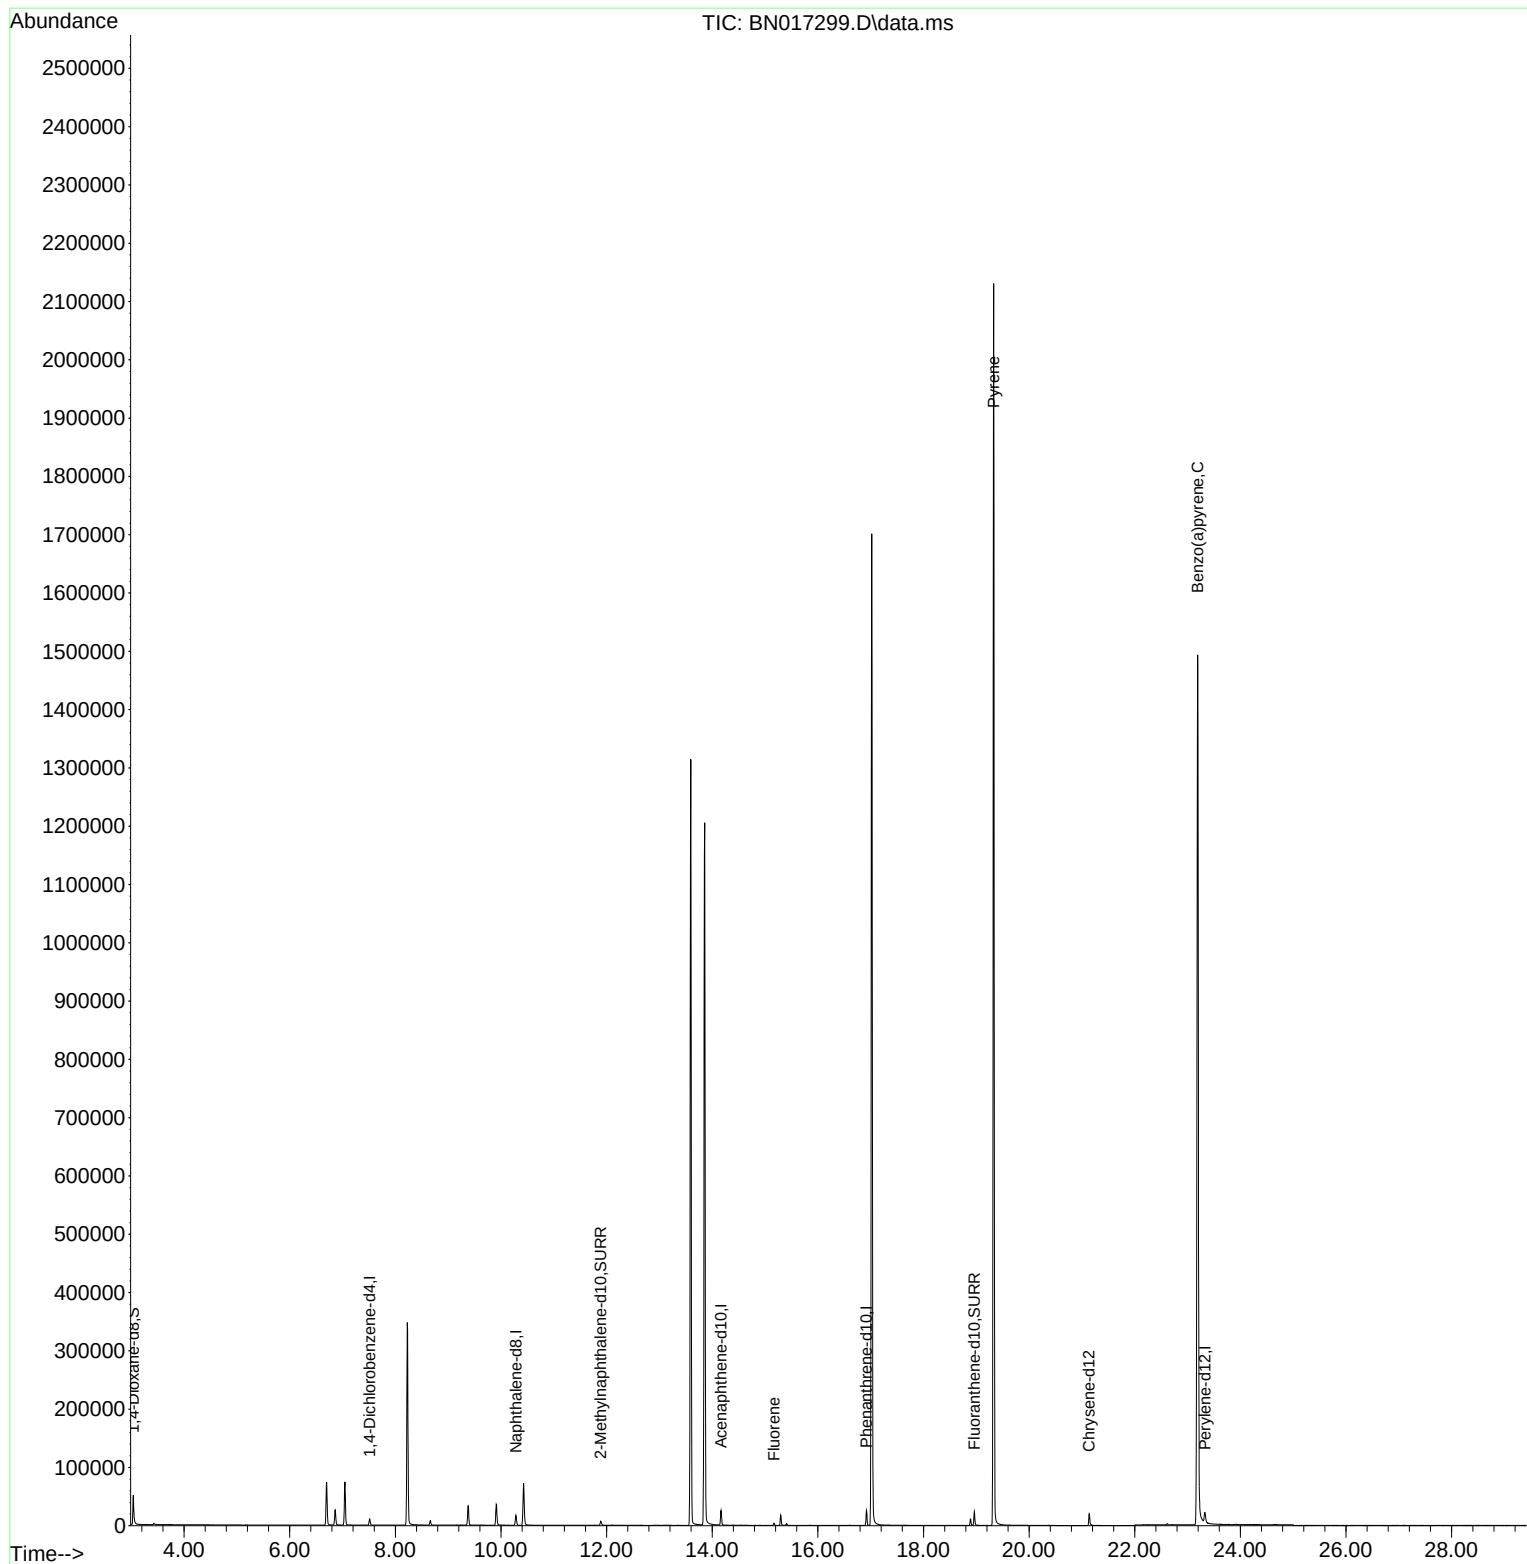


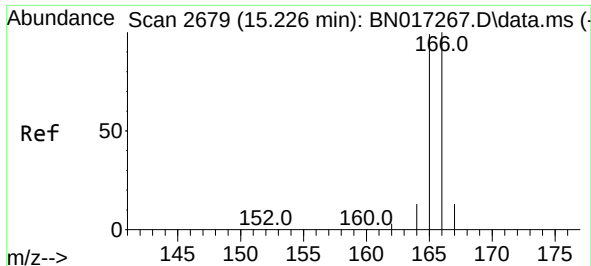

#12
Fluorene
Concen: 0.059 ng/ul
RT: 15.170 min Scan# 2667
Delta R.T. -0.056 min
Lab File: BN017299.D
Acq: 04 Nov 2021 06:22




Instrument :
BNA_N
ClientSampleId :
SBLK425


Tgt Ion:166 Resp: 3271
Ion Ratio Lower Upper
166 100
165 6.6 77.7 116.5#
167 36.0 11.1 16.7#

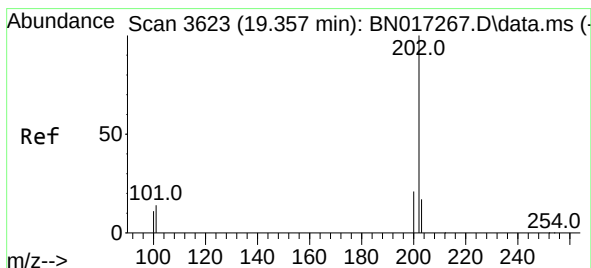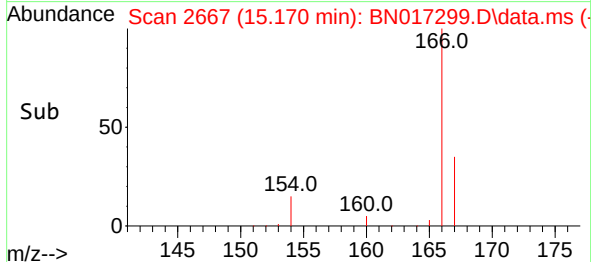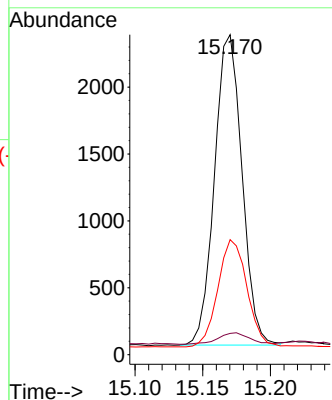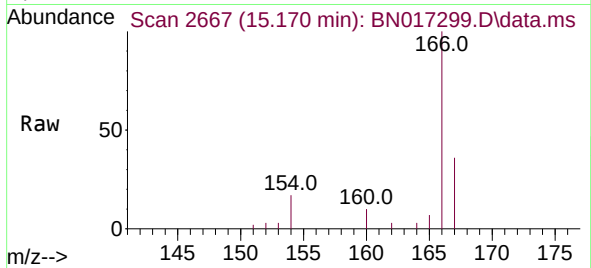

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.329 min Scan# 3617
Delta R.T. -0.027 min
Lab File: BN017299.D
Acq: 04 Nov 2021 06:22

Tgt Ion:202 Resp: 3123
Ion Ratio Lower Upper
202 100
101 145.2 10.3 15.5#
100 1016.5 8.2 12.2#

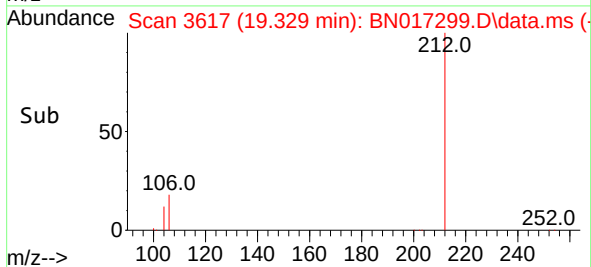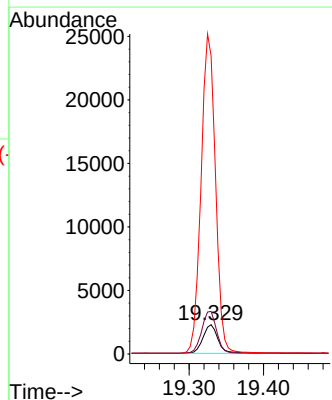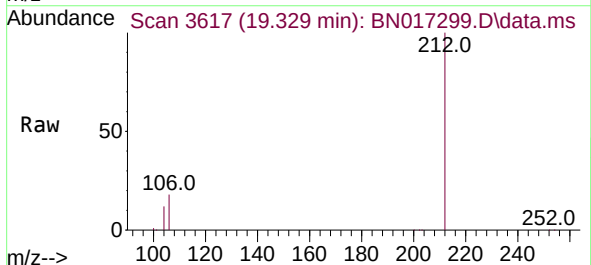

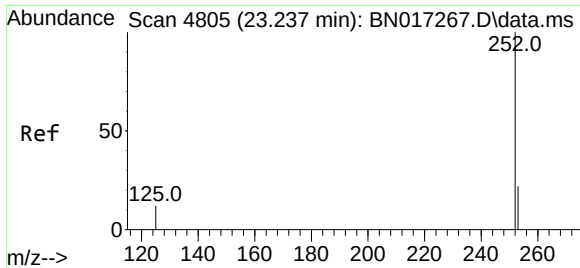

#26

Benzo(a)pyrene

Concen: 0.084 ng/ul

RT: 23.191 min Scan# 41

Delta R.T. -0.046 min

Lab File: BN017299.D


Acq: 04 Nov 2021 06:22

Instrument :

BNA_N

ClientSampleId :

SBLK425

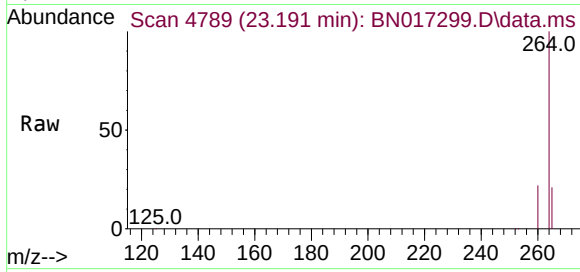

Tgt Ion:252 Resp: 7386

Ion Ratio Lower Upper

252 100

253 37.7 19.3 28.9#

125 23.9 10.8 16.2#

