

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017310.D
 Acq On : 04 Nov 2021 12:57
 Operator : CG/JU
 Sample : M4413-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG361

Quant Time: Nov 08 01:09:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.515	152	4393	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	17692	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	11119	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.924	188	24343	0.400	ng/ul	0.00
17) Chrysene-d12	21.136	240	22322	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	25175	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	22249	4.555	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.890	152	9849	0.381	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	29844	0.510	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.329	202	3571	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.193	252	7646	0.091	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017310.D
Acq On : 04 Nov 2021 12:57
Operator : CG/JU
Sample : M4413-04
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG361

Quant Time: Nov 08 01:09:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




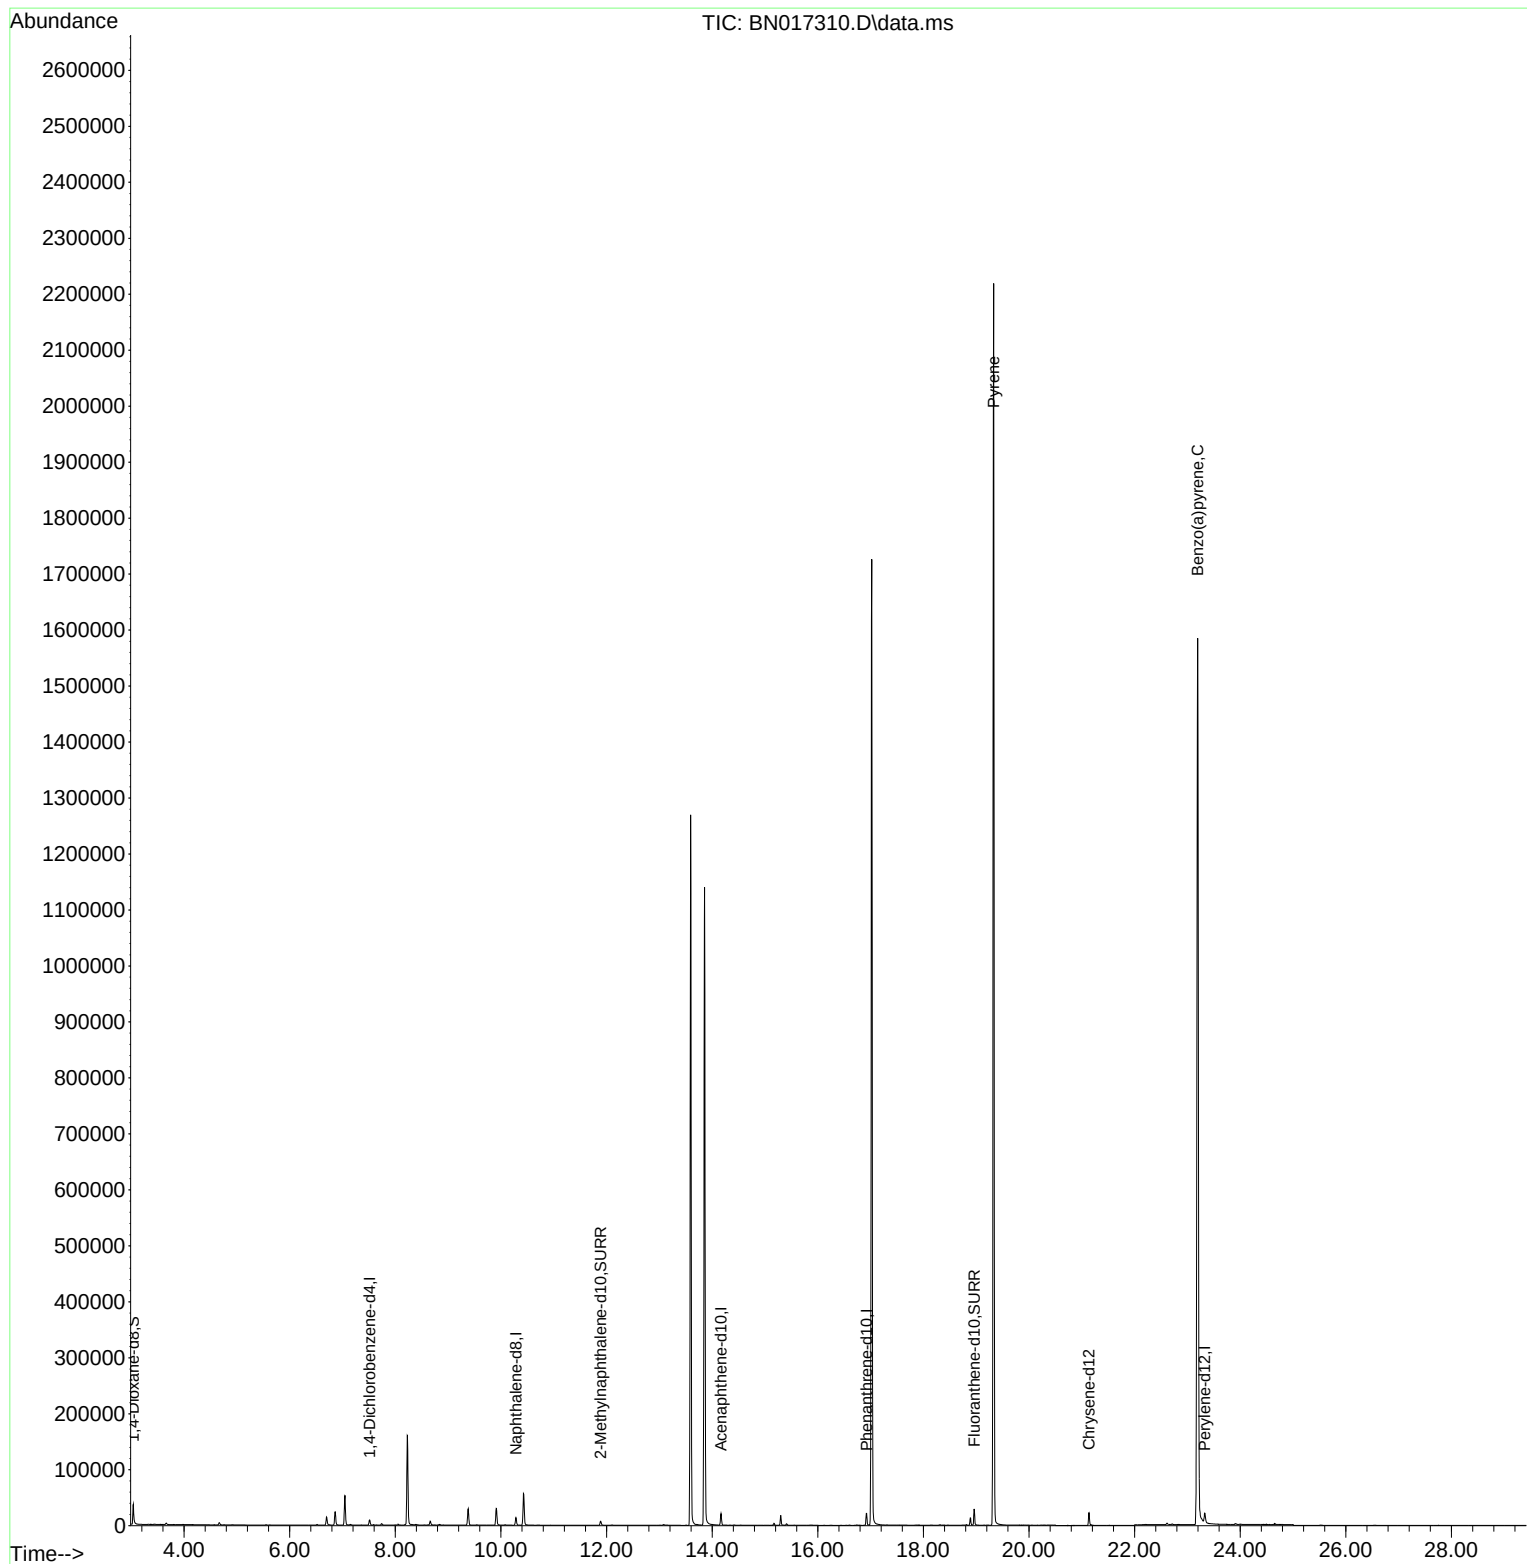


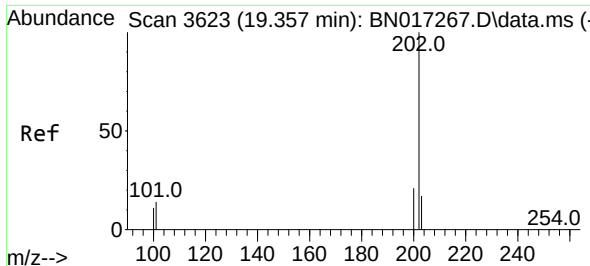

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.329 min Scan# 3617
Delta R.T. -0.027 min
Lab File: BN017310.D
Acq: 04 Nov 2021 12:57

Instrument :
BNA_N
ClientSampleId :
BG361

Tgt Ion:202 Resp: 3571
Ion Ratio Lower Upper
202 100
101 146.1 10.3 15.5#
100 1032.9 8.2 12.2#

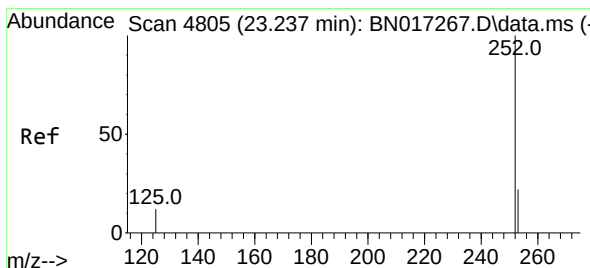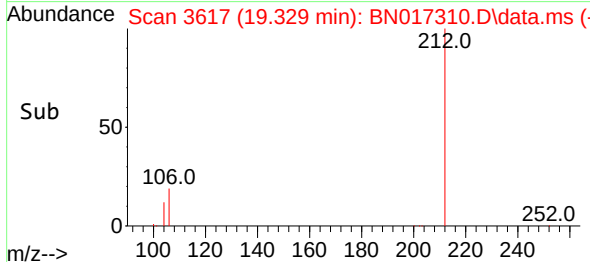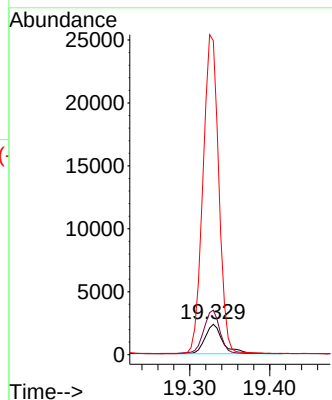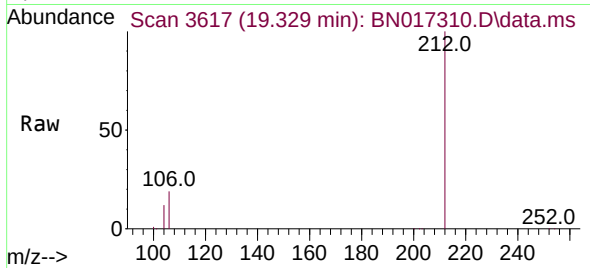

#26
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 23.193 min Scan# 4790
Delta R.T. -0.043 min
Lab File: BN017310.D
Acq: 04 Nov 2021 12:57

Tgt Ion:252 Resp: 7646
Ion Ratio Lower Upper
252 100
253 39.3 19.3 28.9#
125 26.2 10.8 16.2#

