

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017311.D
 Acq On : 04 Nov 2021 13:33
 Operator : CG/JU
 Sample : M4413-05
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG362

Quant Time: Nov 08 01:09:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4250	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	17003	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.165	164	10608	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	23234	0.400	ng/ul	0.00
17) Chrysene-d12	21.135	240	21973	0.400	ng/ul	0.00
23) Perylene-d12	23.329	264	25262	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	21498	4.550	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	9008	0.363	ng/ul	0.00
18) Fluoranthene-d10	18.961	212	27692	0.481	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.328	202	3497	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.192	252	7905	0.094	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017311.D
Acq On : 04 Nov 2021 13:33
Operator : CG/JU
Sample : M4413-05
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG362

Quant Time: Nov 08 01:09:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




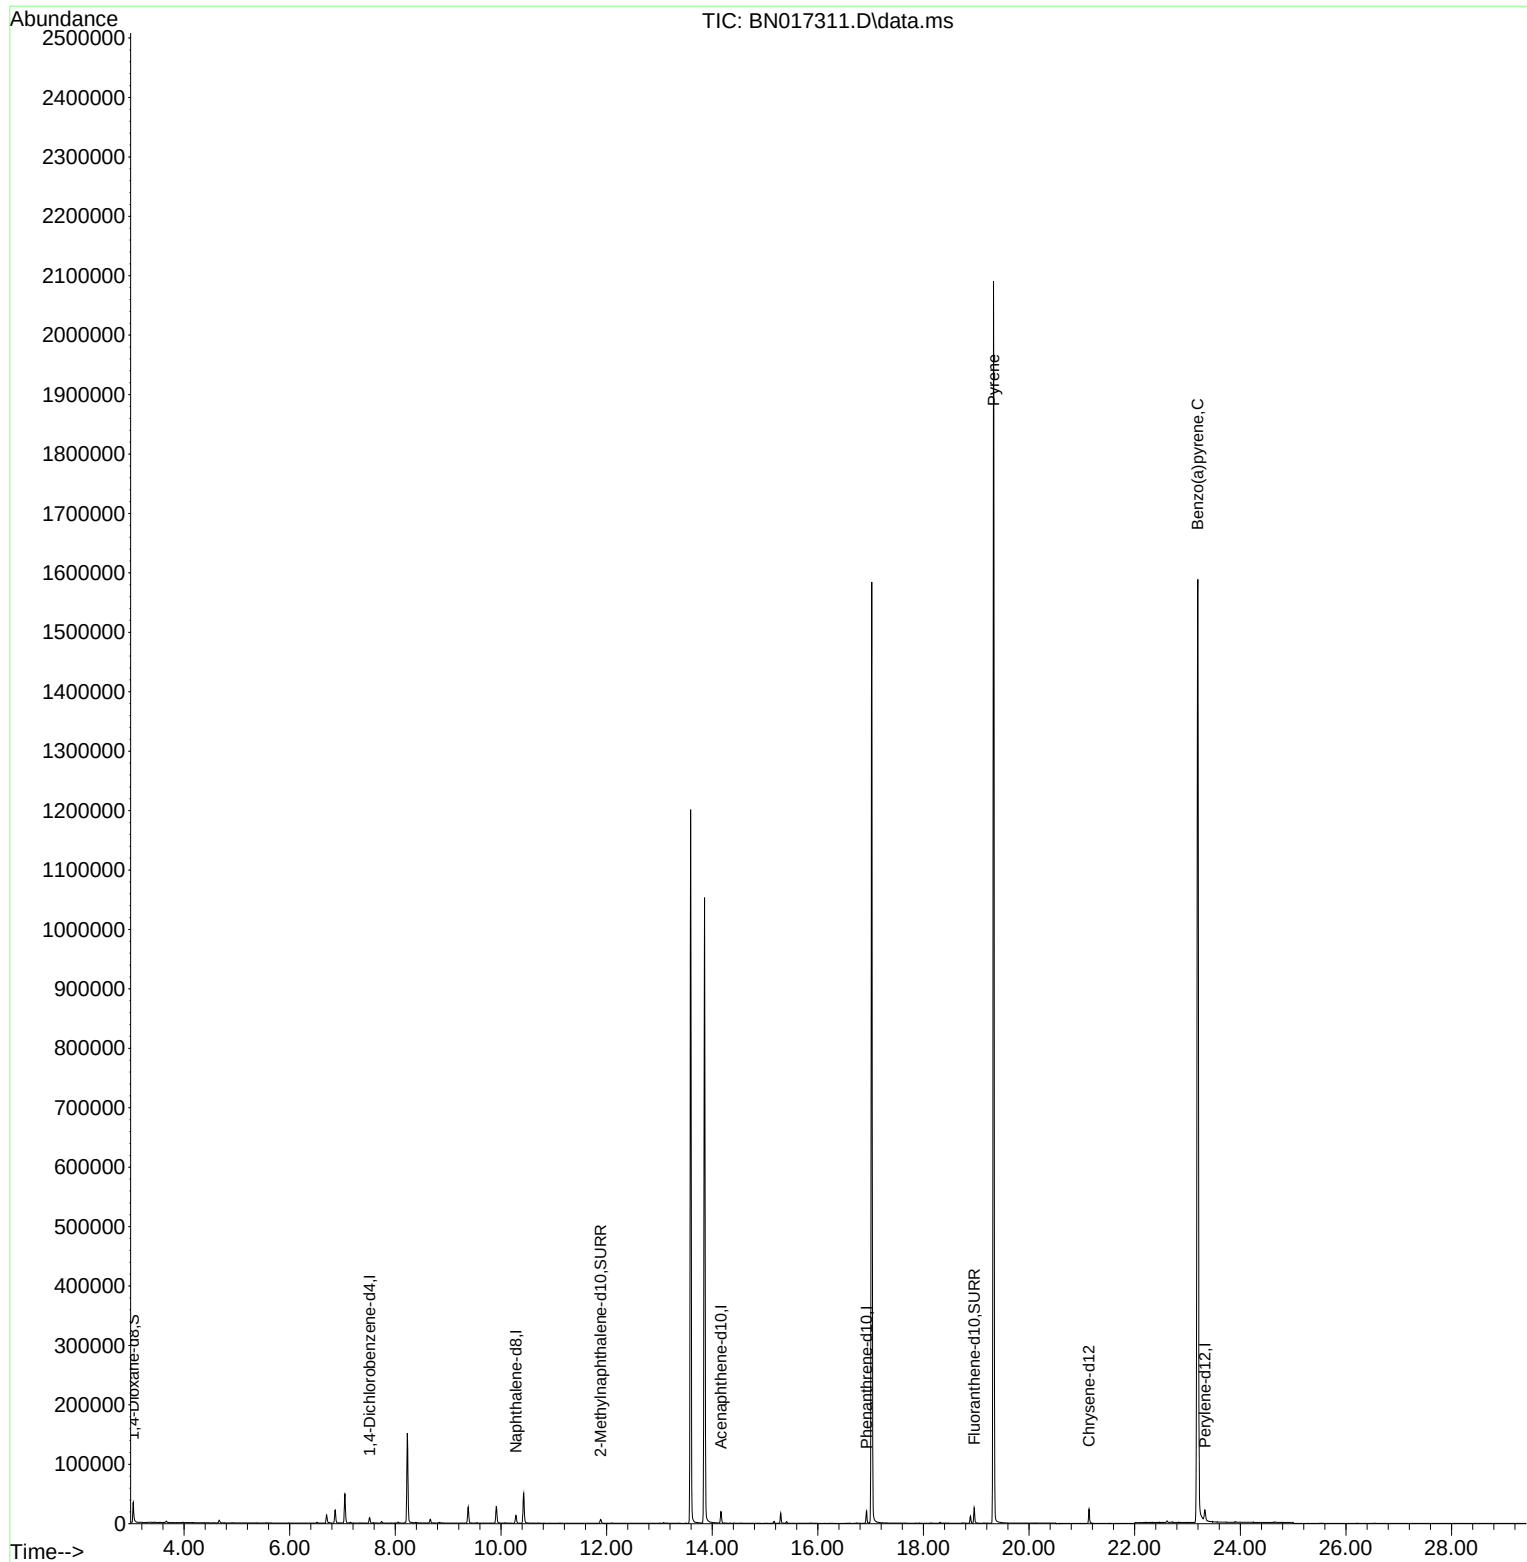


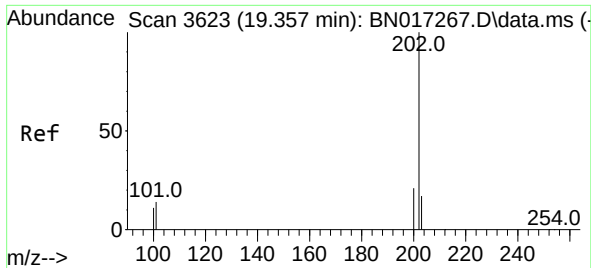

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.328 min Scan# 3617
Delta R.T. -0.029 min
Lab File: BN017311.D
Acq: 04 Nov 2021 13:33

Instrument :
BNA_N
ClientSampleId :
BG362

Tgt Ion:202 Resp: 3497
Ion Ratio Lower Upper
202 100
101 145.9 10.3 15.5#
100 1065.5 8.2 12.2#

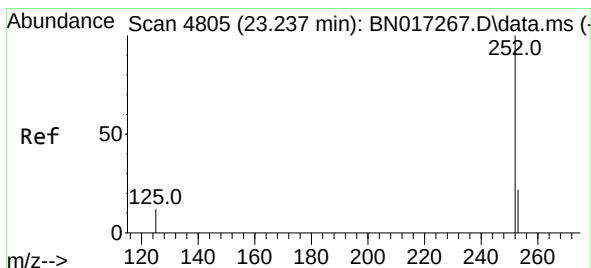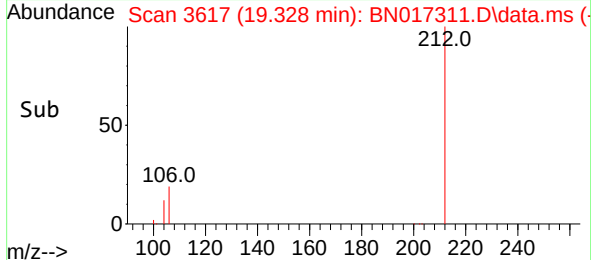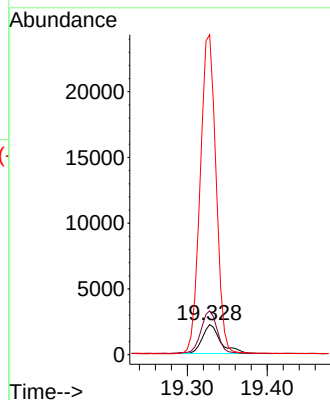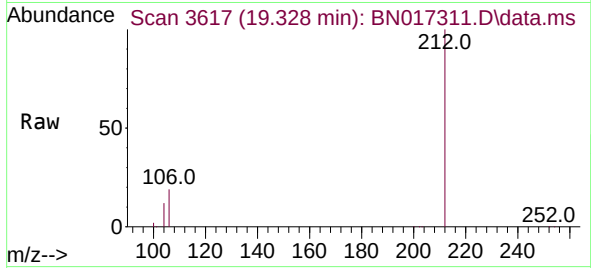

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.192 min Scan# 4790
Delta R.T. -0.045 min
Lab File: BN017311.D
Acq: 04 Nov 2021 13:33

Tgt Ion:252 Resp: 7905
Ion Ratio Lower Upper
252 100
253 39.2 19.3 28.9#
125 26.6 10.8 16.2#

