

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017322.D
 Acq On : 04 Nov 2021 20:47
 Operator : CG/JU
 Sample : M4413-06
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG363

Quant Time: Nov 08 01:10:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	5387	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	21859	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	14013	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.919	188	30775	0.400	ng/ul	0.00
17) Chrysene-d12	21.136	240	27803	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	29992	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	31037	5.182	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.884	152	12173	0.381	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	37389	0.513	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.067	88	155	0.024	ng/ul#	55
20) Pyrene	19.329	202	4248	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.193	252	9315	0.093	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017322.D
Acq On : 04 Nov 2021 20:47
Operator : CG/JU
Sample : M4413-06
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG363

Quant Time: Nov 08 01:10:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




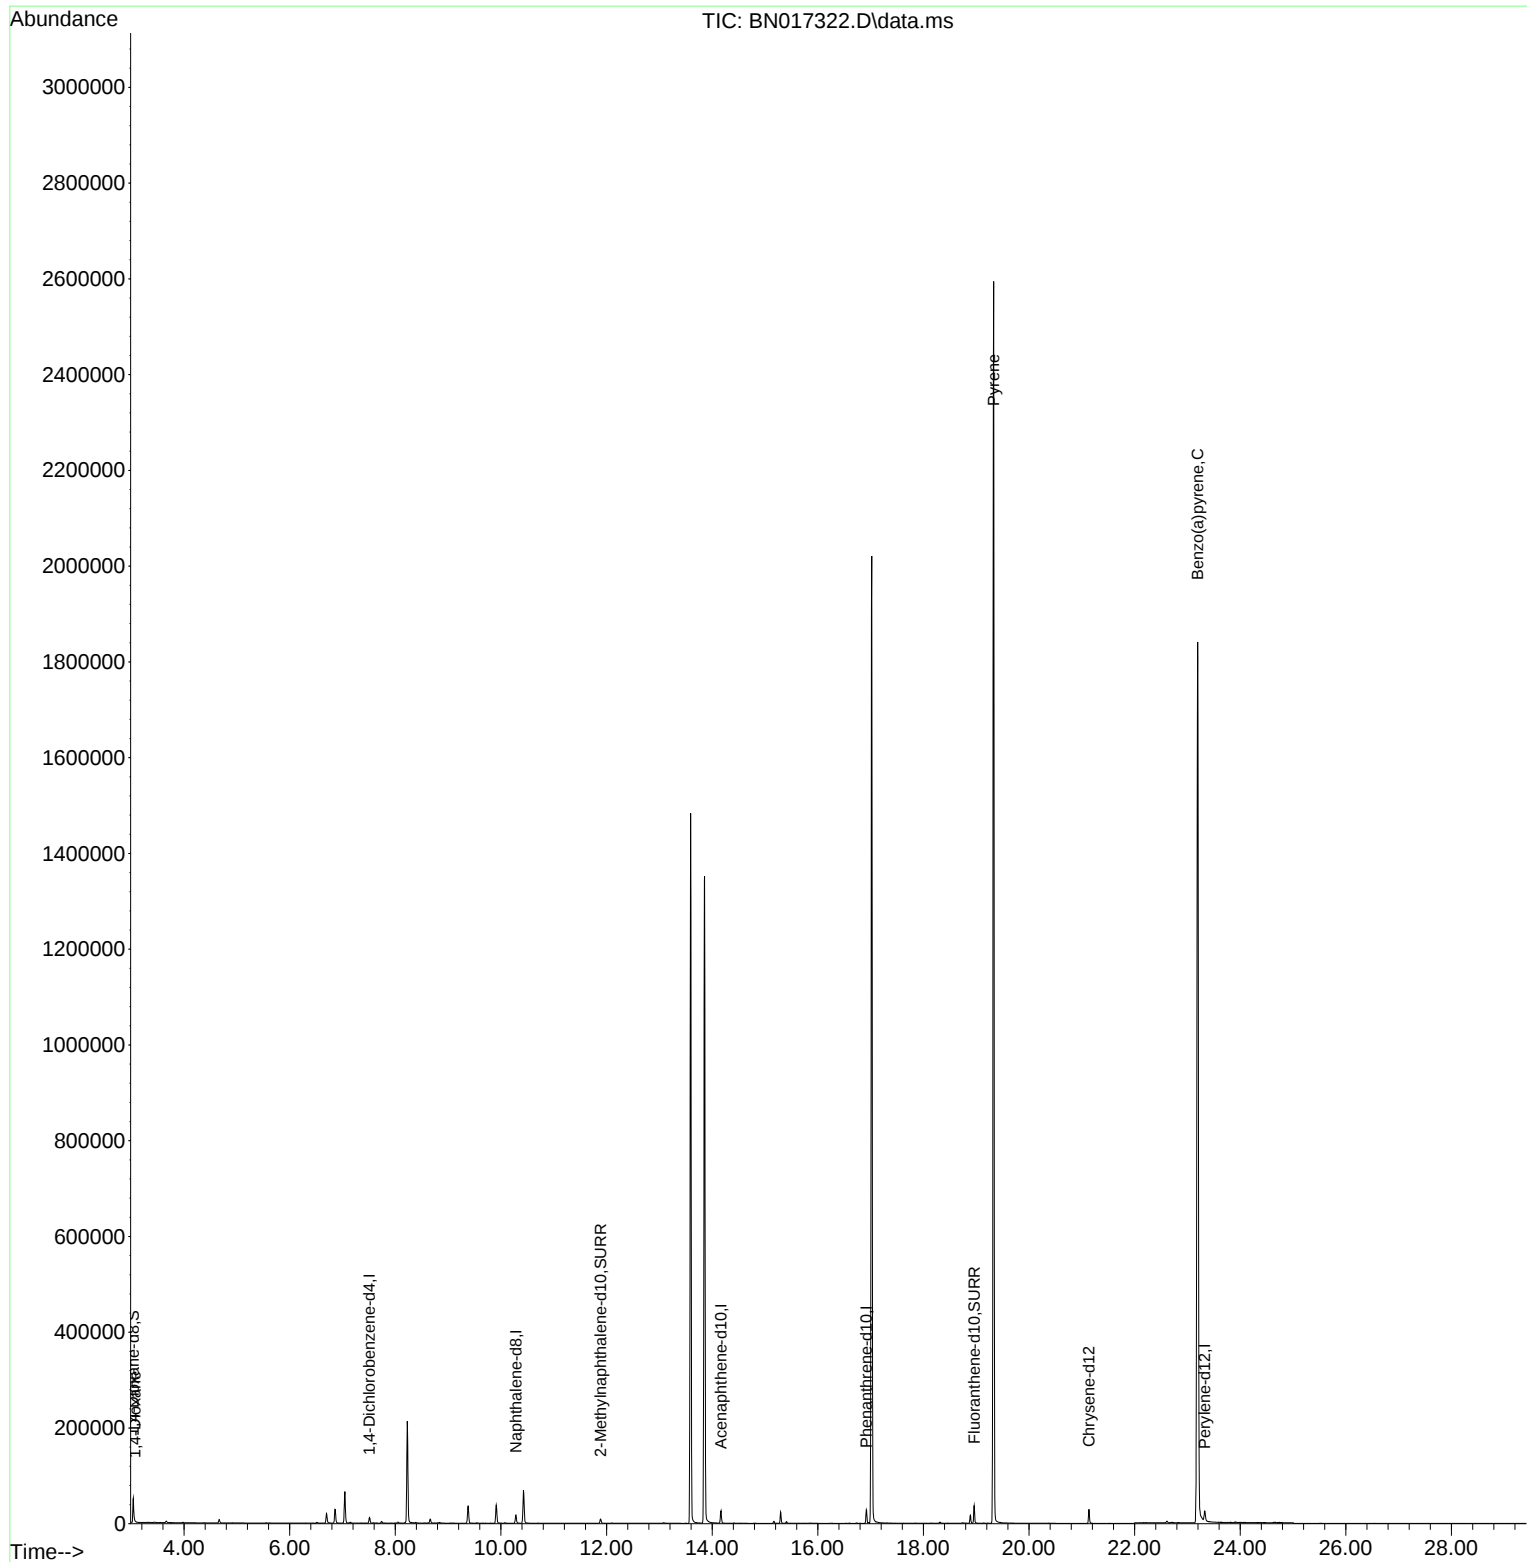


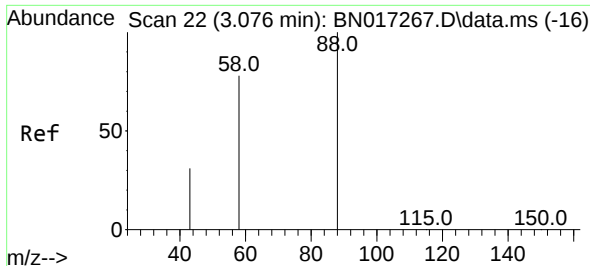

#2
1,4-Dioxane
Concen: 0.024 ng/ul
RT: 3.067 min Scan# 20
Delta R.T. -0.008 min
Lab File: BN017322.D
Acq: 04 Nov 2021 20:47




Instrument :
BNA_N
ClientSampleId :
BG363


Tgt Ion: 88 Resp: 155
Ion Ratio Lower Upper
88 100
43 56.0 31.8 47.6#
58 11.2 41.9 62.9#

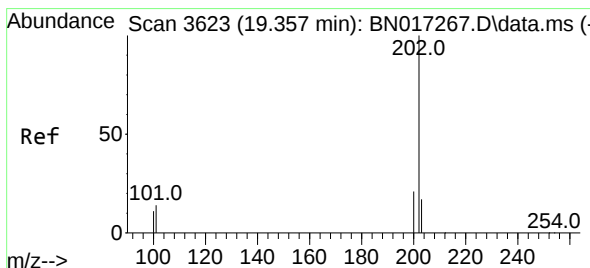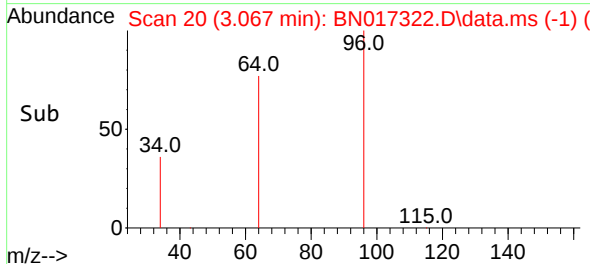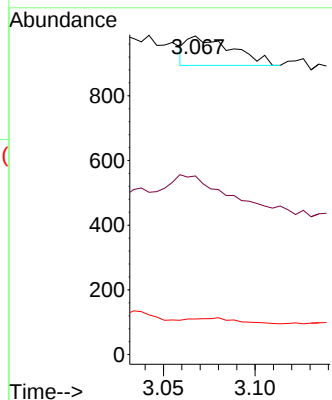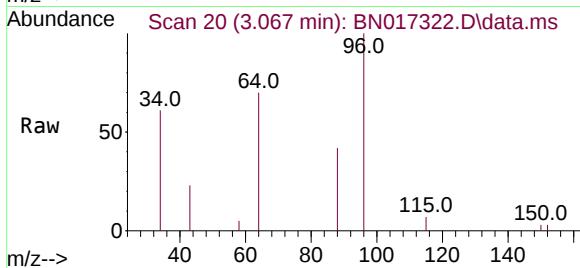

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.329 min Scan# 3617
Delta R.T. -0.028 min
Lab File: BN017322.D
Acq: 04 Nov 2021 20:47


Tgt Ion: 202 Resp: 4248
Ion Ratio Lower Upper
202 100
101 148.3 10.3 15.5#
100 1054.4 8.2 12.2#

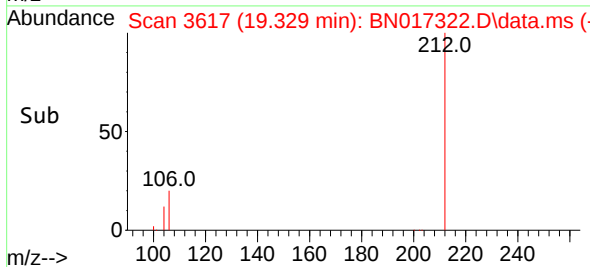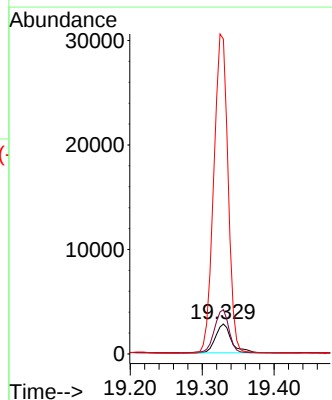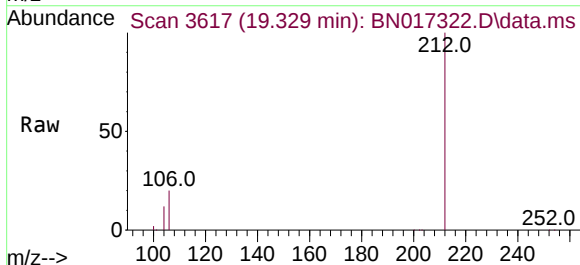

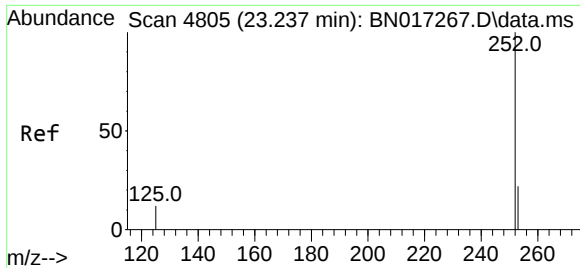

#26
 Benzo(a)pyrene
 Concen: 0.093 ng/ul
 RT: 23.193 min Scan# 41
 Delta R.T. -0.043 min
 Lab File: BN017322.D
 Acq: 04 Nov 2021 20:47

Instrument :
 BNA_N
 ClientSampleId :
 BG363

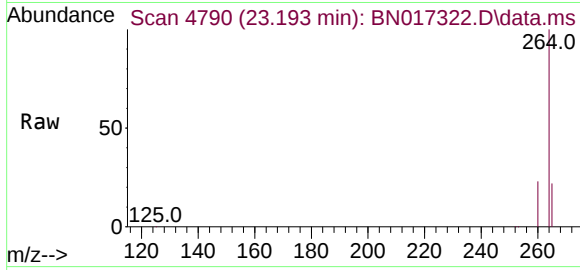

Tgt Ion:	252	Resp:	9315
Ion	Ratio	Lower	Upper
252	100		
253	38.8	19.3	28.9#
125	25.6	10.8	16.2#

