

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017323.D
 Acq On : 04 Nov 2021 21:23
 Operator : CG/JU
 Sample : M4413-07
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG364

Quant Time: Nov 08 01:10:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	5583	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	22099	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.165	164	14049	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	31438	0.400	ng/ul	0.00
17) Chrysene-d12	21.135	240	28145	0.400	ng/ul	0.00
23) Perylene-d12	23.329	264	28623	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	27050	4.358	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	10416	0.323	ng/ul	0.00
18) Fluoranthene-d10	18.961	212	38938	0.528	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.076	88	192	0.029	ng/ul#	56
20) Pyrene	19.328	202	4526	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.195	252	8593	0.090	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017323.D
Acq On : 04 Nov 2021 21:23
Operator : CG/JU
Sample : M4413-07
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG364

Quant Time: Nov 08 01:10:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




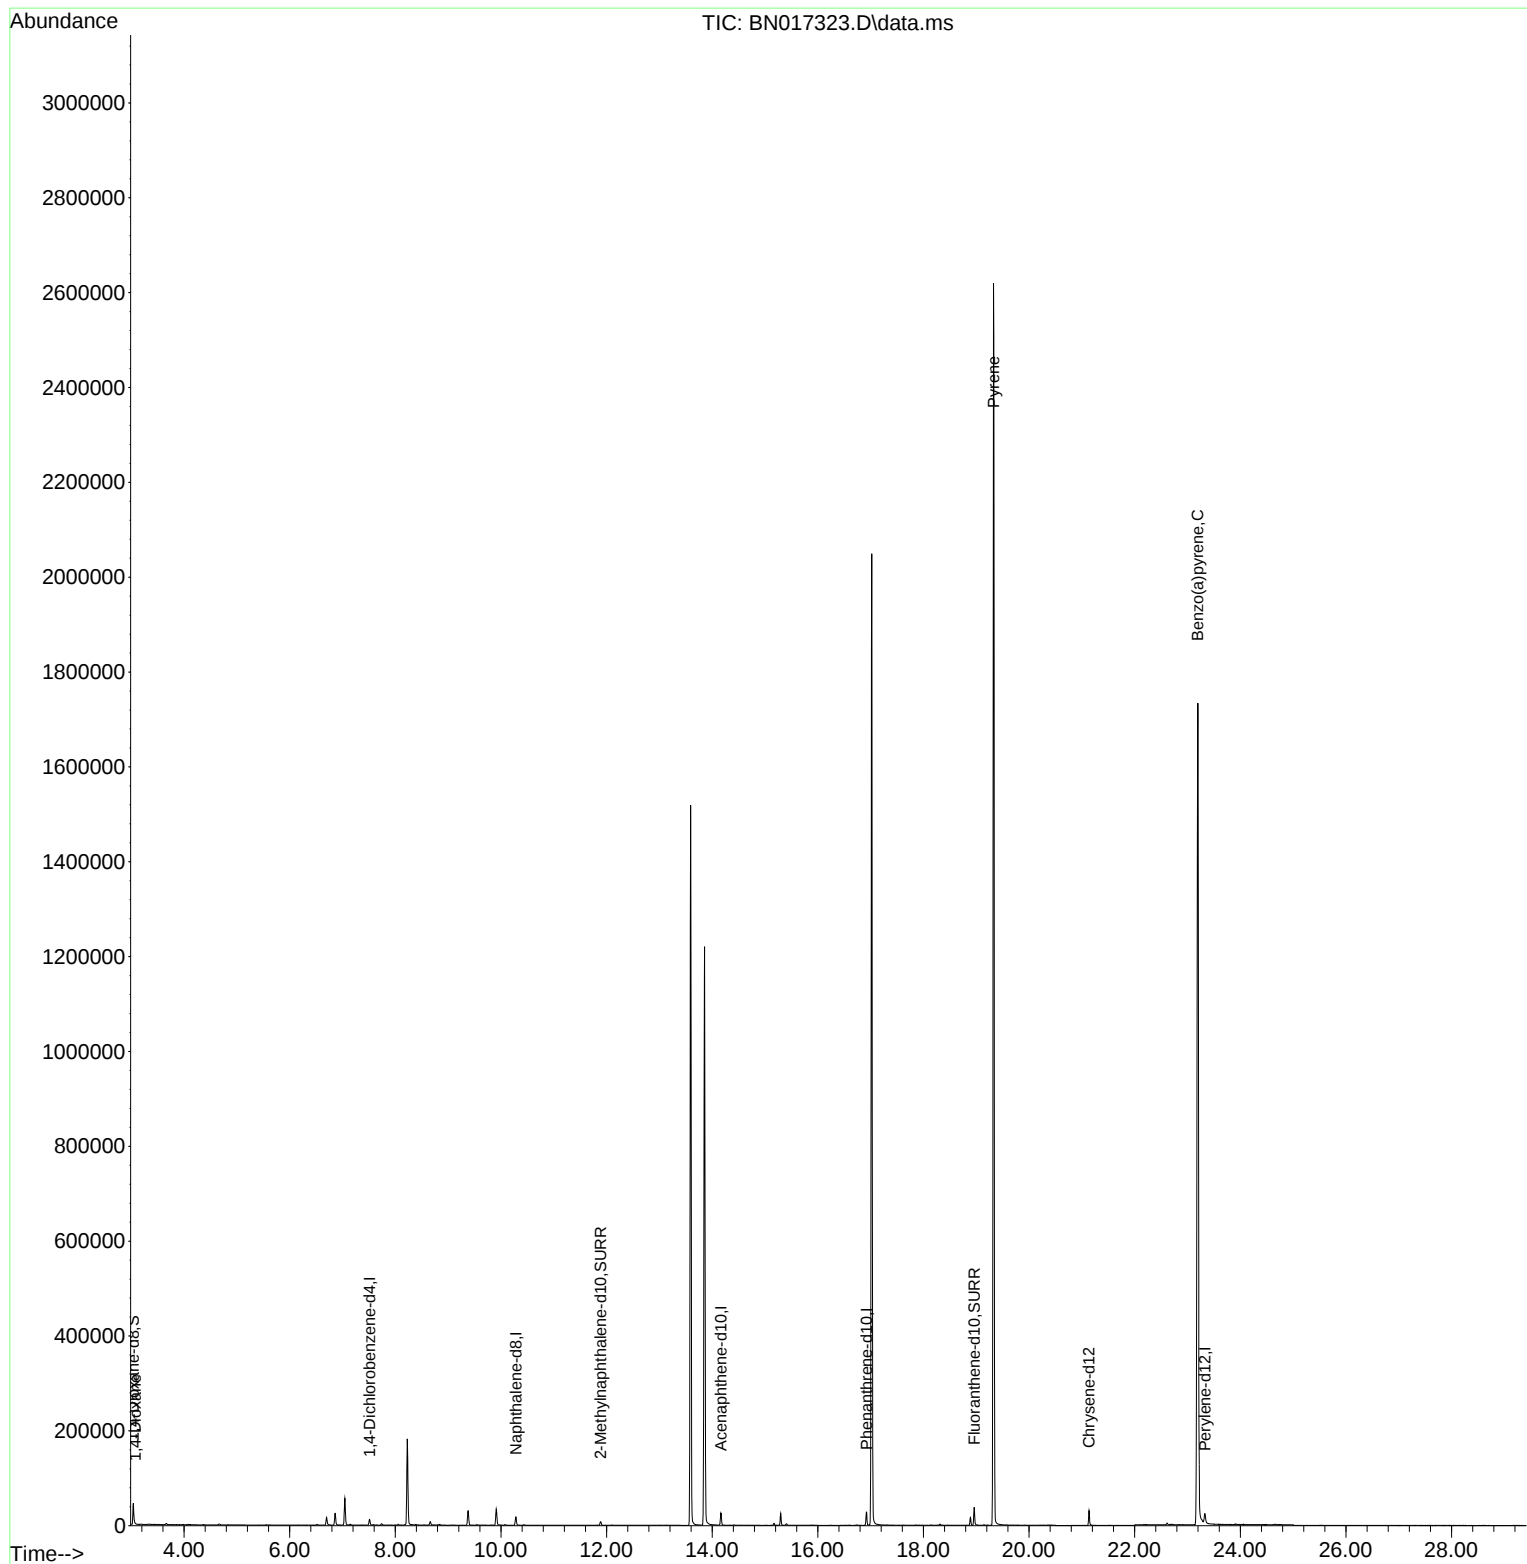


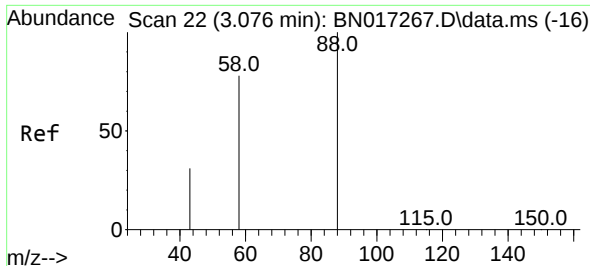

#2
 1,4-Dioxane
 Concen: 0.029 ng/ul
 RT: 3.076 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN017323.D
 Acq: 04 Nov 2021 21:23




Instrument :
 BNA_N
 ClientSampleId :
 BG364


Tgt Ion: 88 Resp: 192
 Ion Ratio Lower Upper
 88 100
 43 57.7 31.8 47.6#
 58 14.0 41.9 62.9#

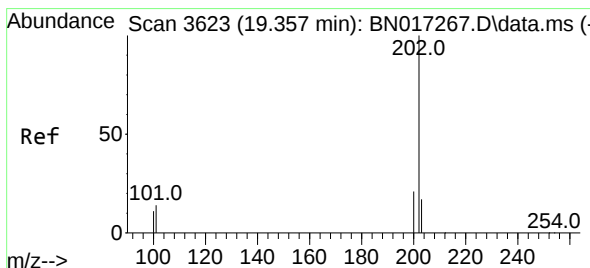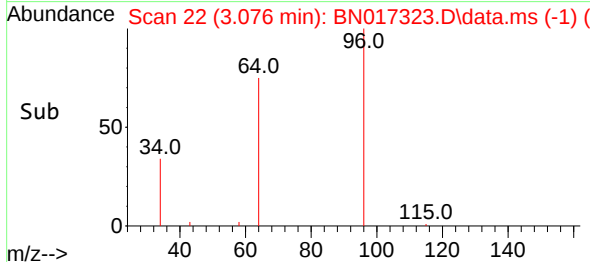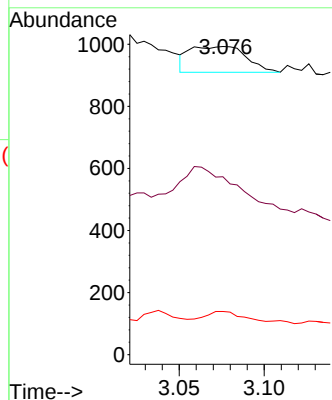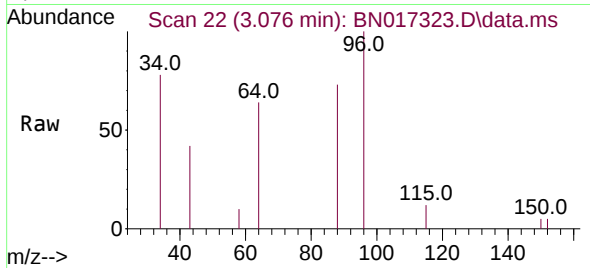

#20
 Pyrene
 Concen: 0.044 ng/ul
 RT: 19.328 min Scan# 3617
 Delta R.T. -0.029 min
 Lab File: BN017323.D
 Acq: 04 Nov 2021 21:23

Tgt Ion: 202 Resp: 4526
 Ion Ratio Lower Upper
 202 100
 101 150.6 10.3 15.5#
 100 1104.6 8.2 12.2#

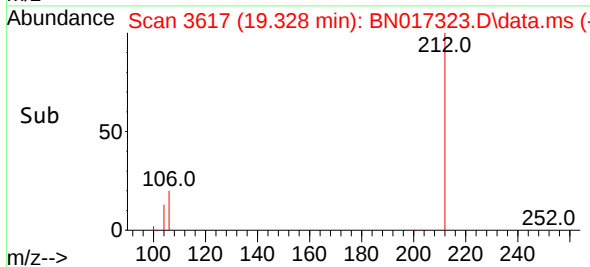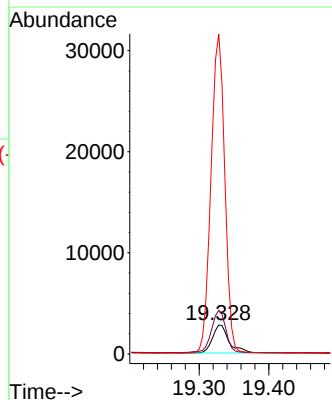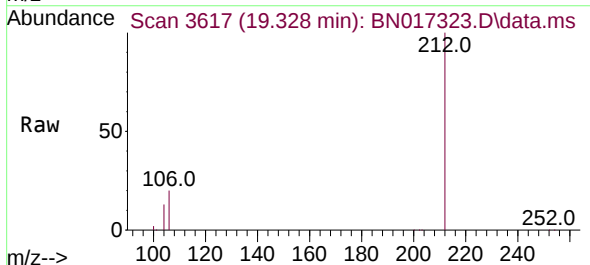

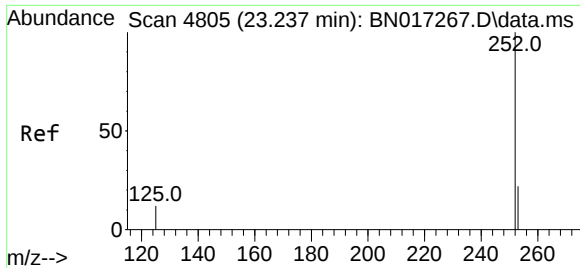

#26

Benzo(a)pyrene

Concen: 0.090 ng/ul

RT: 23.195 min Scan# 41

Delta R.T. -0.042 min

Lab File: BN017323.D


Acq: 04 Nov 2021 21:23

Instrument :

BNA_N

ClientSampleId :

BG364

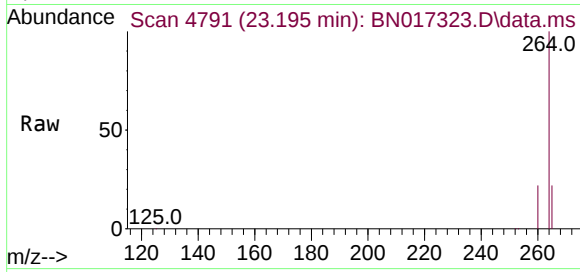

Tgt Ion:252 Resp: 8593

Ion Ratio Lower Upper

252 100

253 39.2 19.3 28.9#

125 26.2 10.8 16.2#

