

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017325.D
 Acq On : 04 Nov 2021 22:35
 Operator : CG/JU
 Sample : M4413-09
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG366

Quant Time: Nov 08 01:10:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	5820	0.400	ng/ul	0.00
4) Naphthalene-d8	10.284	136	22872	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.166	164	14517	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.919	188	32259	0.400	ng/ul	0.00
17) Chrysene-d12	21.133	240	28847	0.400	ng/ul	0.00
23) Perylene-d12	23.328	264	28971	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	29546	4.566	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.884	152	10925	0.327	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	36249	0.479	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.329	202	4081	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.194	252	8167	0.084	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017325.D
Acq On : 04 Nov 2021 22:35
Operator : CG/JU
Sample : M4413-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG366

Quant Time: Nov 08 01:10:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration




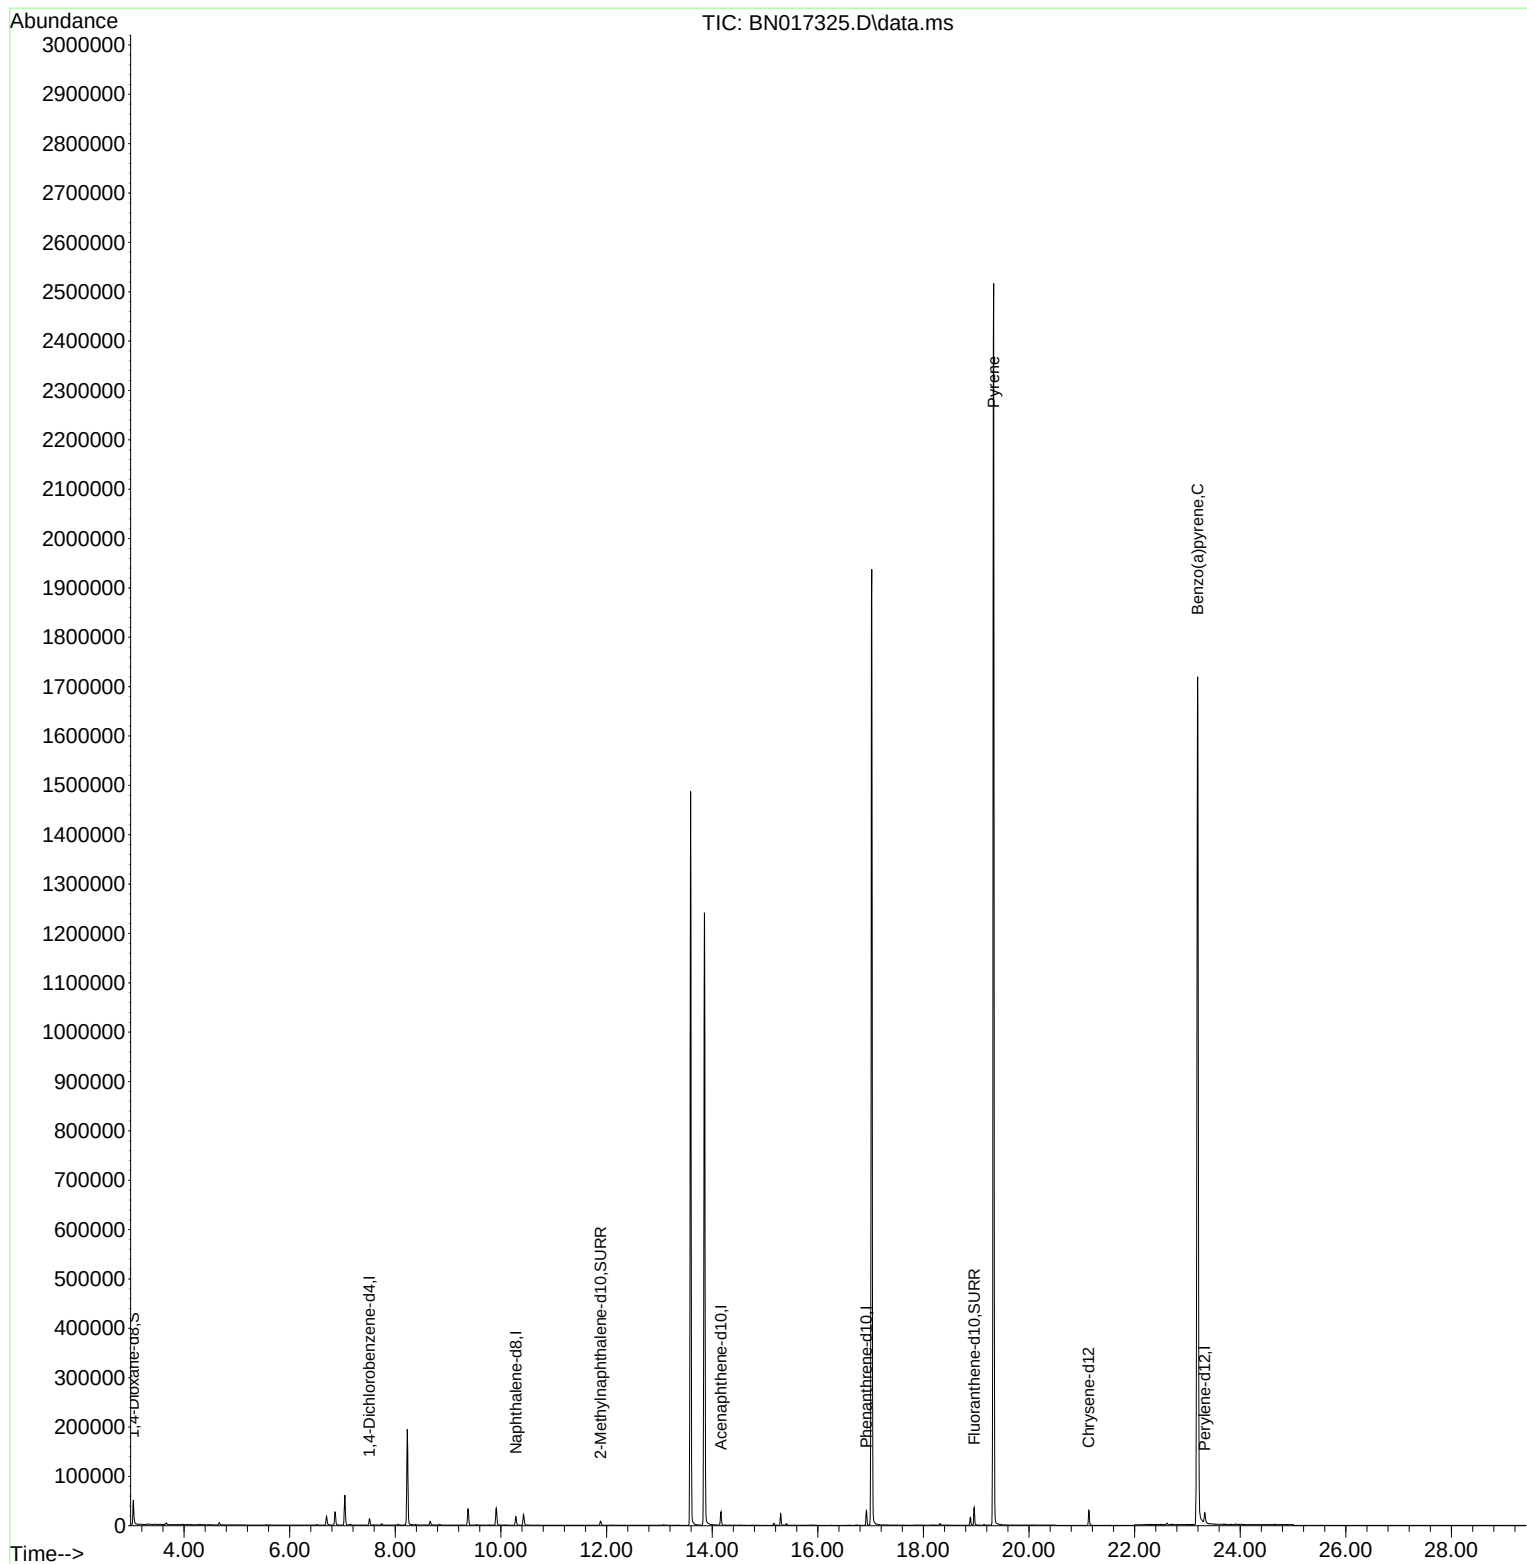


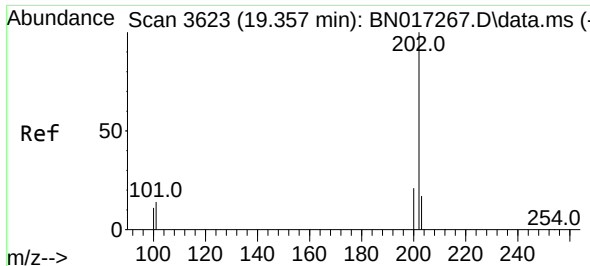

#20
Pyrene
Concen: 0.039 ng/ul
RT: 19.329 min Scan# 30
Delta R.T. -0.027 min
Lab File: BN017325.D
Acq: 04 Nov 2021 22:35

Instrument :
BNA_N
ClientSampleId :
BG366

Tgt Ion:202 Resp: 4081
Ion Ratio Lower Upper
202 100
101 144.1 10.3 15.5#
100 1007.7 8.2 12.2#

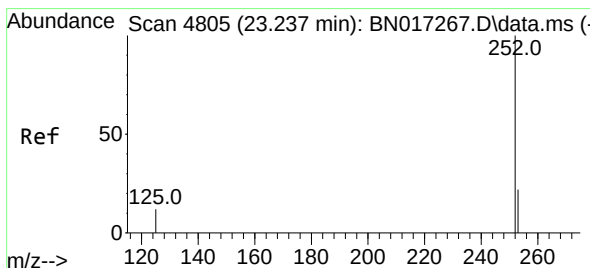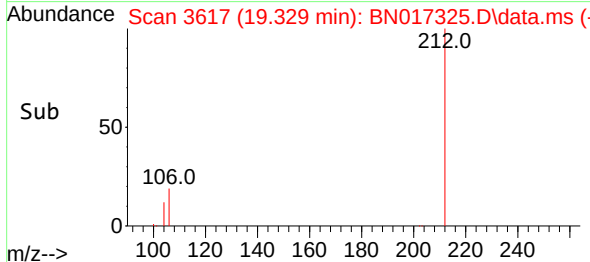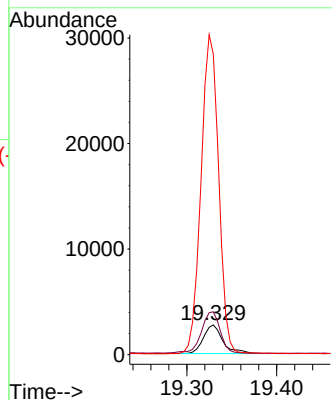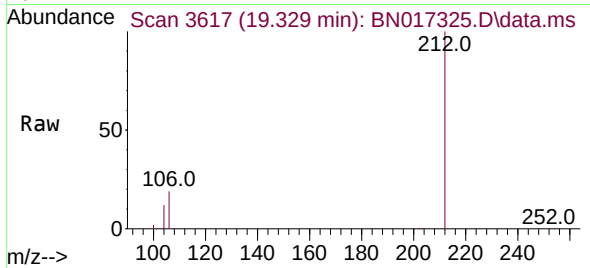

#26
Benzo(a)pyrene
Concen: 0.084 ng/ul
RT: 23.194 min Scan# 4790
Delta R.T. -0.043 min
Lab File: BN017325.D
Acq: 04 Nov 2021 22:35

Tgt Ion:252 Resp: 8167
Ion Ratio Lower Upper
252 100
253 39.1 19.3 28.9#
125 25.8 10.8 16.2#

