

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017272.D
 Acq On : 03 Nov 2021 12:55
 Operator : CG/JU
 Sample : M4364-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG337

Quant Time: Nov 03 13:23:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4308	0.400	ng/ul	0.00
4) Naphthalene-d8	10.283	136	17619	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	11219	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	24773	0.400	ng/ul	0.00
17) Chrysene-d12	21.138	240	23406	0.400	ng/ul	0.00
23) Perylene-d12	23.332	264	24987	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.034	96	21996	4.592	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	8893	0.346	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	27462	0.448	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.964	178	2000	0.025	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017272.D
 Acq On : 03 Nov 2021 12:55
 Operator : CG/JU
 Sample : M4364-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG337


Quant Time: Nov 03 13:23:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

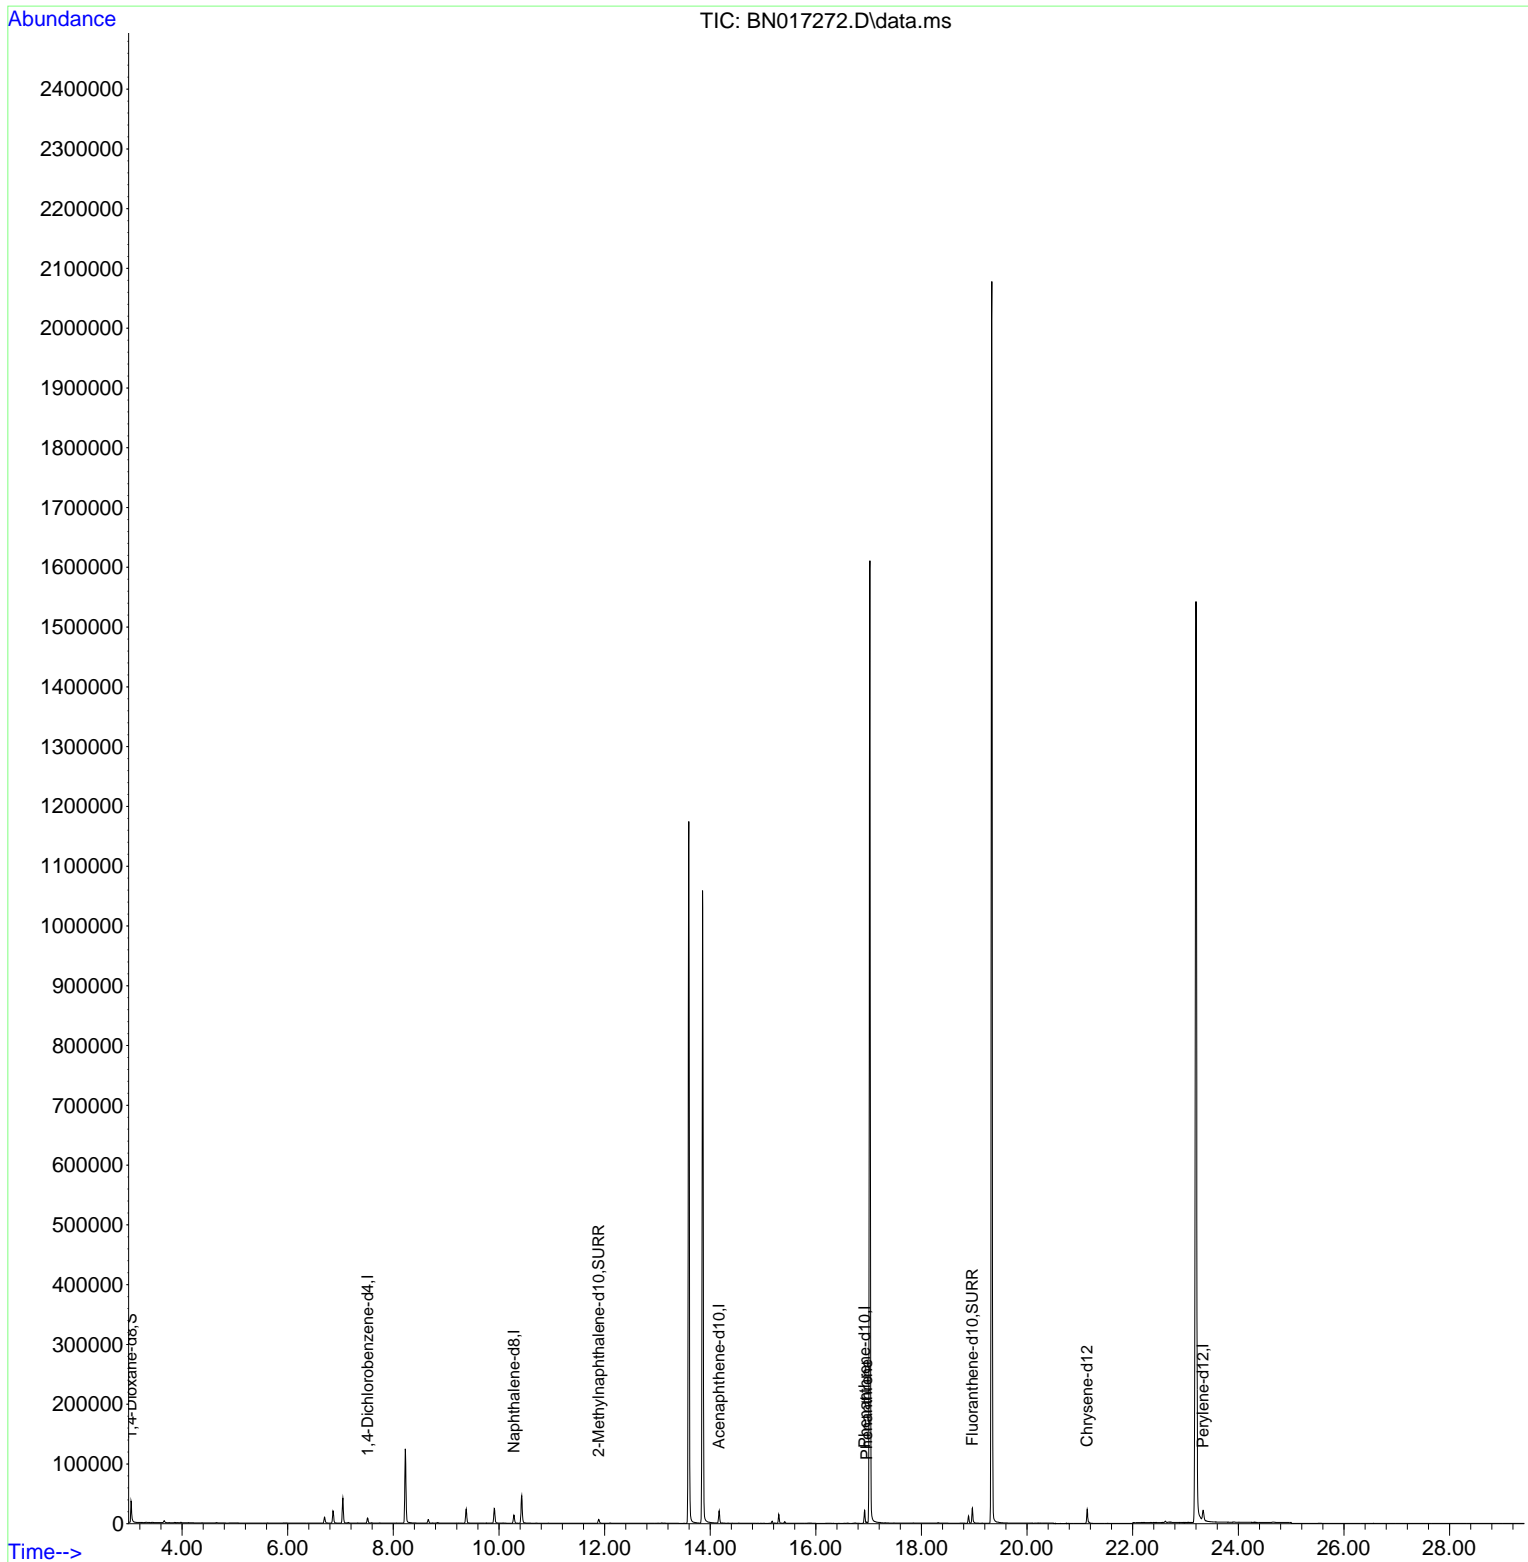

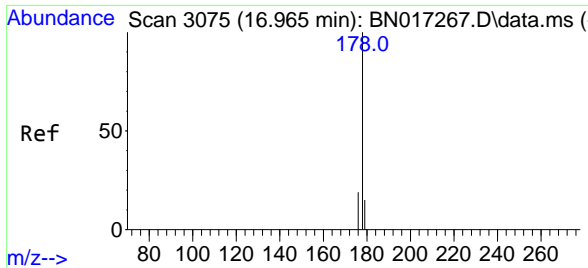

#15
 Phenanthrene
 Concen: 0.025 ng/ul
 RT: 16.964 min Scan# 30
 Delta R.T. -0.001 min
 Lab File: BN017272.D
 Acq: 03 Nov 2021 12:55

Instrument :
 BNA_N
 ClientSampleId :
 BG337

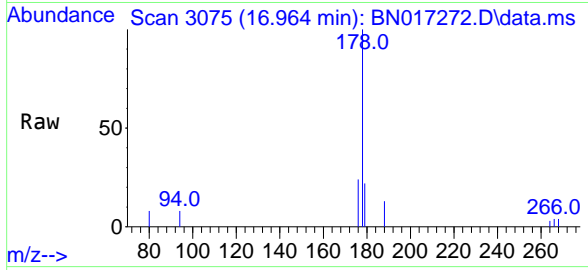

Tgt Ion:178 Resp: 2000

Ion	Ratio	Lower	Upper
178	100		
179	21.9	12.6	19.0#
176	23.9	15.5	23.3#

