

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017274.D
 Acq On : 03 Nov 2021 14:07
 Operator : CG/JU
 Sample : M4364-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG340

Quant Time: Nov 03 14:37:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4359	0.400	ng/ul	0.00
4) Naphthalene-d8	10.288	136	17760	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	11518	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	24882	0.400	ng/ul	0.00
17) Chrysene-d12	21.138	240	23310	0.400	ng/ul	0.00
23) Perylene-d12	23.332	264	25175	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	25132	5.186	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	10194	0.393	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	31791	0.520	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.964	178	4116	0.052	ng/ul	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017274.D
Acq On : 03 Nov 2021 14:07
Operator : CG/JU
Sample : M4364-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG340

Quant Time: Nov 03 14:37:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration

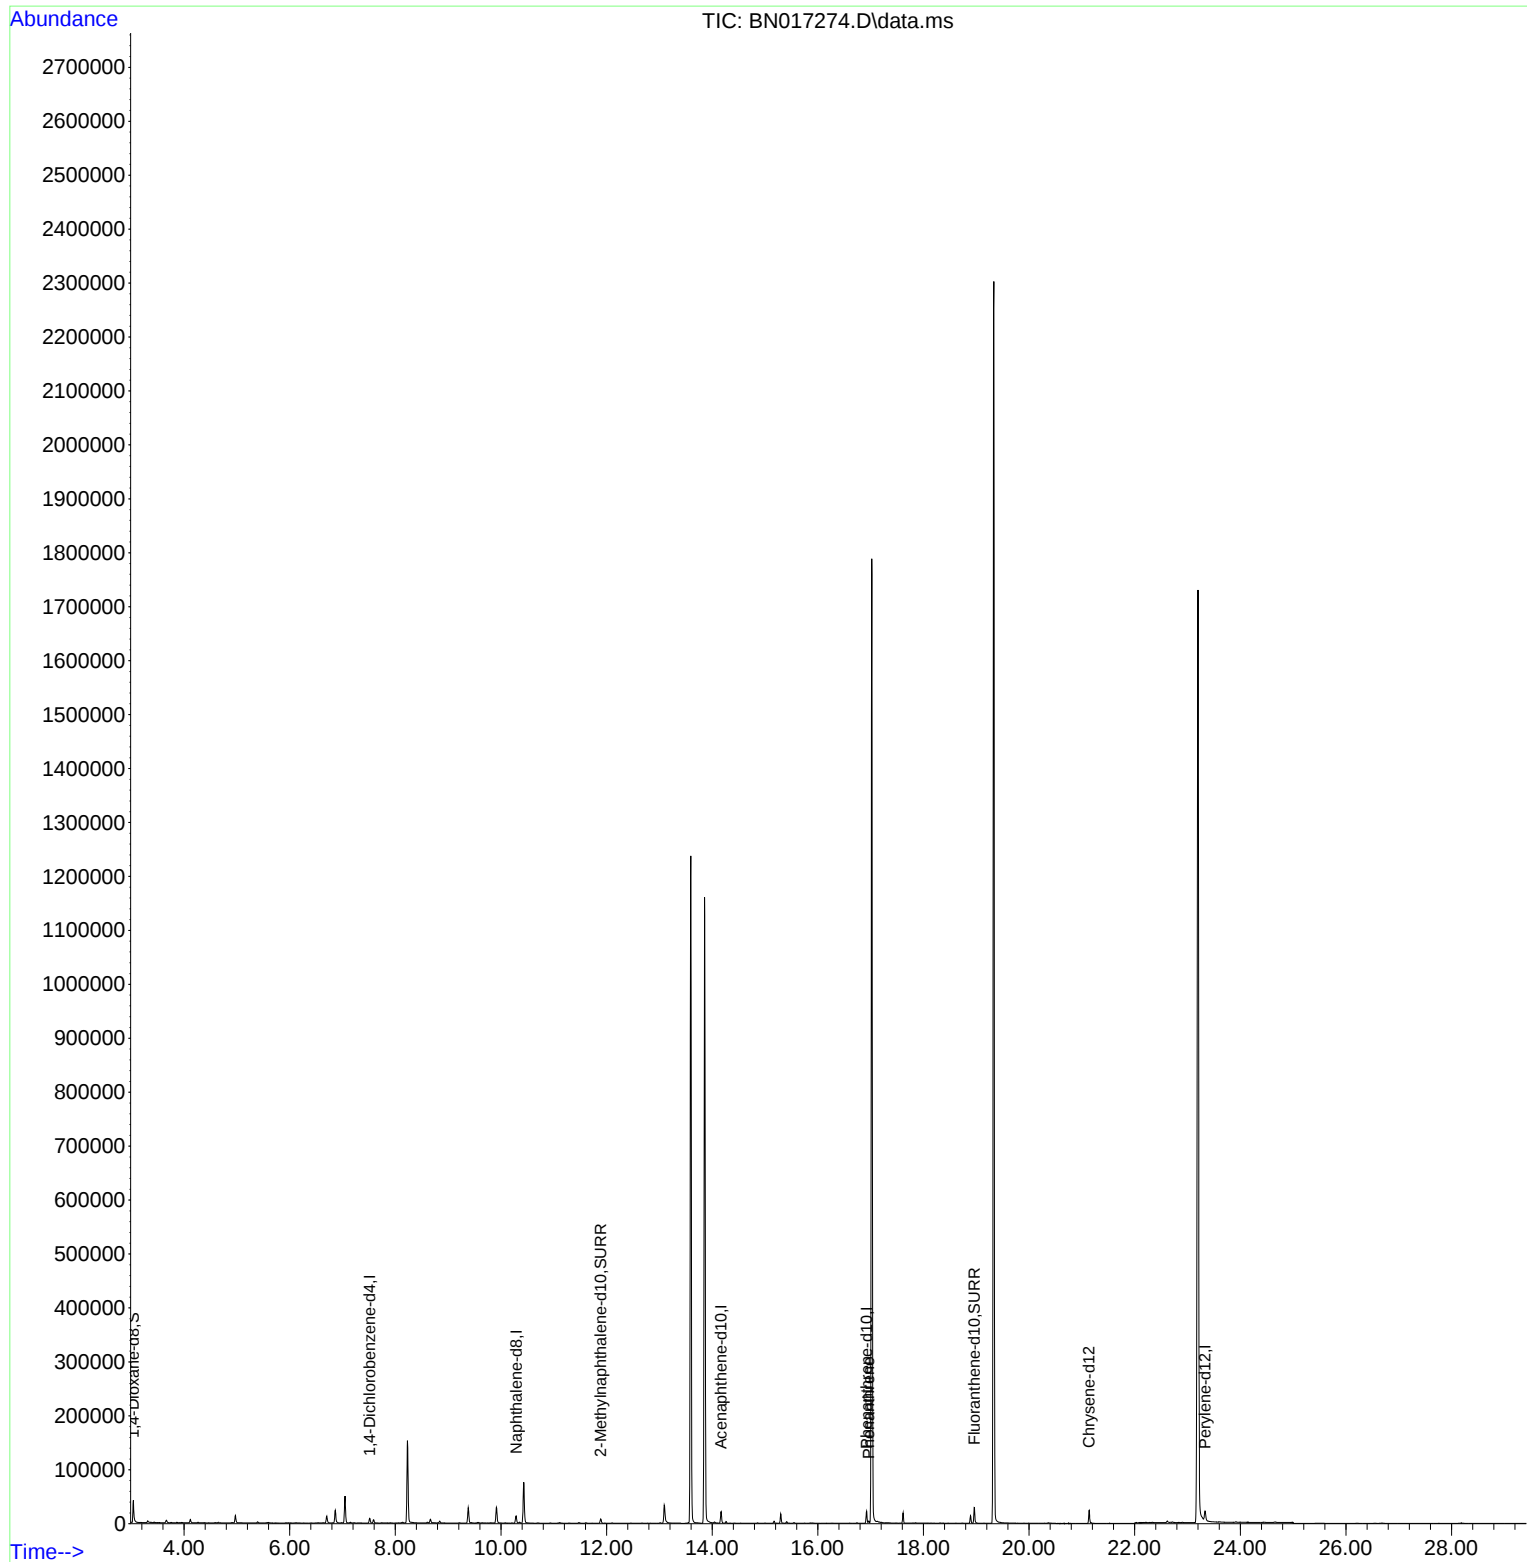

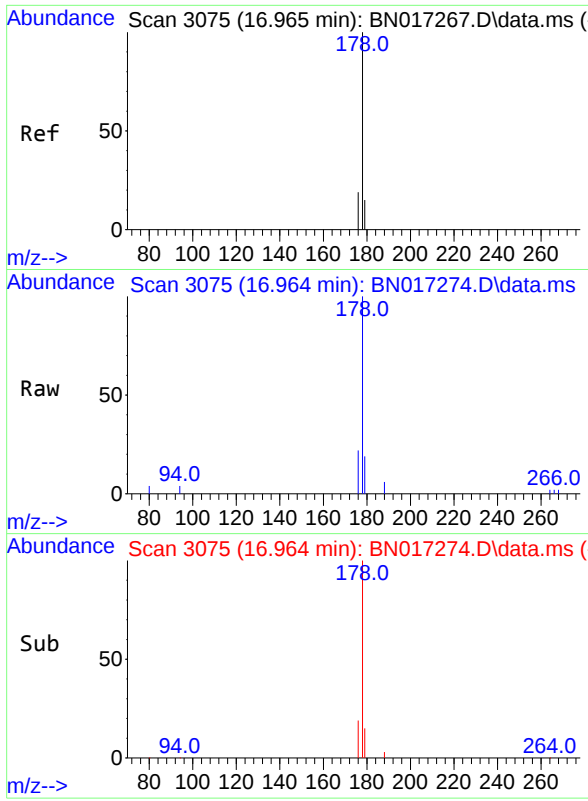

#15
Phenanthrene
Concen: 0.052 ng/ul
RT: 16.964 min Scan# 3075
Delta R.T. -0.001 min
Lab File: BN017274.D
Acq: 03 Nov 2021 14:07

Instrument :
BNA_N
ClientSampleId :
BG340

Tgt Ion:	178	Resp:	4116
Ion	Ratio	Lower	Upper
178	100		
179	18.7	12.6	19.0
176	21.5	15.5	23.3

