

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017279.D
 Acq On : 03 Nov 2021 17:08
 Operator : CG/JU
 Sample : M4374-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG340

Quant Time: Nov 03 17:37:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4600	0.400	ng/ul	0.00
4) Naphthalene-d8	10.288	136	18536	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	12139	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	26503	0.400	ng/ul	0.00
17) Chrysene-d12	21.138	240	25763	0.400	ng/ul	0.00
23) Perylene-d12	23.332	264	29014	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	26604	5.202	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	10736	0.397	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	34610	0.513	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.964	178	4295	0.051	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017279.D
Acq On : 03 Nov 2021 17:08
Operator : CG/JU
Sample : M4374-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG340


Quant Time: Nov 03 17:37:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration

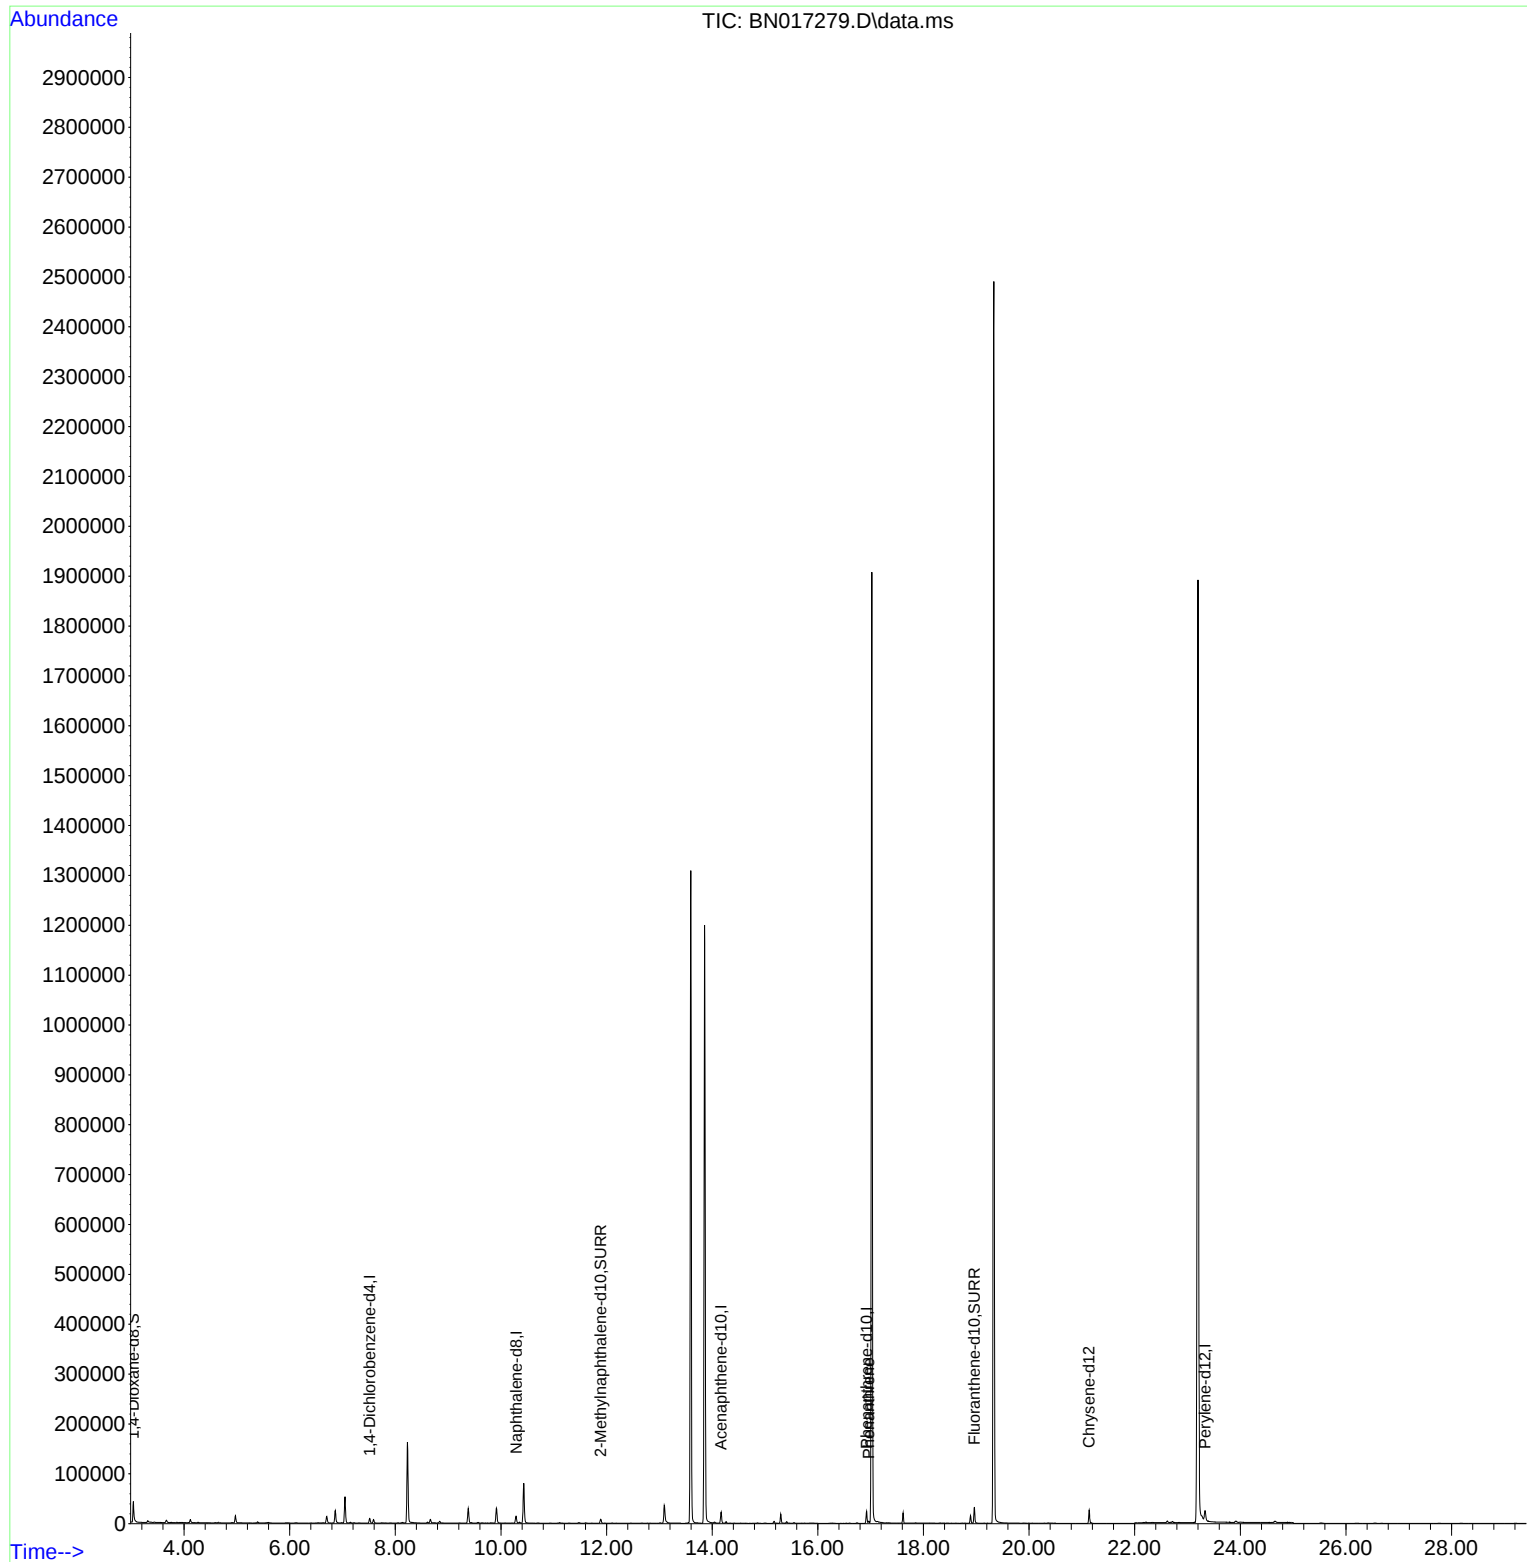

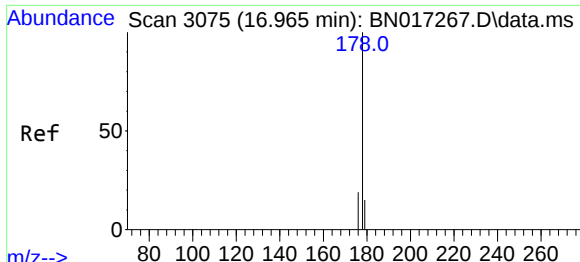

#15
 Phenanthrene
 Concen: 0.051 ng/ul
 RT: 16.964 min Scan# 3075
 Delta R.T. -0.001 min
 Lab File: BN017279.D
 Acq: 03 Nov 2021 17:08

Instrument :
 BNA_N
 ClientSampleId :
 BG340

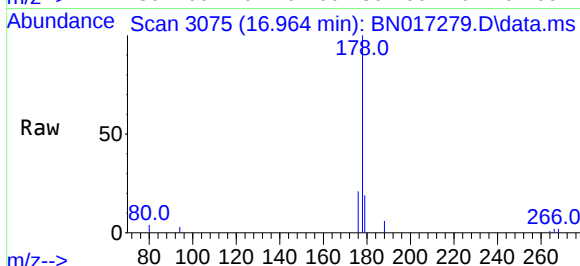

Tgt Ion:178 Resp: 4295

Ion	Ratio	Lower	Upper
178	100		
179	18.5	12.6	19.0
176	20.9	15.5	23.3

