

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
 Data File : BN017287.D
 Acq On : 03 Nov 2021 22:33
 Operator : CG/JU
 Sample : M4364-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG320

Quant Time: Nov 08 01:06:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 03 10:42:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.514	152	4855	0.400	ng/ul	0.00
4) Naphthalene-d8	10.282	136	19847	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.169	164	12370	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.922	188	27252	0.400	ng/ul	0.00
17) Chrysene-d12	21.138	240	23999	0.400	ng/ul	0.00
23) Perylene-d12	23.329	264	27646	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.038	96	21169	3.922	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.888	152	9444	0.326	ng/ul	0.00
18) Fluoranthene-d10	18.965	212	28230	0.449	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.964	178	1860	0.022	ng/ul#	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110321\
Data File : BN017287.D
Acq On : 03 Nov 2021 22:33
Operator : CG/JU
Sample : M4364-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG320


Quant Time: Nov 08 01:06:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 03 10:42:03 2021
Response via : Initial Calibration

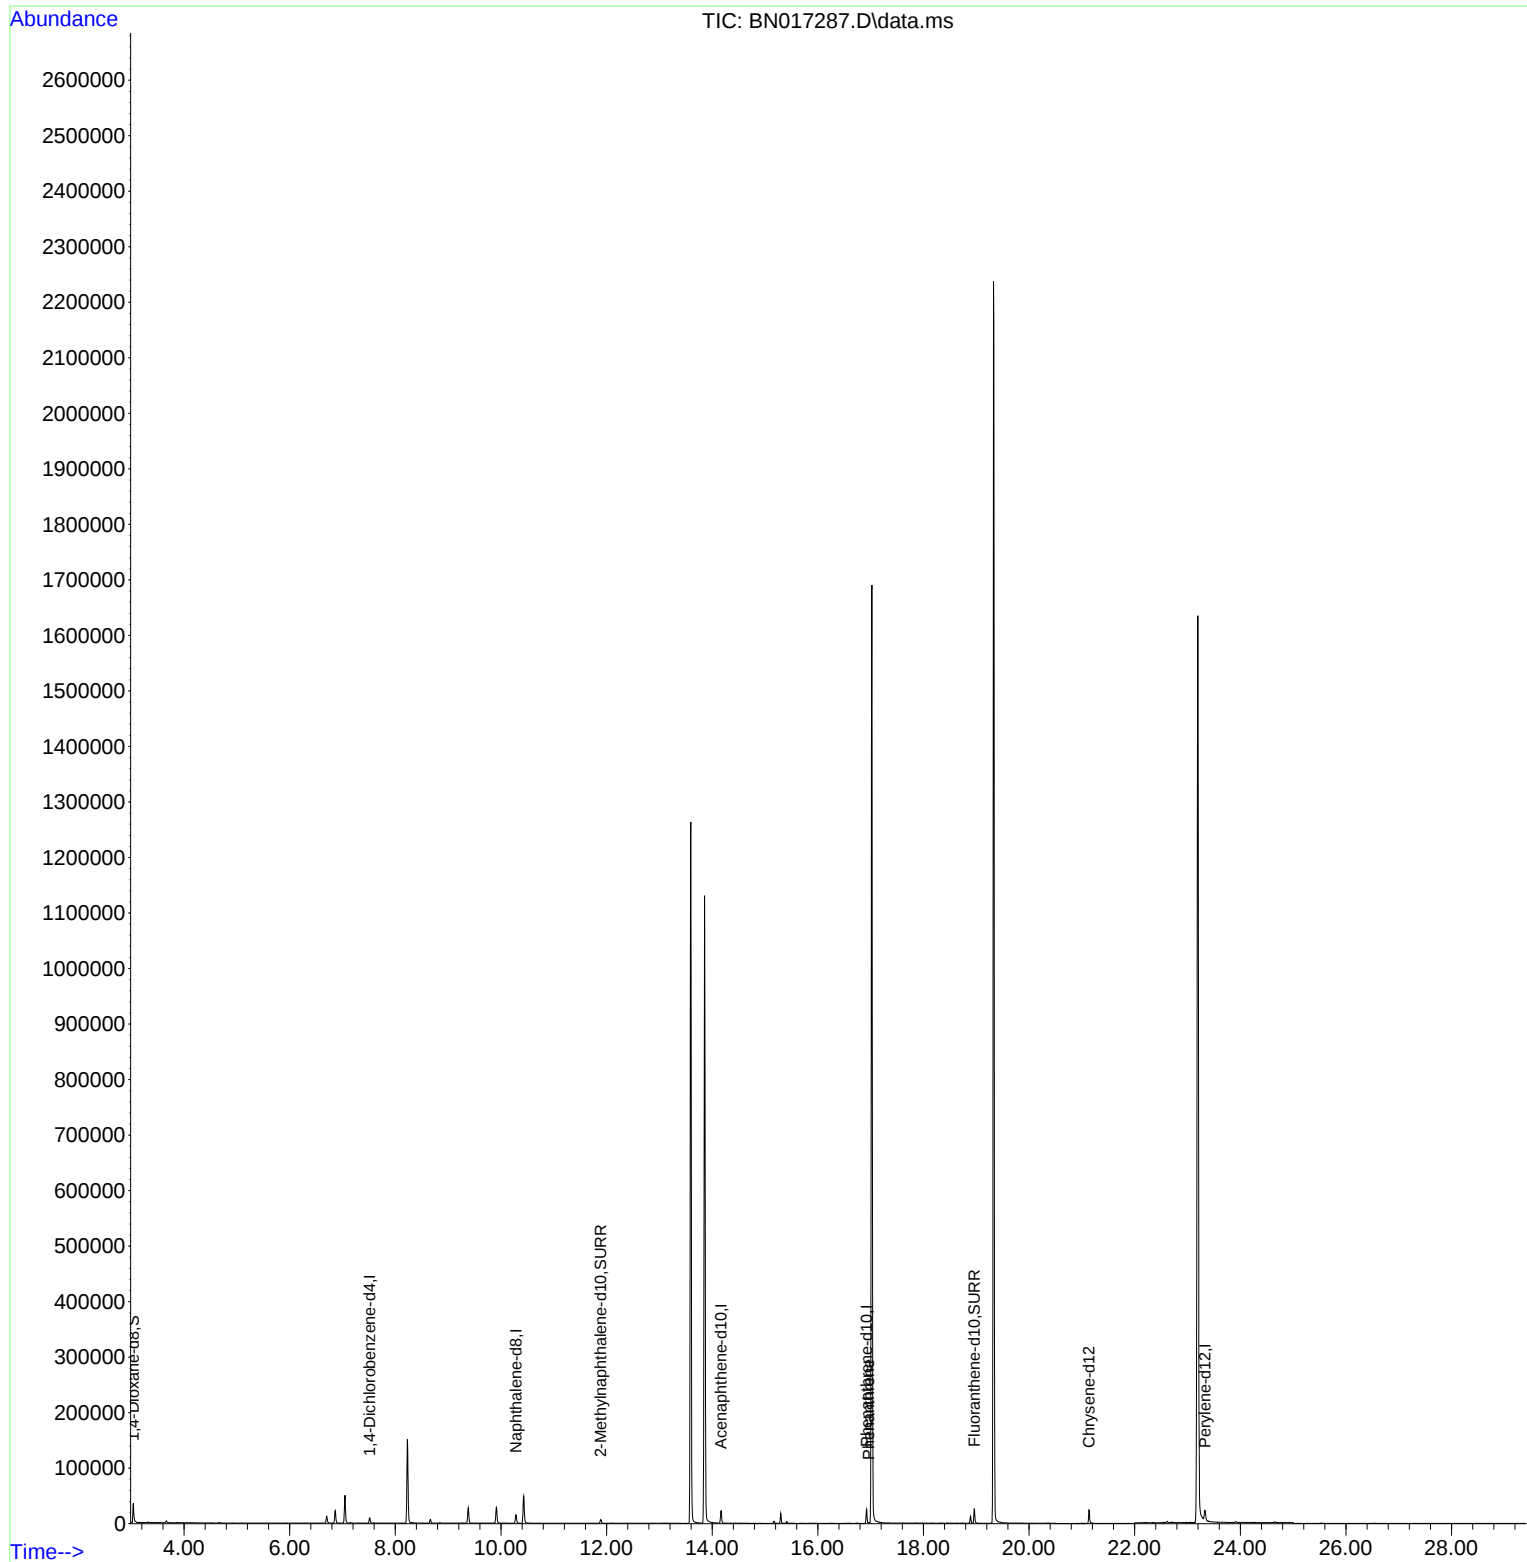

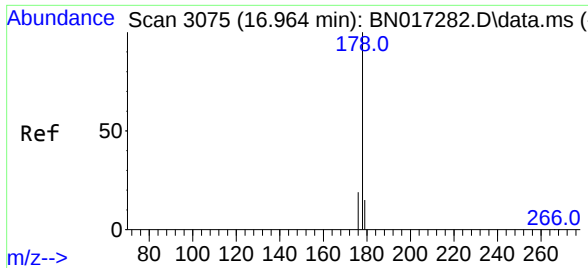

#15
 Phenanthrene
 Concen: 0.022 ng/ul
 RT: 16.964 min Scan# 3075
 Delta R.T. -0.001 min
 Lab File: BN017287.D
 Acq: 03 Nov 2021 22:33

Instrument :
 BNA_N
 ClientSampleId :
 BG320

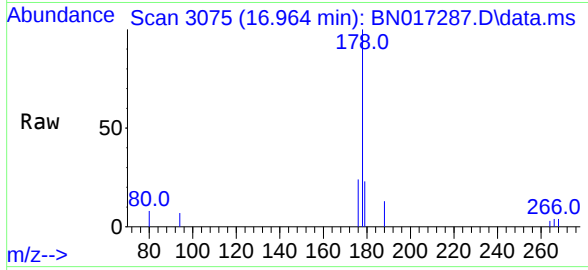

Tgt Ion:178 Resp: 1860

Ion	Ratio	Lower	Upper
178	100		
179	23.0	12.6	19.0#
176	23.6	15.5	23.3#

