
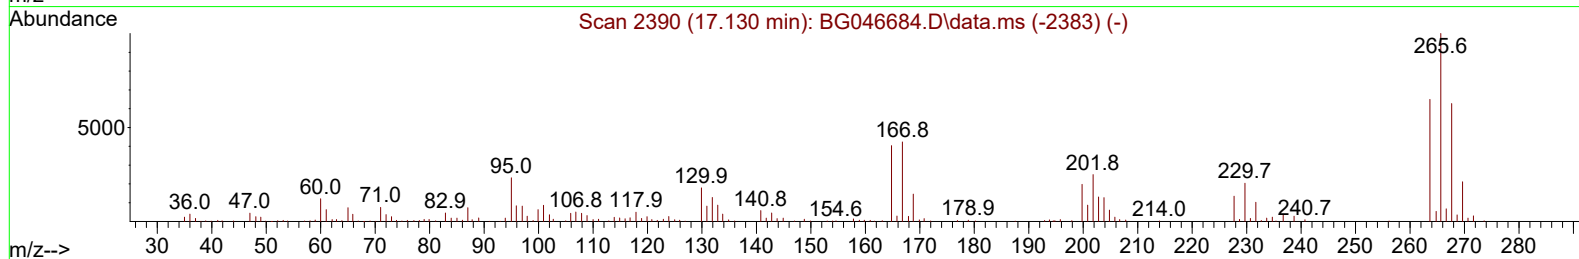
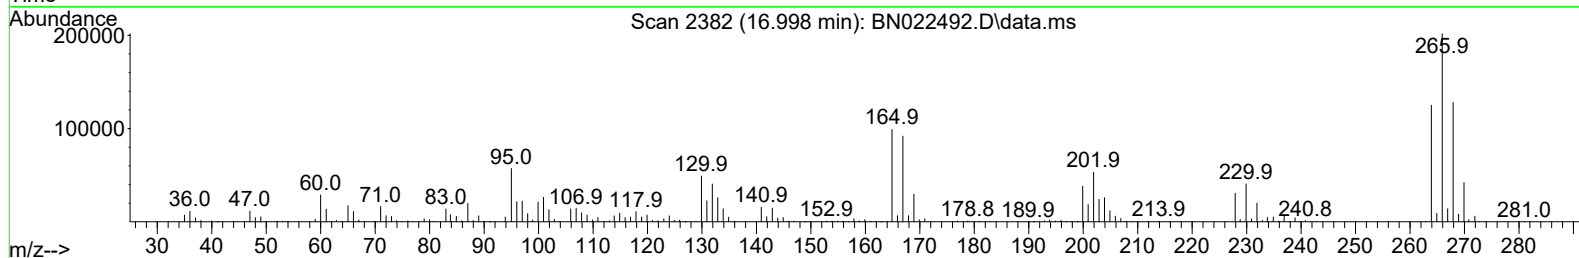


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
Data File : BN022492.D
Acq On : 04 Nov 2022 00:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 07:53:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 07:51:43 2022
Response via : Initial Calibration

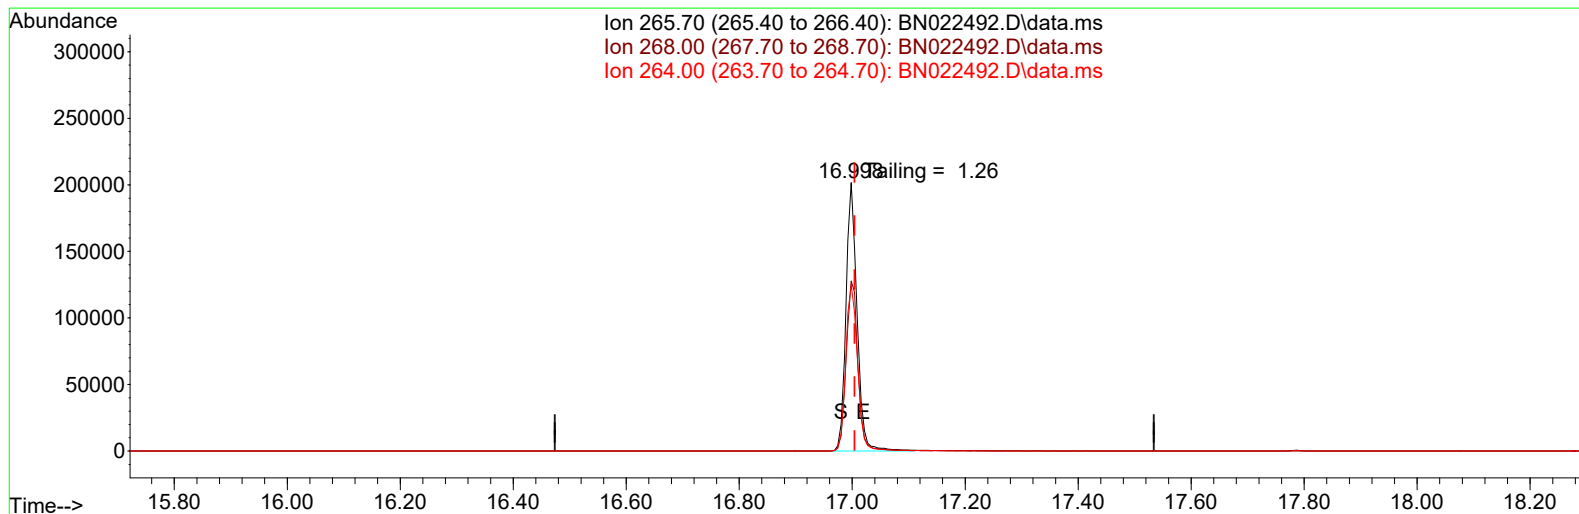

TIC: BN022492.D\data.ms

(70) Pentachlorophenol (C)




16.998min (-0.006) 20713.55 ng

response 276343

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.41
264.00	61.60	62.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
Data File : BN022492.D
Acq On : 04 Nov 2022 00:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 07:53:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 07:51:43 2022
Response via : Initial Calibration

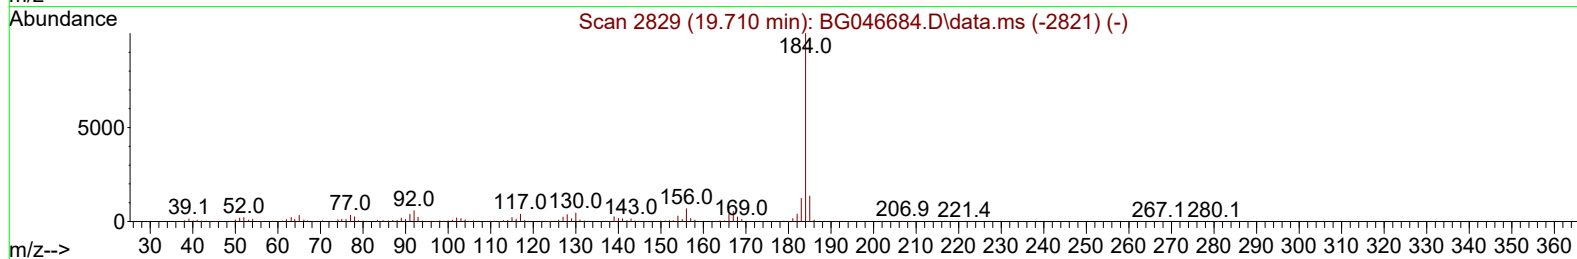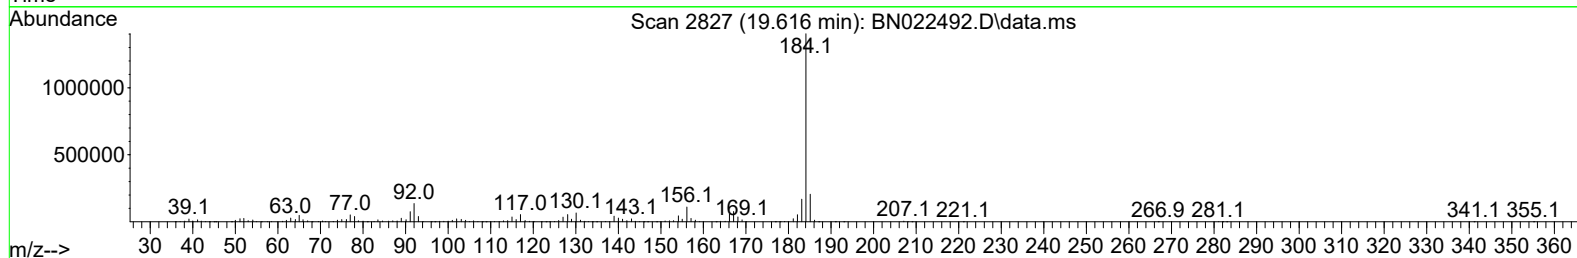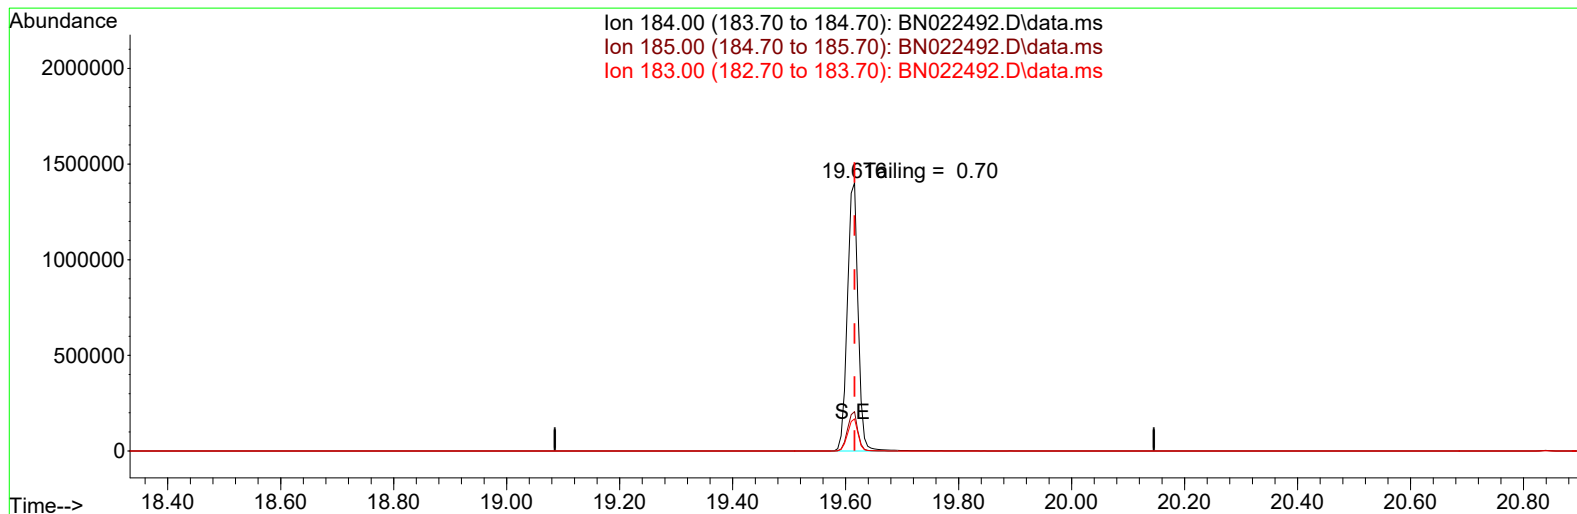

TIC: BN022492.D\data.ms

(77) Benzidine**19.616min (-0.000) 411984.31 ng****response 1828738**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	12.02
0.00	0.00	0.00