


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
 Data File : BN022474.D
 Acq On : 03 Nov 2022 12:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 04 03:28:17 2022

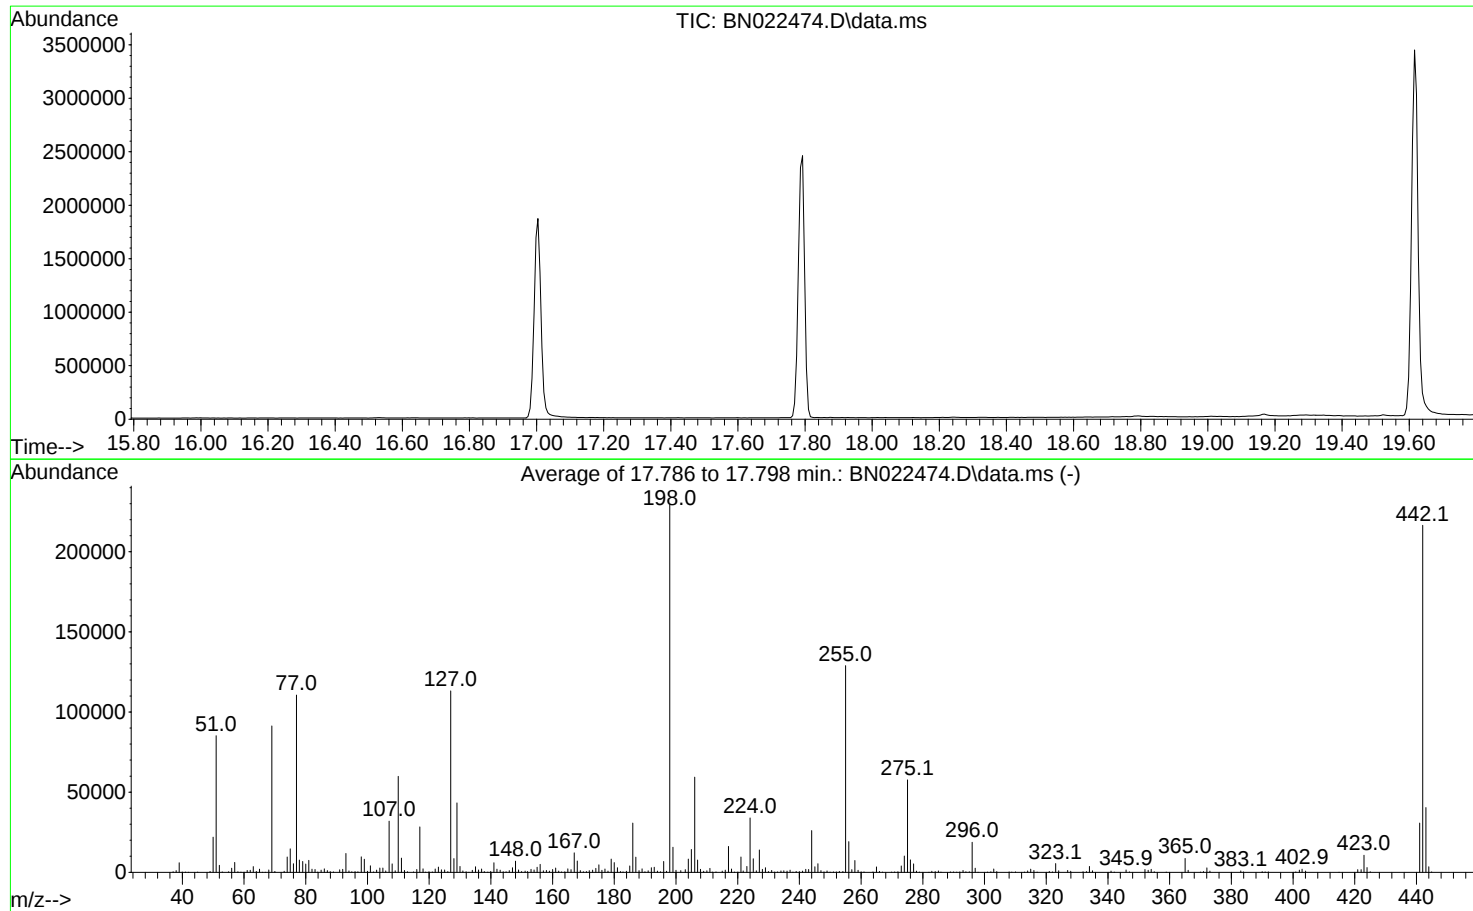




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	85241	PASS
68	69	0.00	2	1.6	1494	PASS
69	198	0.00	100	39.8	91274	PASS
70	69	0.00	2	0.6	521	PASS
127	198	10	80	49.3	113147	PASS
197	198	0.00	2	0.3	687	PASS
198	198	100	100	100.0	229525	PASS
199	198	5	9	6.8	15626	PASS
275	198	10	60	25.1	57640	PASS
365	198	1	100	3.8	8693	PASS
441	198	0.01	100	13.4	30731	PASS
442	442	50	100	100.0	216469	PASS
443	442	15	24	18.7	40403	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
 Data File : BN022474.D
 Acq On : 03 Nov 2022 12:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 04 07:51:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 04 07:51:43 2022
 Response via : Initial Calibration

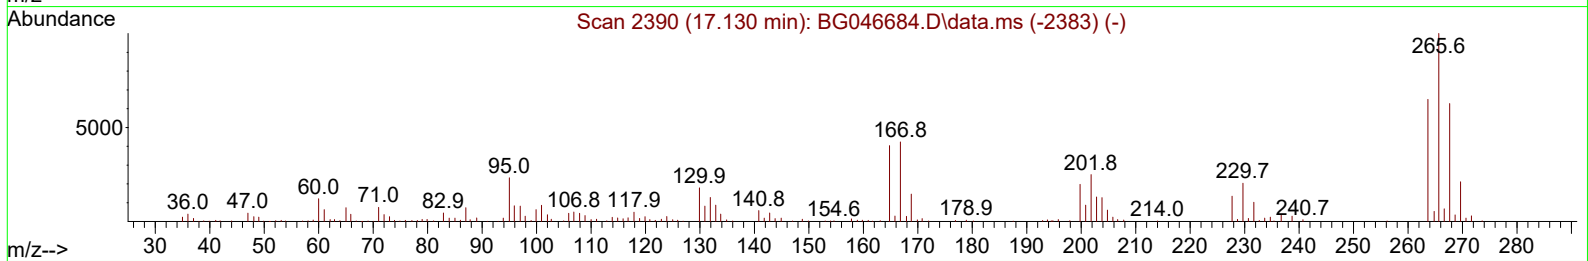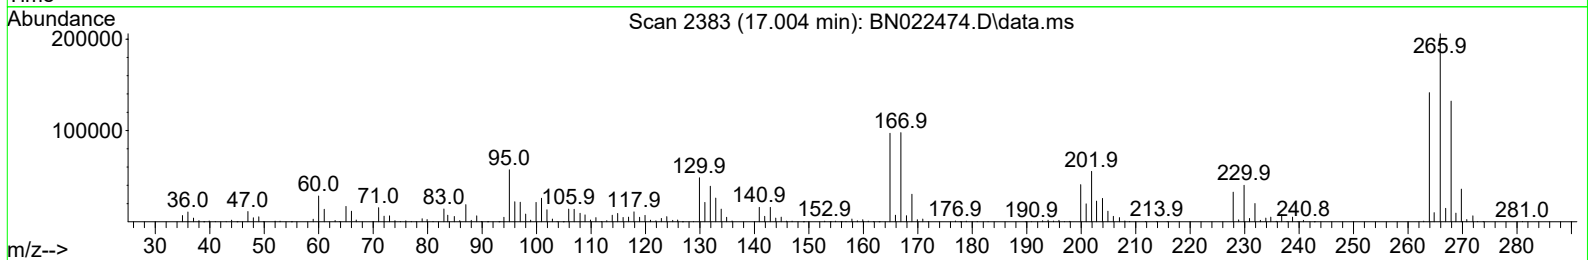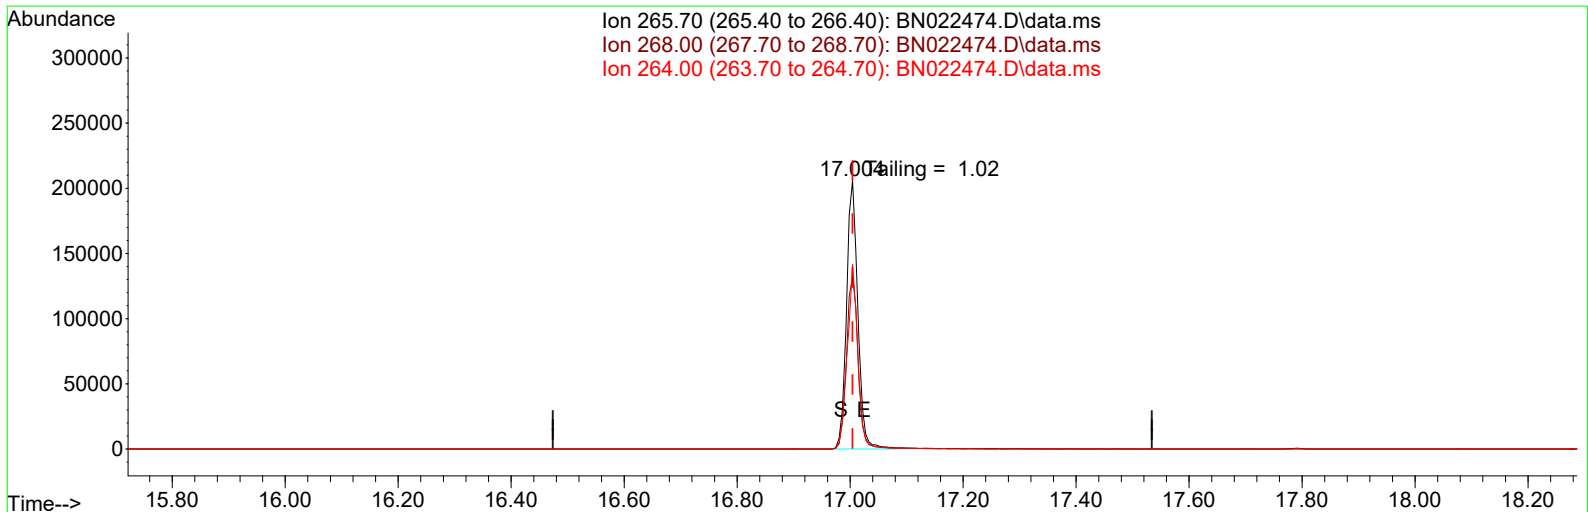

TIC: BN022474.D\data.ms

(70) Pentachlorophenol (C)

17.004min (0.000) 23082.26 ng




response 288562

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.16
264.00	61.60	68.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
Data File : BN022474.D
Acq On : 03 Nov 2022 12:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 07:51:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 07:51:43 2022
Response via : Initial Calibration

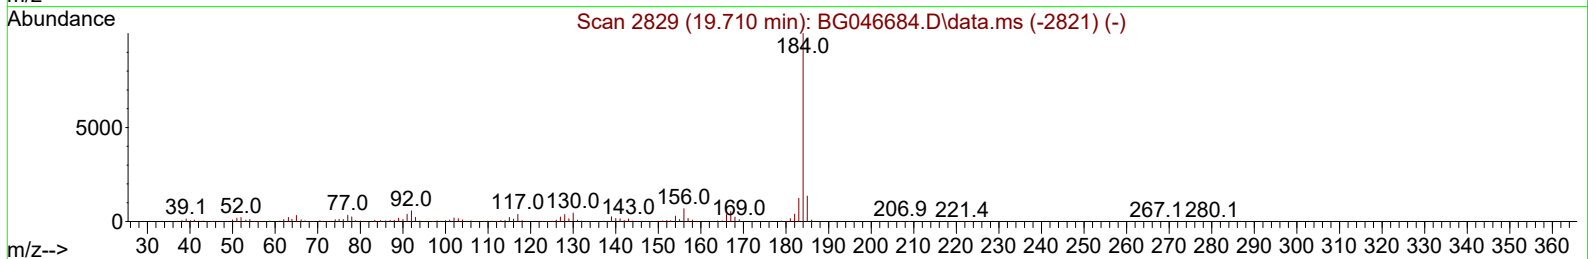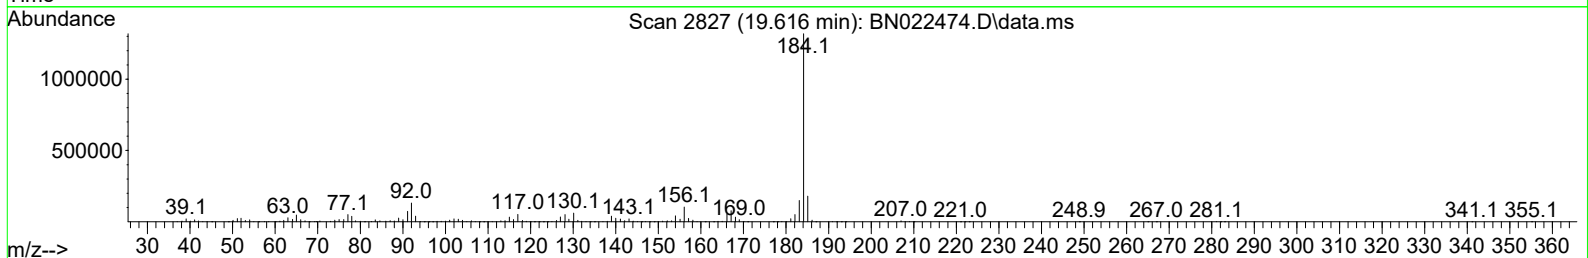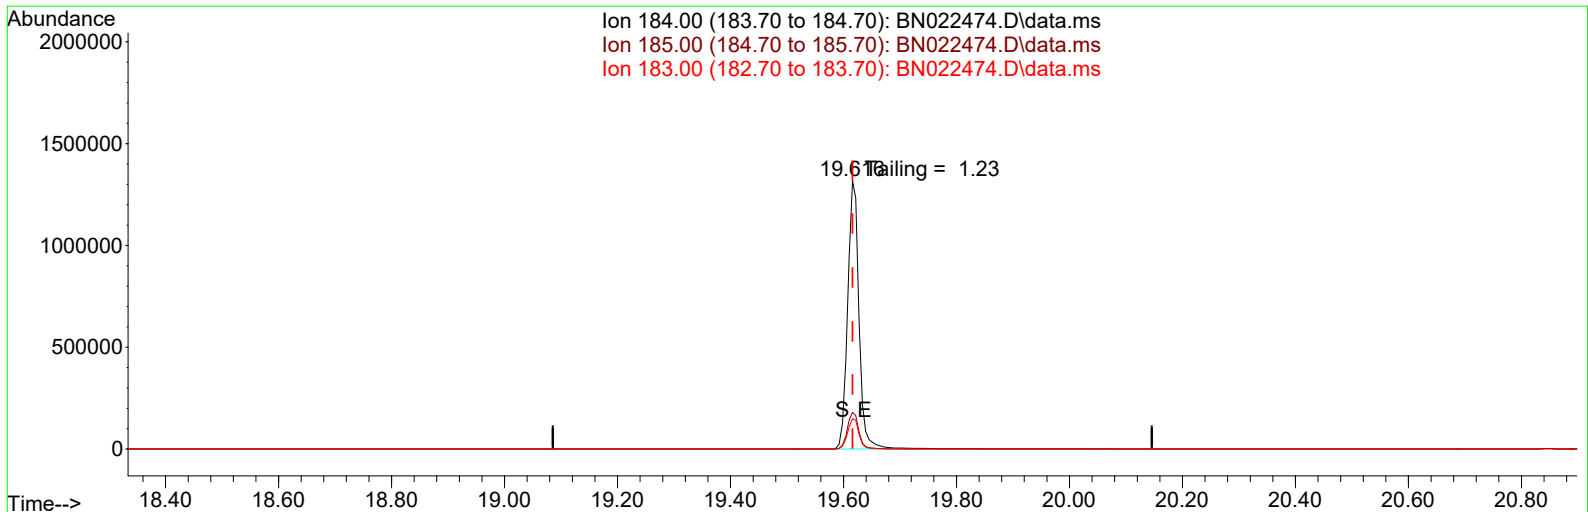

TIC: BN022474.D\data.ms

(77) Benzidine

19.616min (0.000) 336622.06 ng

response 1805511

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.67
183.00	13.20	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2022	BNA_N	<u>BN022474.D</u>
Compound Name	Response	Retention Time
DDT	762934	20.851
DDD	18489	20.404
DDE	166	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18655	781589	2.39

Instrument :
BNA_N
ClientSampleId :
DFTPP