


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
 Data File : BN022492.D
 Acq On : 04 Nov 2022 00:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN110322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 04 03:28:17 2022

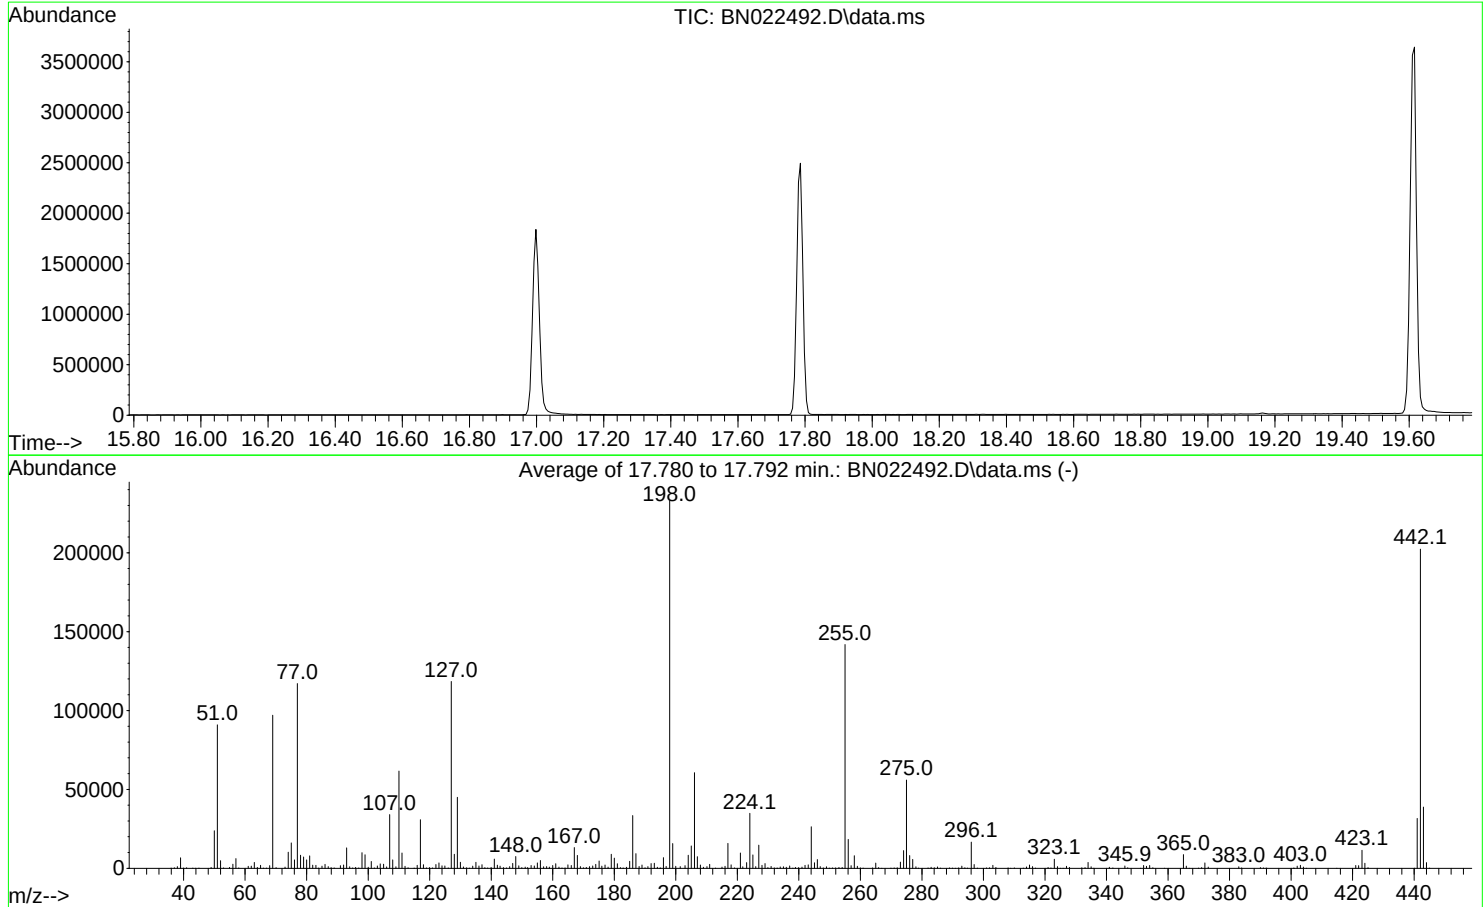




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	90896	PASS
68	69	0.00	2	1.7	1690	PASS
69	198	0.00	100	41.6	97029	PASS
70	69	0.00	2	0.5	511	PASS
127	198	10	80	50.8	118461	PASS
197	198	0.00	2	0.5	1127	PASS
198	198	100	100	100.0	233173	PASS
199	198	5	9	6.7	15642	PASS
275	198	10	60	24.0	55968	PASS
365	198	1	100	3.7	8716	PASS
441	198	0.01	100	13.5	31560	PASS
442	442	50	100	100.0	202261	PASS
443	442	15	24	19.2	38776	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
Data File : BN022492.D
Acq On : 04 Nov 2022 00:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 07:53:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 07:51:43 2022
Response via : Initial Calibration

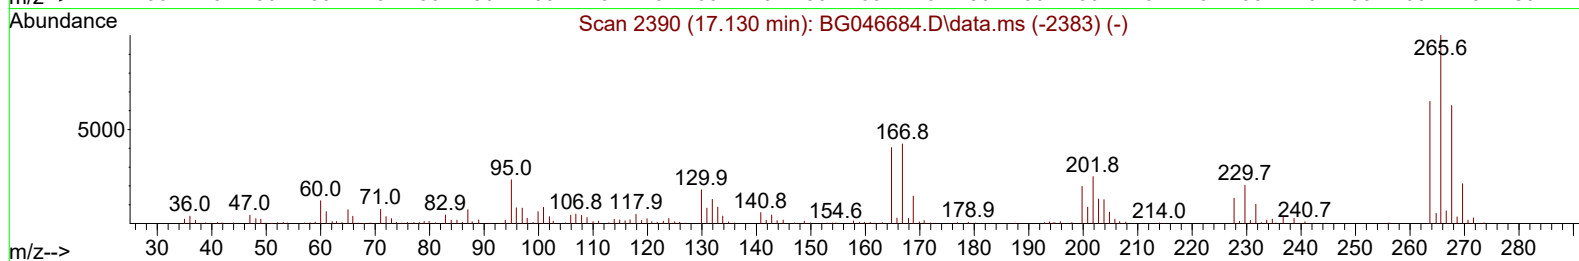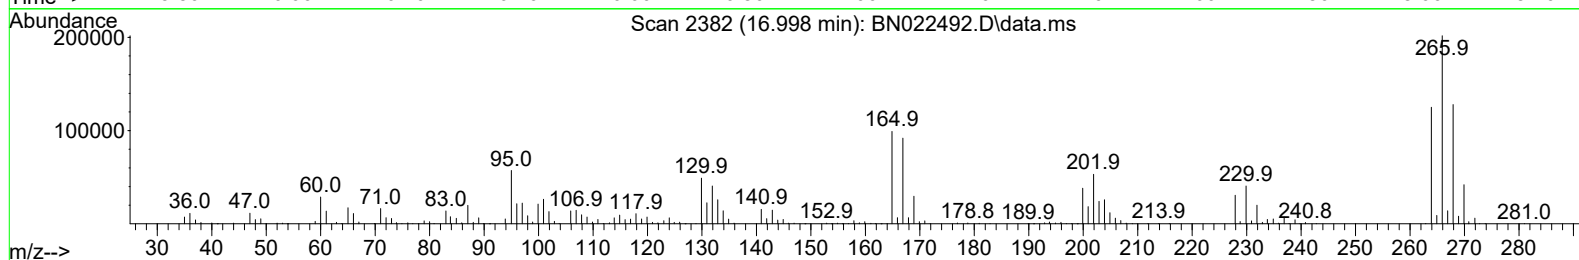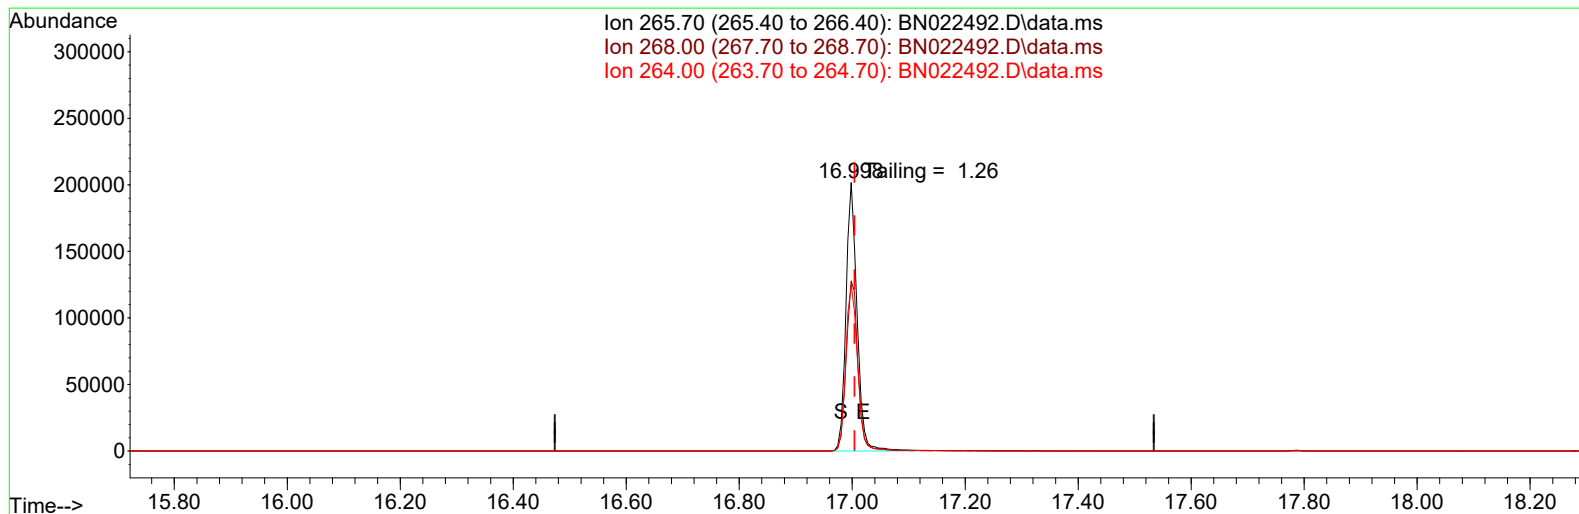

TIC: BN022492.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.006) 20713.55 ng




response 276343

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.41
264.00	61.60	62.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110322\
Data File : BN022492.D
Acq On : 04 Nov 2022 00:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 04 07:53:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 04 07:51:43 2022
Response via : Initial Calibration

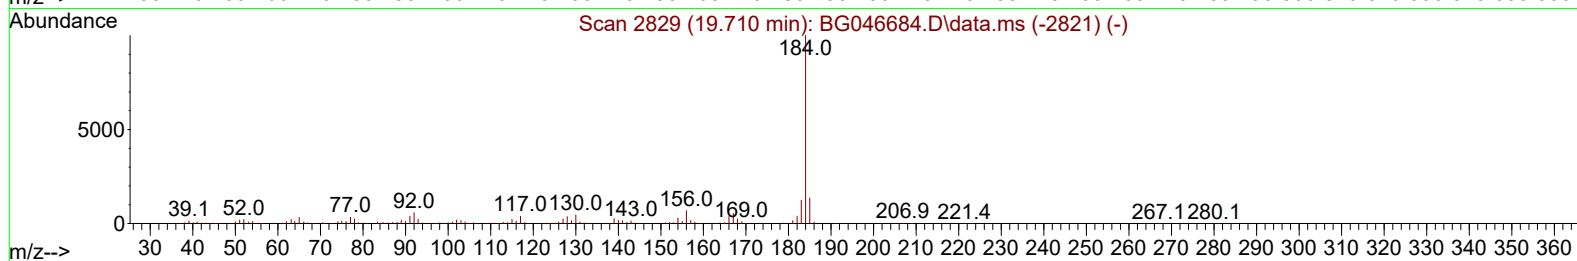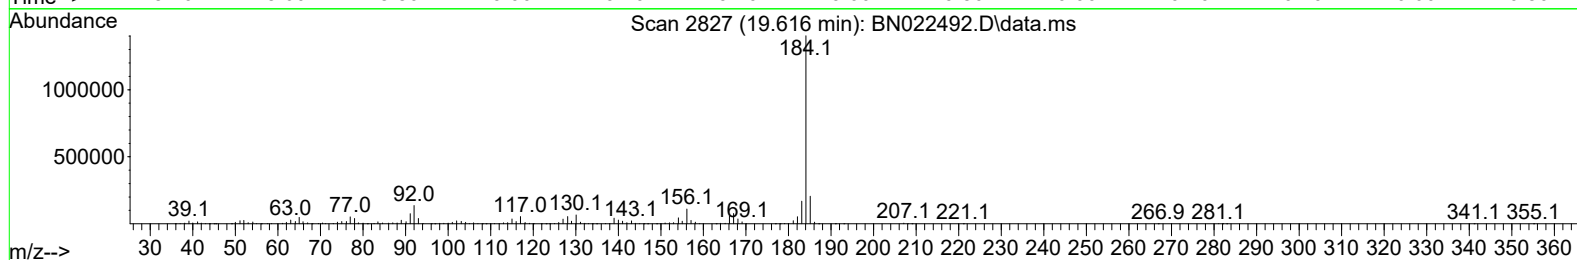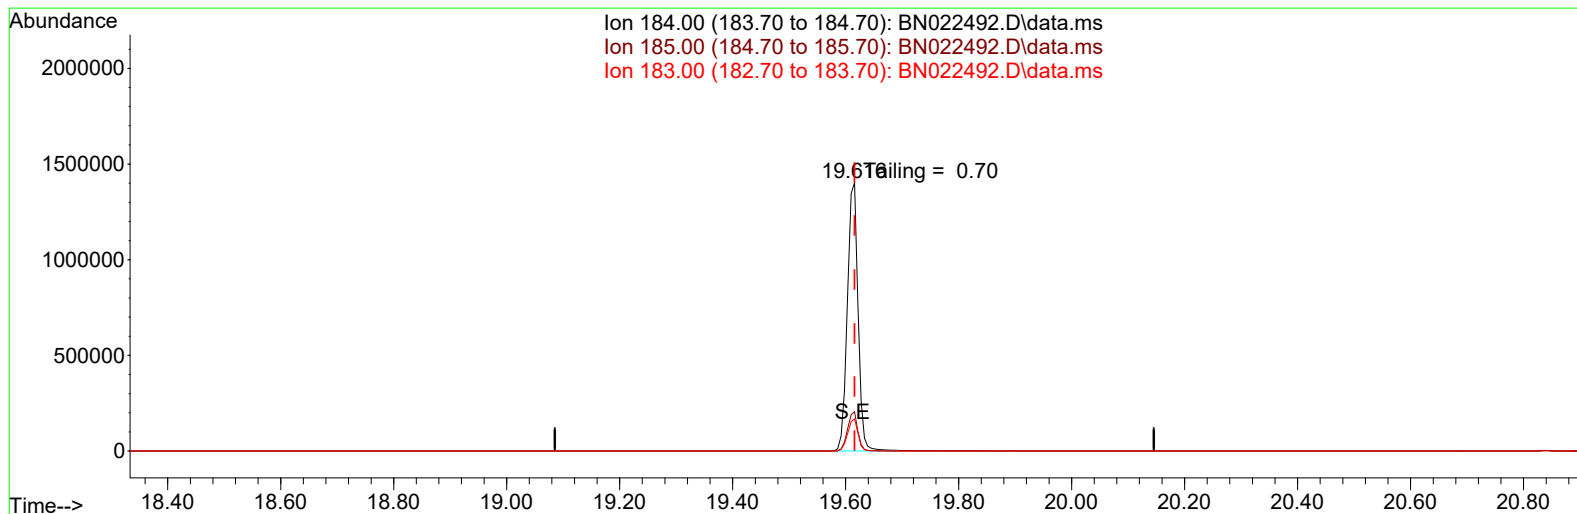

TIC: BN022492.D\data.ms

(77) Benzidine

19.616min (-0.000) 411984.31 ng

response 1828738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2022	BNA_N	<u>BN022492.D</u>
Compound Name	Response	Retention Time
DDT	809217	20.839
DDD	18712	20.398
DDE	163	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18875	828092	2.28

Instrument :
BNA_N
ClientSampleId :
DFTPP