
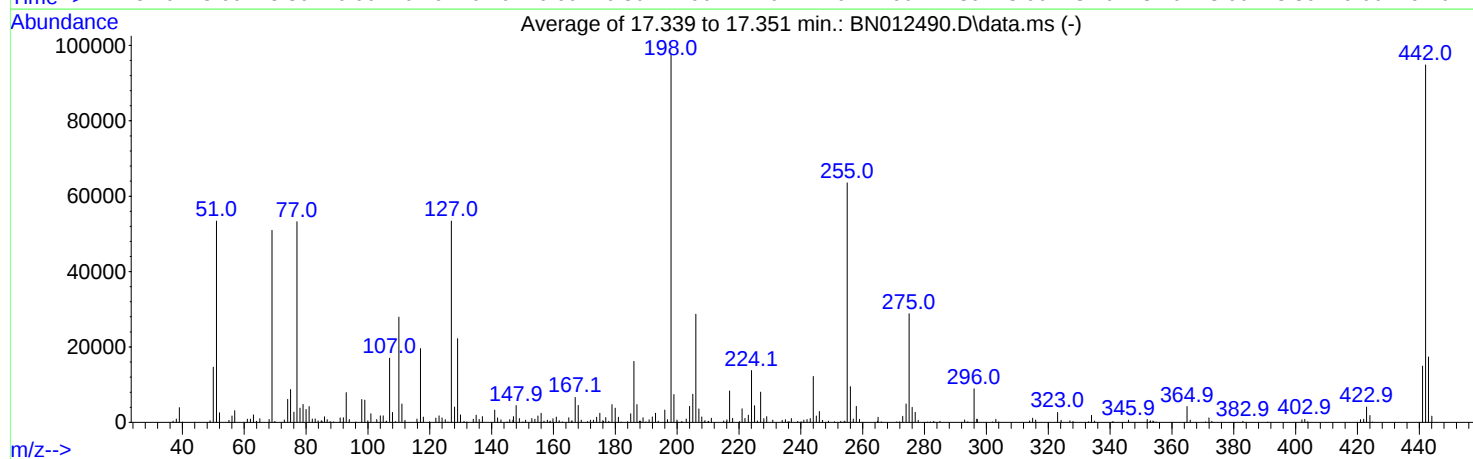


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110420\
 Data File : BN012490.D
 Acq On : 04 Nov 2020 13:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 05 05:46:47 2020

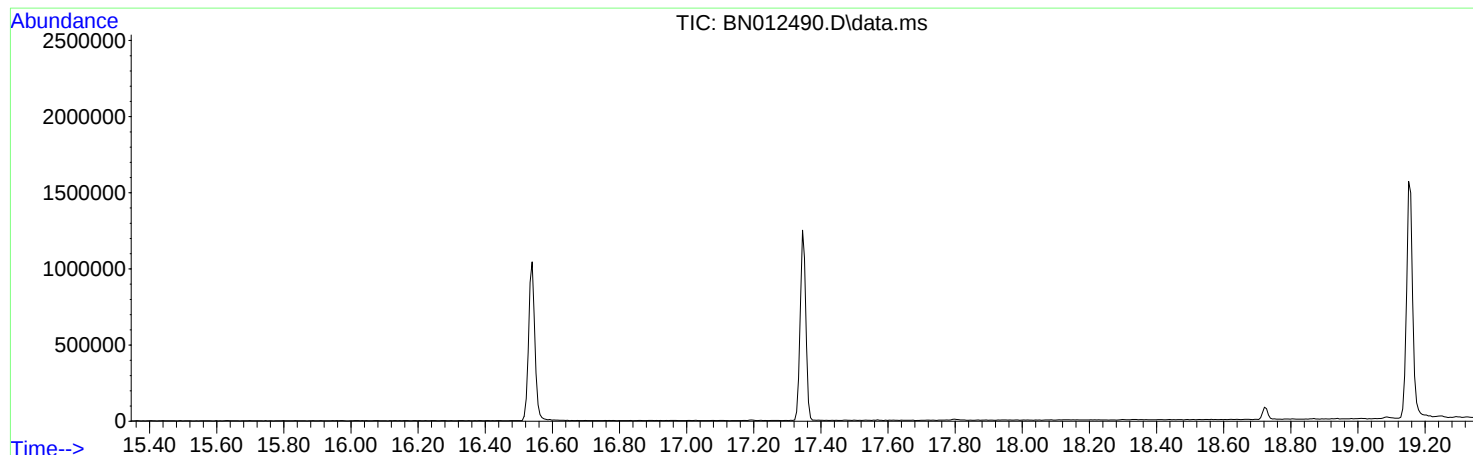

AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2434

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	53416	PASS
68	69	0.00	2	1.5	752	PASS
69	198	0.00	100	52.2	50947	PASS
70	69	0.00	2	0.5	275	PASS
127	198	10	80	54.7	53408	PASS
197	198	0.00	2	0.7	715	PASS
198	198	100	100	100.0	97592	PASS
199	198	5	9	7.6	7377	PASS
275	198	10	60	29.5	28837	PASS
365	198	1	100	4.3	4220	PASS
441	198	0.01	100	15.3	14932	PASS
442	198	50	100	97.2	94845	PASS
443	442	15	24	18.3	17352	PASS