
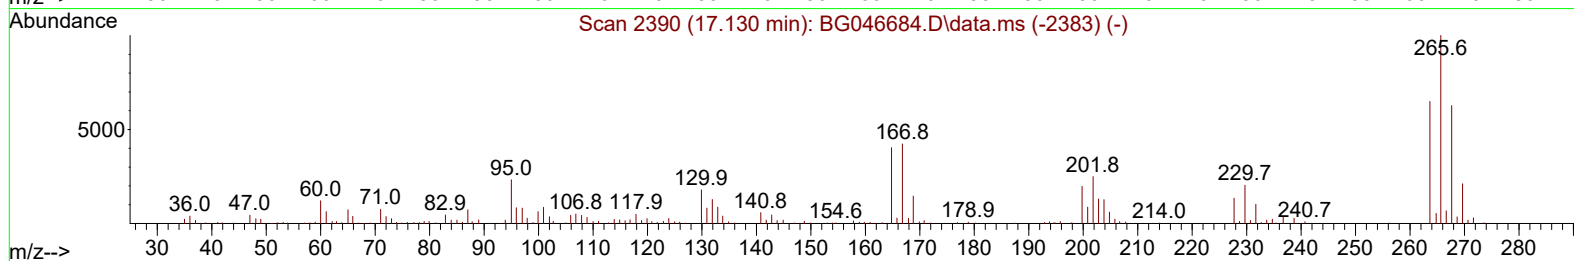
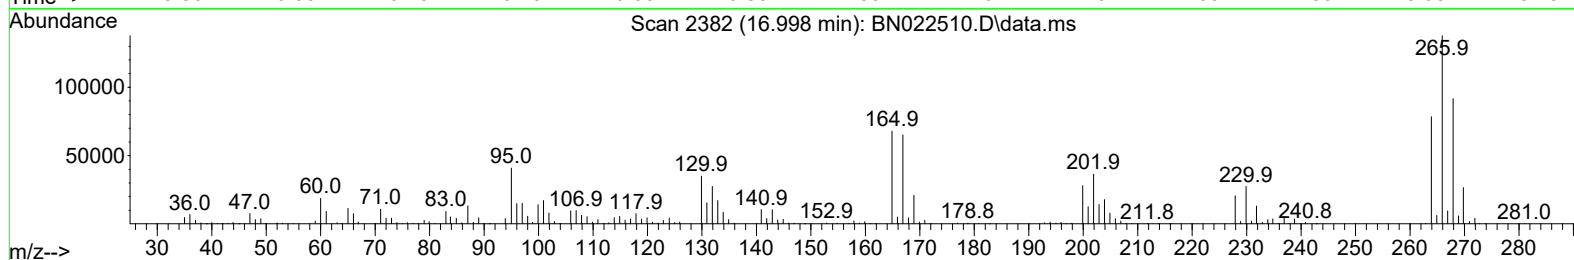


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110422\
Data File : BN022510.D
Acq On : 04 Nov 2022 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 04:35:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 05 04:35:21 2022
Response via : Initial Calibration

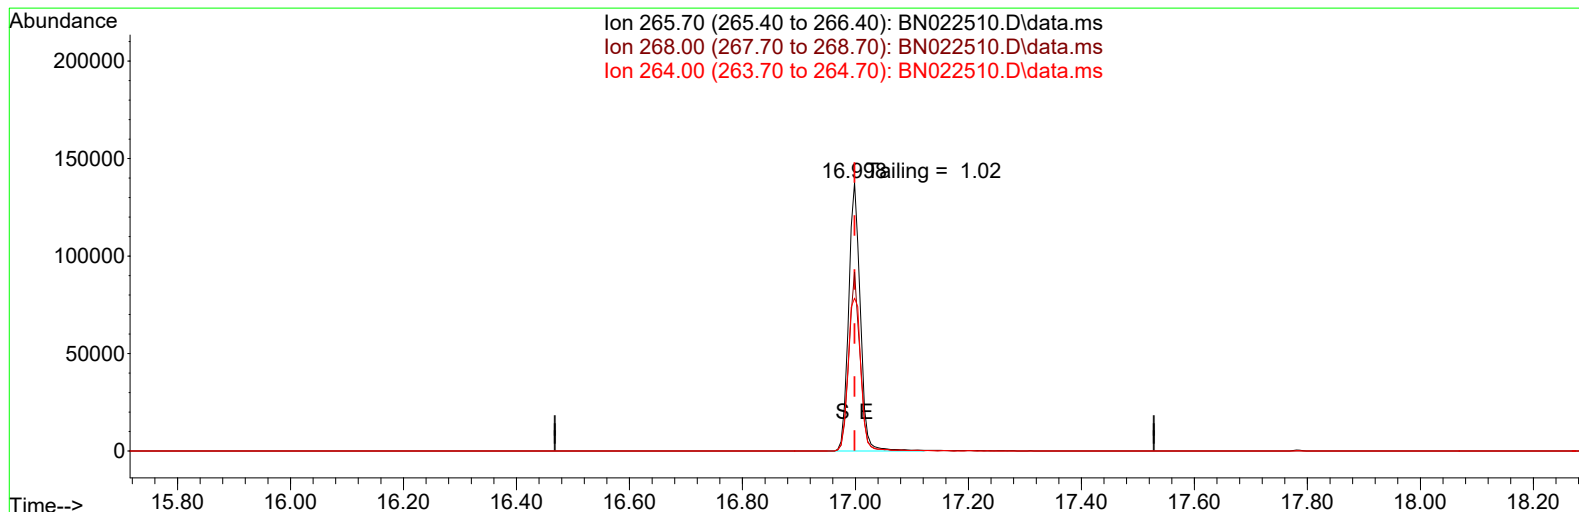

TIC: BN022510.D\data.ms

(70) Pentachlorophenol (C)




16.998min (0.000) 20796.05 ng

response 196985

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.59
264.00	61.60	56.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN110422\
Data File : BN022510.D
Acq On : 04 Nov 2022 15:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 05 04:35:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 05 04:35:21 2022
Response via : Initial Calibration

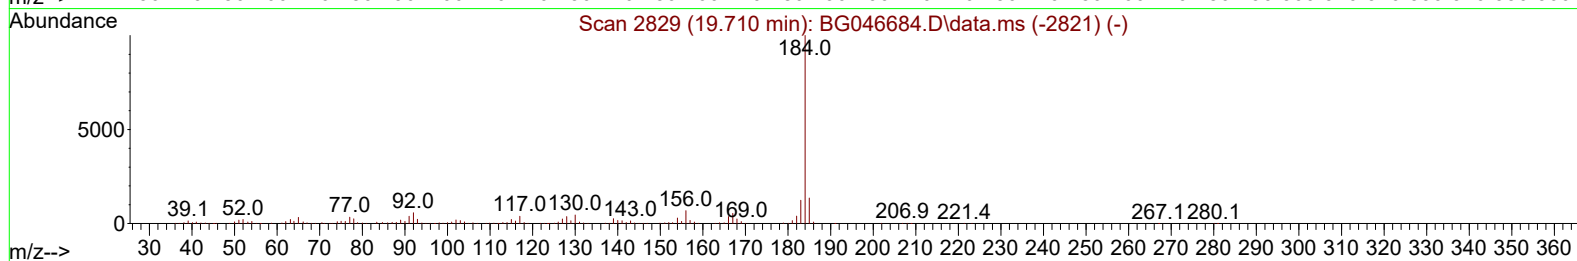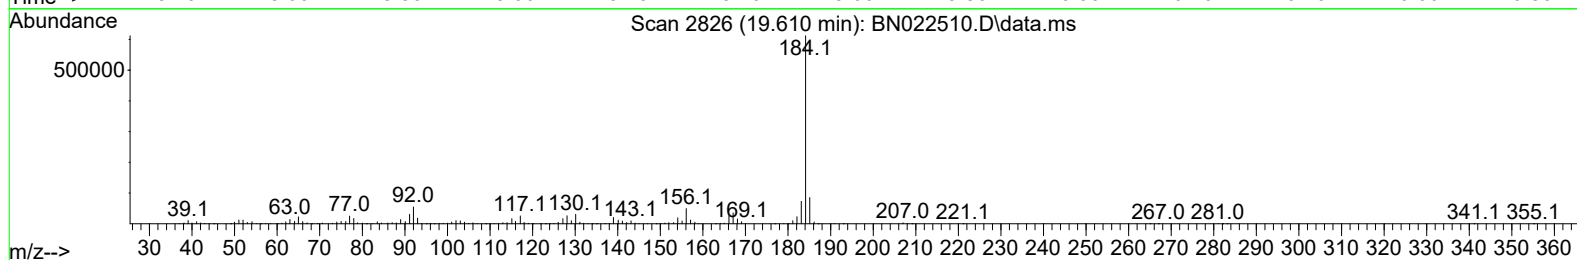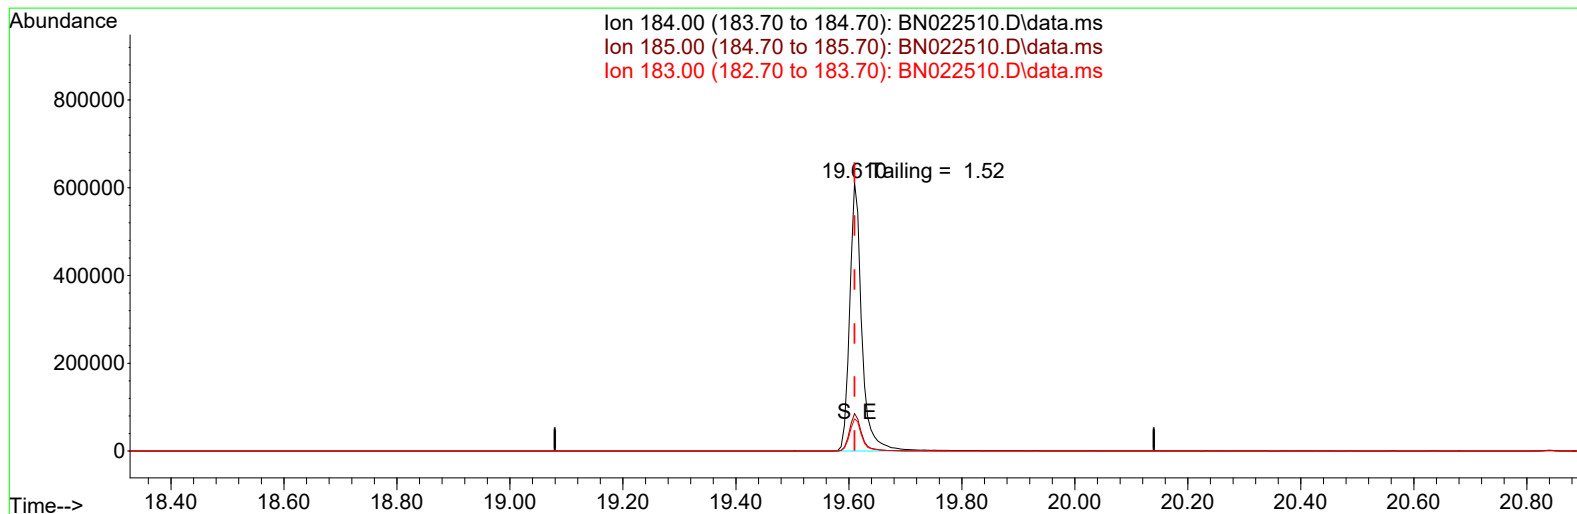

TIC: BN022510.D\data.ms

(77) Benzidine

19.610min (0.000) 0.00 ng

response 916998

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	11.97
0.00	0.00	0.00